

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081720\

Data File : VW016206.D

Acq On : 17 Aug 2020 10:19

Operator : SY/VA

Sample : VW0817SBL01

Misc : 5.00G/10ML/MSVOA W/SOIL

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 18 03:28:16 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M

Quant Title : VOC Analysis

QLast Update : Tue Aug 18 03:20:41 2020

Response via : Initial Calibration

Instrument :

MSVOA_W

Client Sampled :


VBLK03

Manual Integrations

APPROVED

MMDadoda

8/19/2020 5:25:11 PM

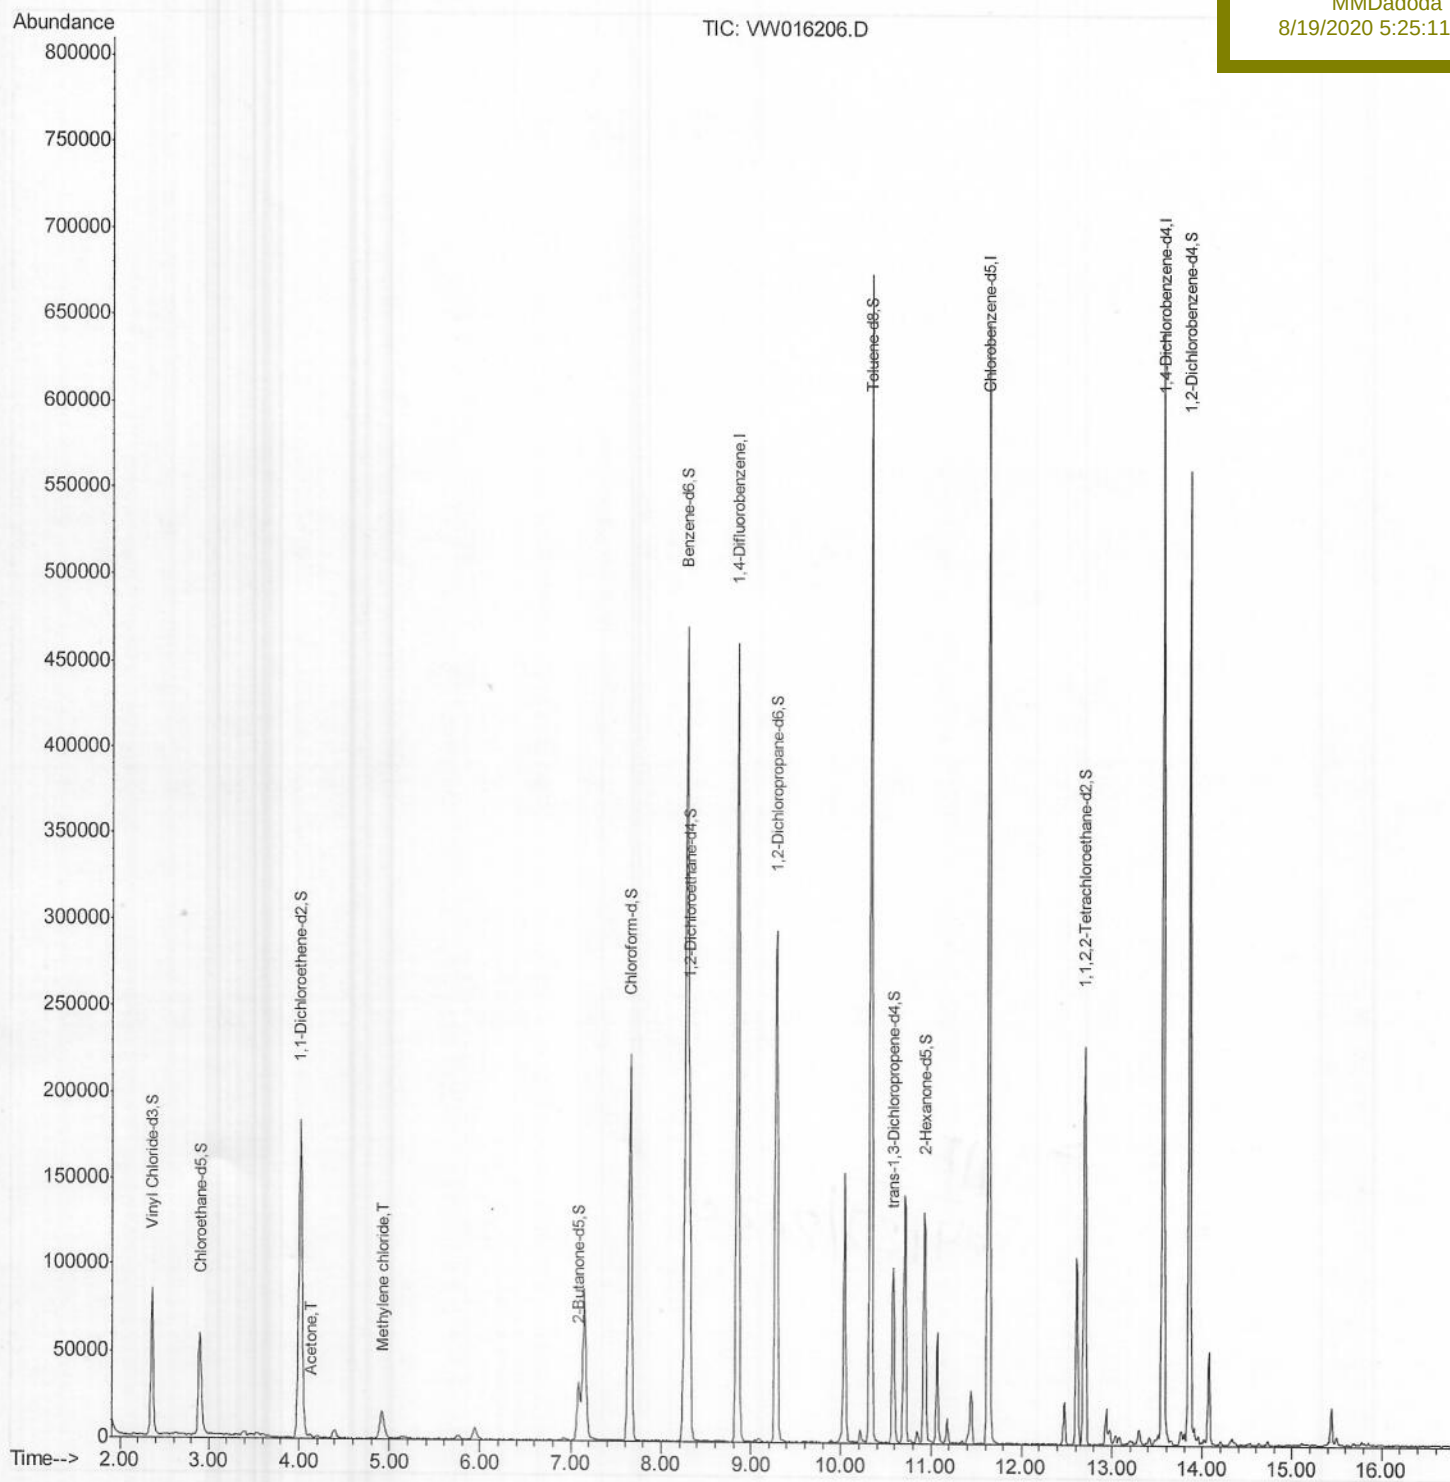

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081720\
 Data File : VW016206.D
 Acq On : 17 Aug 2020 10:19
 Operator : SY/VA
 Sample : VW0817SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 VBLK03

Quant Time: Aug 18 03:28:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 18 03:20:41 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/19/2020 5:25:11 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	399877	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	377203	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	167969	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	99218	20.01	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.04%
7) Chloroethane-d5	2.90	69	81639	21.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.76%
10) 1,1-Dichloroethene-d2	4.01	63	177995	16.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.60%
20) 2-Butanone-d5	7.08	46	58014	44.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.94%
24) Chloroform-d	7.65	84	238642	22.24	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.96%
26) 1,2-Dichloroethane-d4	8.31	65	122666	21.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.08%
29) Benzene-d6	8.28	84	484386	23.61	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.44%
33) 1,2-Dichloropropane-d6	9.28	67	140629	23.31	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.24%
37) Toluene-d8	10.33	98	447085	23.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.04%
38) trans-1,3-Dichloropropene-	10.58	79	59101	21.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.16%
39) 2-Hexanone-d5	10.93	63	46899	45.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.10%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	114153	23.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	152550	25.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.48%

Target Compounds

Target Compounds				Ovalue
13) Acetone	4.12	43	2555	2.589 ug/L
16) Methylene chloride	4.91	84	13374m	2.118 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> MD
 08/19/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081720\

Data File : VW016206.D

Acq On : 17 Aug 2020 10:19

Operator : SY/VA

Sample : VW0817SBL01

Misc : 5.00G/10ML/MSVOA W/SOIL

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 18 03:22:03 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M

Quant Title : VOC Analysis

QLast Update : Tue Aug 18 03:20:41 2020

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :




VBLK03

Manual Integrations

APPROVED

MMDadoda

8/19/2020 5:25:11 PM

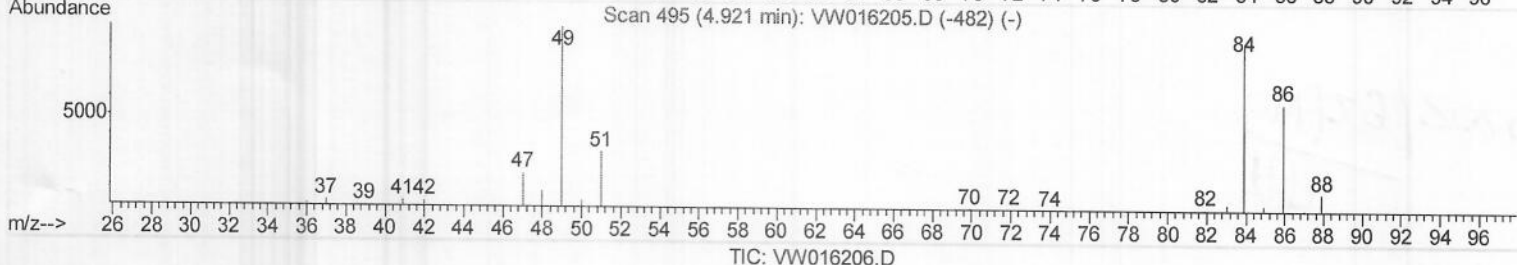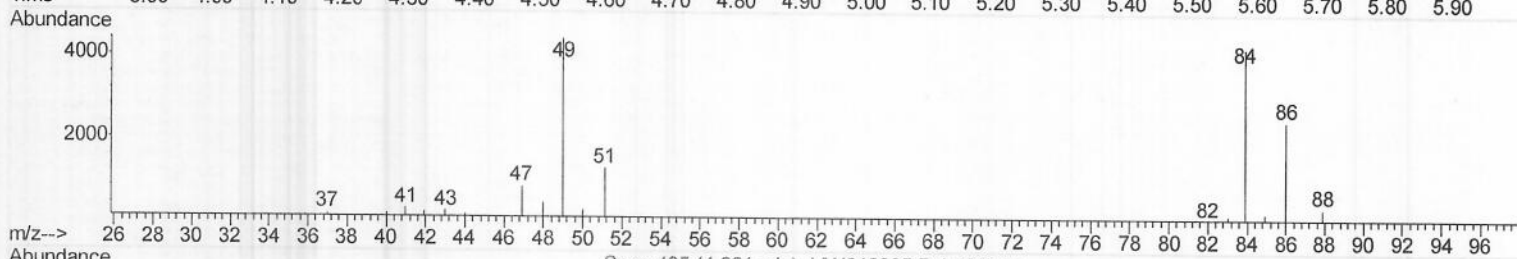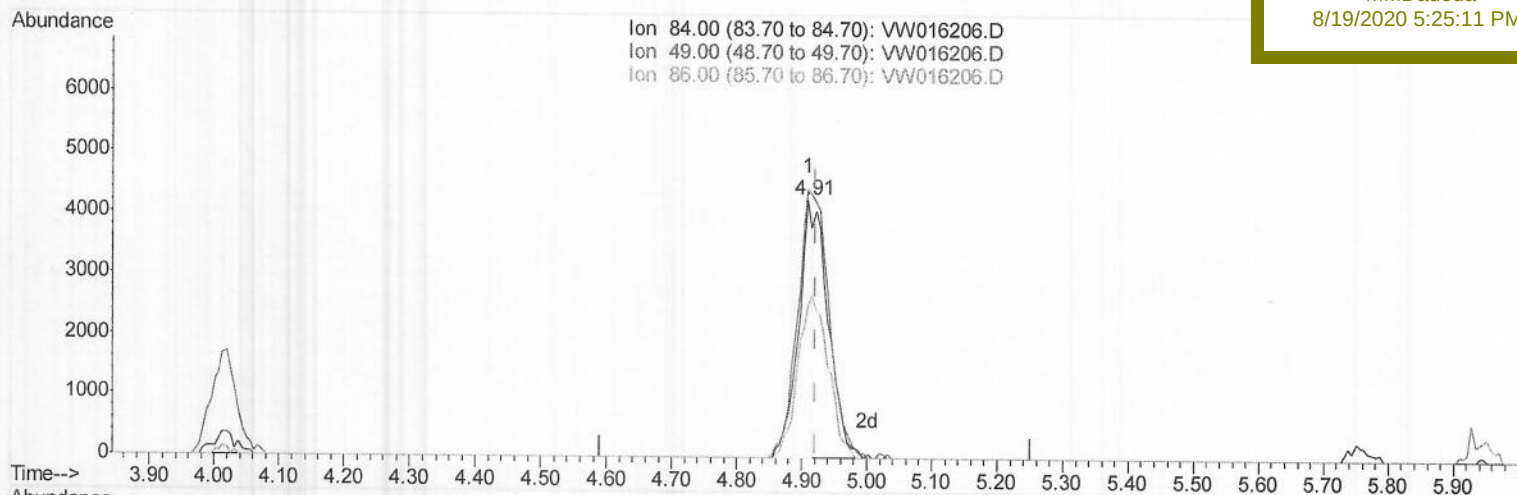

(16) Methylene chloride (T)

4.909min (-0.012) 1.05ug/L

response 6654

Ion	Exp%	Act%
84.00	100	100
49.00	114.90	104.05
86.00	62.50	58.61
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081720\

Data File : VW016206.D

Acq On : 17 Aug 2020 10:19

Operator : SY/VA

Sample : VW0817SBL01

Misc : 5.00G/10ML/MSVOA W/SOIL

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 18 03:22:03 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M

Quant Title : VOC Analysis

QLast Update : Tue Aug 18 03:20:41 2020




Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :

VBLK03

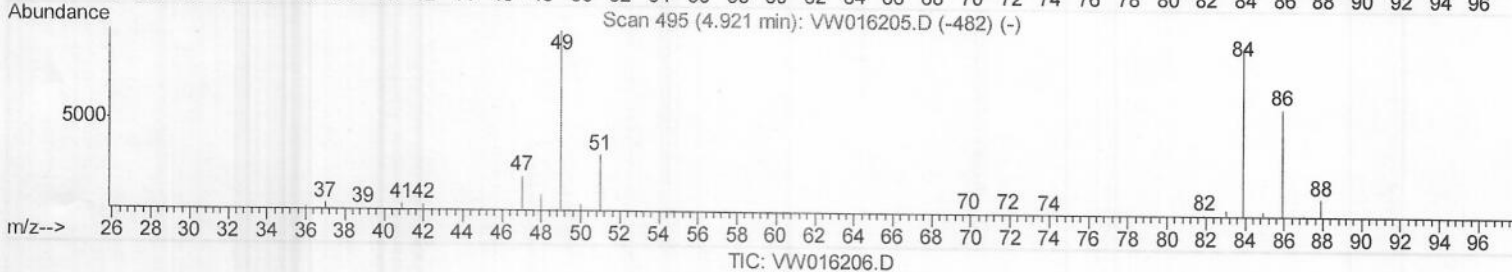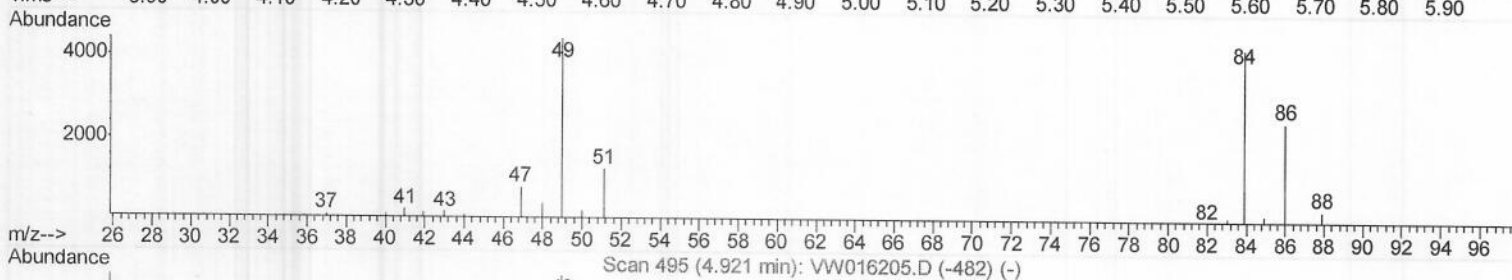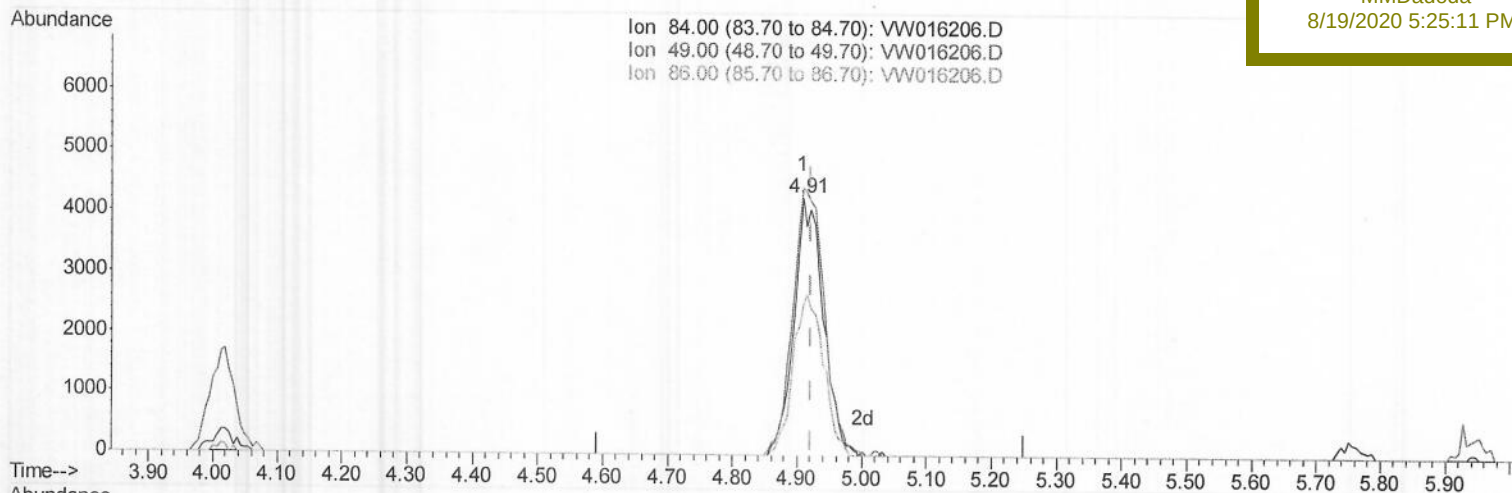Manual Integrations
APPROVEDMMDadoda
8/19/2020 5:25:11 PM

(16) Methylene chloride (T)

4.909min (-0.012) 2.12ug/L m

response 13374

Ion	Exp%	Act%
84.00	100	100
49.00	114.90	104.05
86.00	62.50	58.61
0.00	0.00	0.00

MD
08/19/20