


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW081720\
 Data File : VW016204.D
 Acq On : 17 Aug 2020 08:47
 Operator : SY/VA
 Sample : BFB10
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB10

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Title : VOC Analysis
 Last Update : Tue Aug 18 03:20:41 2020

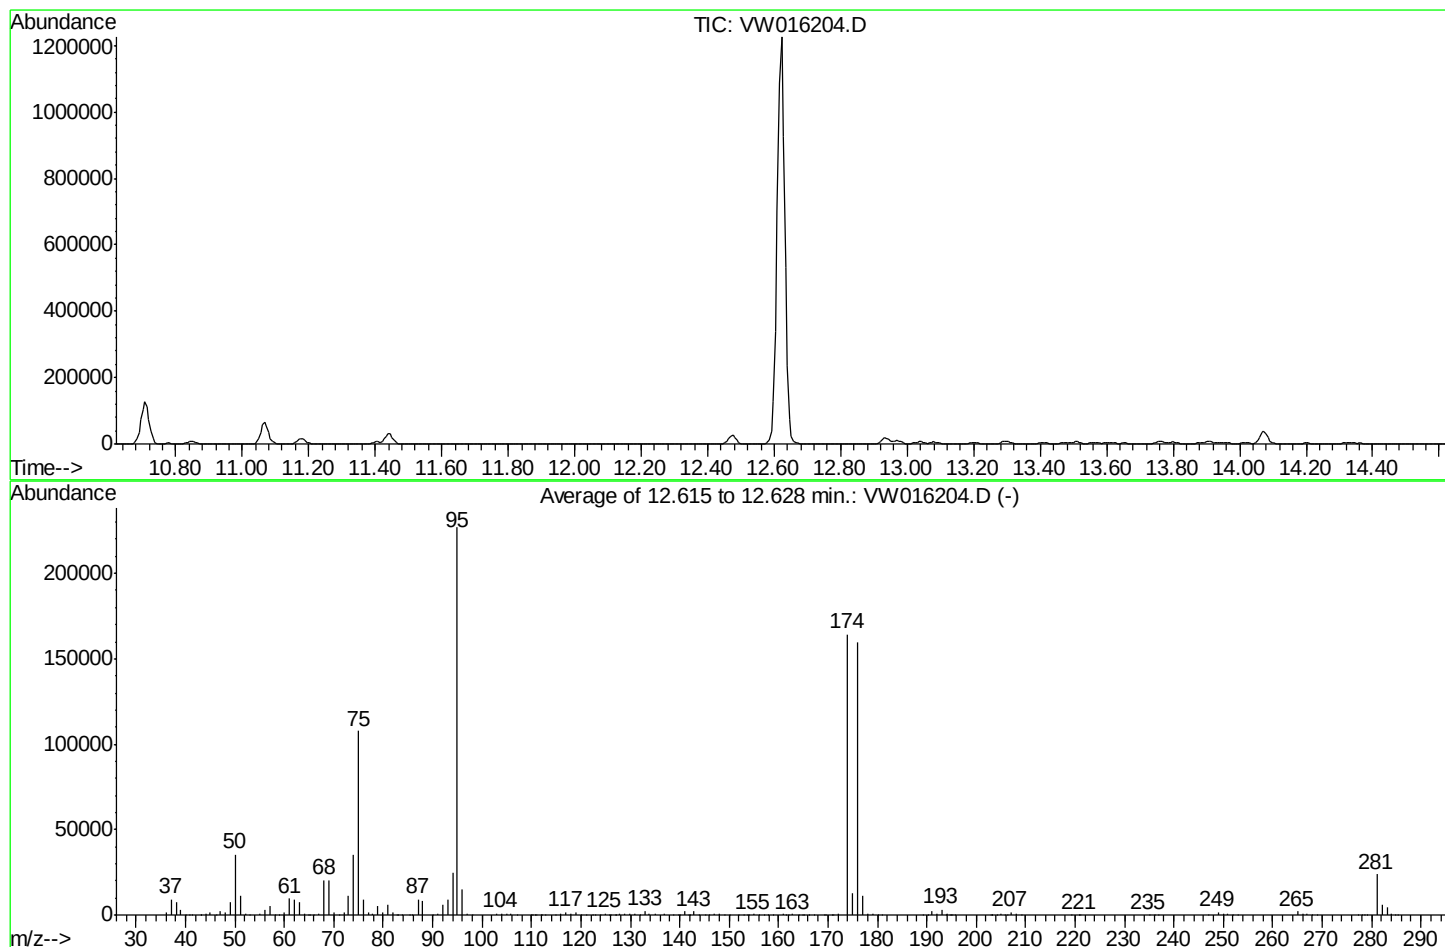

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	35402	PASS
75	95	30	80	47.5	107834	PASS
95	95	100	100	100.0	226944	PASS
96	95	5	9	6.6	14907	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	164224	PASS
175	174	5	9	7.9	13011	PASS
176	174	95	101	97.3	159808	PASS
177	176	5	9	7.2	11464	PASS

m/z	Abundance
36.00	1644.0
37.10	9440.0
38.00	8102.0
39.00	3182.0
40.10	191.0
40.90	58.0
41.30	59.0
43.00	285.0
44.10	1052.0
45.00	2005.0
46.10	124.0
47.10	2618.0
48.00	1205.0
49.00	7924.0
50.00	37136.0
51.10	11585.0
52.00	470.0
53.10	68.0
55.00	497.0
56.00	2967.0
57.00	5286.0
58.10	208.0
59.10	524.0
60.00	1803.0
61.00	10212.0
62.00	9512.0
63.10	7530.0
64.00	677.0
65.10	693.0
67.00	681.0
68.00	20840.0
69.00	21160.0
70.00	1657.0
71.00	143.0
72.00	1195.0
73.00	12302.0
74.00	34624.0
75.00	110968.0
76.00	9585.0
77.00	1087.0
77.90	878.0
78.90	5805.0
79.90	1672.0
80.90	6201.0
81.90	1362.0
82.80	212.0
83.70	120.0
85.20	59.0
85.90	438.0
87.00	9093.0
88.00	8416.0
90.10	60.0
91.00	817.0
92.00	5680.0
93.00	9620.0
94.00	24680.0
95.00	226816.0
96.00	15481.0
97.00	444.0
97.90	51.0
103.00	923.0
103.90	1063.0
104.90	635.0
105.90	898.0
107.00	199.0
110.00	323.0
111.10	475.0
111.90	354.0
112.90	248.0
114.90	426.0
116.00	709.0
117.00	1636.0
118.10	1054.0
118.90	1407.0
120.00	186.0
120.90	267.0
122.40	53.0
123.00	67.0
123.90	262.0
124.90	1671.0
125.70	481.0
126.90	105.0
127.90	700.0
128.90	351.0
129.90	675.0
131.00	413.0
132.00	288.0
133.10	3658.0
133.80	1125.0
135.00	796.0
136.90	491.0
139.80	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

140.00	130.0
141.00	1849.0
141.80	186.0
143.00	2106.0
144.00	155.0
145.00	385.0
146.00	334.0
147.10	757.0
147.90	551.0
148.90	344.0
150.00	215.0
152.00	129.0
152.90	160.0
153.70	83.0
154.90	609.0
156.90	390.0
158.90	316.0
160.90	572.0
161.50	82.0
162.90	738.0
164.10	249.0
164.90	487.0
167.10	92.0
169.50	52.0
171.00	194.0
172.00	1020.0
174.00	151040.0
175.00	12155.0
176.00	143296.0
177.00	10954.0
178.00	595.0
179.00	969.0
180.00	292.0
180.80	99.0
189.10	402.0
190.20	194.0
191.00	3173.0
192.00	762.0
193.00	4325.0
194.10	950.0
194.90	577.0
202.90	433.0
204.20	119.0
205.10	818.0
205.90	222.0
207.00	2019.0
208.10	512.0
209.00	344.0
219.10	70.0
221.00	141.0
235.00	470.0
236.90	126.0
246.90	89.0
249.10	2293.0
250.00	608.0
251.00	1300.0
252.00	215.0
253.00	196.0
265.00	2822.0
266.10	1128.0
267.00	704.0
268.00	160.0
269.00	78.0
277.30	63.0
278.20	101.0
279.10	356.0
281.00	33808.0
282.10	8952.0
283.10	5991.0
284.00	1061.0
284.90	251.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

m/z	Abundance
36.00	2022.0
37.00	10110.0
38.00	8707.0
39.00	3564.0
40.00	340.0
40.80	82.0
42.90	87.0
43.20	105.0
44.00	1278.0
45.00	1849.0
46.10	244.0
47.00	2682.0
48.00	1294.0
49.00	8793.0
50.00	40200.0
51.00	13186.0
52.10	447.0
52.90	99.0
55.00	556.0
56.00	3249.0
57.00	6158.0
58.00	311.0
58.90	401.0
60.00	2143.0
61.00	10314.0
62.00	10510.0
63.00	7902.0
64.10	829.0
64.80	479.0
65.90	60.0
67.10	620.0
68.00	22864.0
69.00	23688.0
70.10	1581.0
71.10	169.0
72.00	1444.0
73.00	13111.0
74.00	40424.0
75.00	120096.0
76.00	10418.0
77.00	1552.0
77.90	1039.0
78.90	6175.0
80.00	1655.0
81.00	5929.0
81.90	1236.0
83.20	208.0
83.70	119.0
85.90	380.0
87.00	11107.0
88.00	9593.0
90.10	72.0
90.80	816.0
92.00	6892.0
93.00	10089.0
94.00	28808.0
95.00	258688.0
96.00	16712.0
97.10	426.0
102.90	636.0
103.90	1105.0
104.90	491.0
105.90	987.0
106.90	343.0
109.80	327.0
111.00	502.0
112.10	336.0
112.90	250.0
114.80	397.0
115.90	895.0
117.00	1737.0
117.90	1060.0
119.00	1690.0
119.90	116.0
121.00	147.0
124.00	171.0
125.00	754.0
126.00	356.0
126.90	140.0
127.80	859.0
128.90	465.0
130.00	906.0
130.90	436.0
132.00	208.0
133.10	3021.0
134.90	594.0
136.90	414.0
138.60	57.0
140.00	216.0
140.90	2256.0
142.00	238.0
142.90	2428.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

144.00	125.0
145.00	336.0
146.00	288.0
147.00	556.0
147.90	665.0
149.00	306.0
149.80	202.0
152.00	194.0
153.00	235.0
154.00	66.0
155.00	573.0
156.10	114.0
157.00	513.0
157.80	58.0
158.90	308.0
160.80	376.0
162.80	400.0
164.90	375.0
166.10	56.0
169.20	50.0
172.00	1227.0
174.00	188864.0
175.00	14500.0
176.00	185024.0
177.00	12766.0
178.00	499.0
179.10	824.0
179.90	96.0
189.10	343.0
191.00	2127.0
192.00	670.0
193.00	3349.0
193.90	512.0
194.60	182.0
195.10	340.0
195.70	69.0
202.80	201.0
203.10	179.0
205.10	804.0
206.40	317.0
207.10	1694.0
208.10	445.0
209.10	276.0
219.20	59.0
220.70	82.0
221.10	85.0
234.90	312.0
236.10	90.0
248.90	1844.0
249.90	488.0
250.90	707.0
252.00	153.0
252.90	153.0
265.10	1996.0
266.10	793.0
266.90	455.0
268.00	81.0
278.10	104.0
278.50	110.0
281.10	27136.0
282.10	6420.0
283.10	4519.0
284.10	973.0
285.20	230.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

m/z	Abundance
36.00	1312.0
37.10	7485.0
38.10	6200.0
39.00	2462.0
40.00	344.0
40.90	75.0
43.00	158.0
44.00	938.0
45.00	1323.0
46.10	166.0
47.00	2020.0
48.00	1079.0
49.00	6695.0
50.00	28872.0
51.00	9002.0
52.00	372.0
52.90	60.0
55.10	388.0
56.10	2411.0
57.00	4118.0
58.00	159.0
59.00	230.0
60.10	1504.0
61.10	8074.0
62.00	7541.0
63.10	6049.0
64.00	507.0
65.10	433.0
65.90	52.0
67.10	513.0
68.00	18064.0
69.00	16584.0
70.00	1518.0
71.00	148.0
72.00	1023.0
73.00	9348.0
74.00	30448.0
75.00	92440.0
76.10	7737.0
76.90	1101.0
77.90	801.0
79.00	4698.0
80.00	1476.0
80.90	4968.0
82.00	1067.0
83.00	149.0
86.00	190.0
87.00	7628.0
87.90	7444.0
90.90	643.0
92.00	5535.0
93.00	7961.0
94.00	21488.0
95.00	195328.0
96.00	12528.0
97.00	430.0
102.90	272.0
104.00	903.0
104.90	341.0
105.90	739.0
107.10	164.0
110.10	175.0
110.80	315.0
112.00	161.0
113.00	114.0
115.00	293.0
115.90	593.0
117.00	1228.0
117.90	805.0
118.90	1138.0
124.00	107.0
124.90	470.0
126.10	120.0
127.10	59.0
127.90	642.0
129.00	406.0
129.90	659.0
131.00	398.0
131.90	93.0
133.10	1052.0
133.90	246.0
135.00	442.0
137.00	324.0
140.00	113.0
141.00	1999.0
141.90	282.0
143.00	2024.0
143.80	118.0
145.10	257.0
146.00	294.0
146.90	283.0
147.90	593.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

149.00	103.0
150.00	240.0
151.90	91.0
152.90	129.0
154.10	68.0
154.90	483.0
156.90	296.0
158.90	215.0
160.90	445.0
161.90	55.0
162.80	254.0
164.80	140.0
165.20	161.0
169.10	81.0
169.60	74.0
170.70	125.0
172.00	804.0
174.00	152768.0
175.00	12378.0
176.00	151104.0
177.00	10674.0
177.90	310.0
178.90	324.0
179.90	63.0
189.10	135.0
191.00	1258.0
191.90	230.0
193.00	1758.0
193.80	214.0
195.00	194.0
203.30	74.0
205.10	422.0
206.20	88.0
207.10	1039.0
208.20	293.0
209.10	105.0
220.90	67.0
234.90	93.0
249.00	1005.0
250.10	175.0
251.10	366.0
252.10	76.0
253.00	94.0
265.10	1070.0
265.90	243.0
267.00	294.0
267.90	58.0
279.00	92.0
281.10	11000.0
282.10	3000.0
283.10	2197.0
284.10	508.0
284.90	151.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

Scan 1749 (12.567 min): VW016204.D
BFB10

m/z	Abundance
39.80	218.0
43.90	190.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10