

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081722\
 Data File : VW024267.D
 Acq On : 17 Aug 2022 12:05
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK535

Quant Time: Aug 18 01:05:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 18 01:04:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	263184	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	258865	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	127832	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	109876	19.973	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.880%
7) Chloroethane-d5	2.873	69	70750	20.645	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.600%
11) 1,1-Dichloroethene-d2	4.013	63	97414	15.538	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.160%
21) 2-Butanone-d5	7.080	46	49980	48.834	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.660%
24) Chloroform-d	7.646	84	168967	21.218	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.880%
26) 1,2-Dichloroethane-d4	8.305	65	97869	22.136	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.560%
32) Benzene-d6	8.268	84	313534	20.537	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.160%
36) 1,2-Dichloropropane-d6	9.268	67	96848	21.486	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.960%
41) Toluene-d8	10.323	98	285842	20.031	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.120%
43) trans-1,3-Dichloroprop...	10.579	79	41313	20.925	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.680%
47) 2-Hexanone-d5	10.920	63	36768	44.161	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.320%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	94179	21.535	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	106204	22.703	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.800%
Target Compounds					Qvalue	
13) Acetone	4.129	43	2813	3.733	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081722\
Data File : VW024267.D
Acq On : 17 Aug 2022 12:05
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK535

Quant Time: Aug 18 01:05:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 18 01:04:13 2022
Response via : Initial Calibration

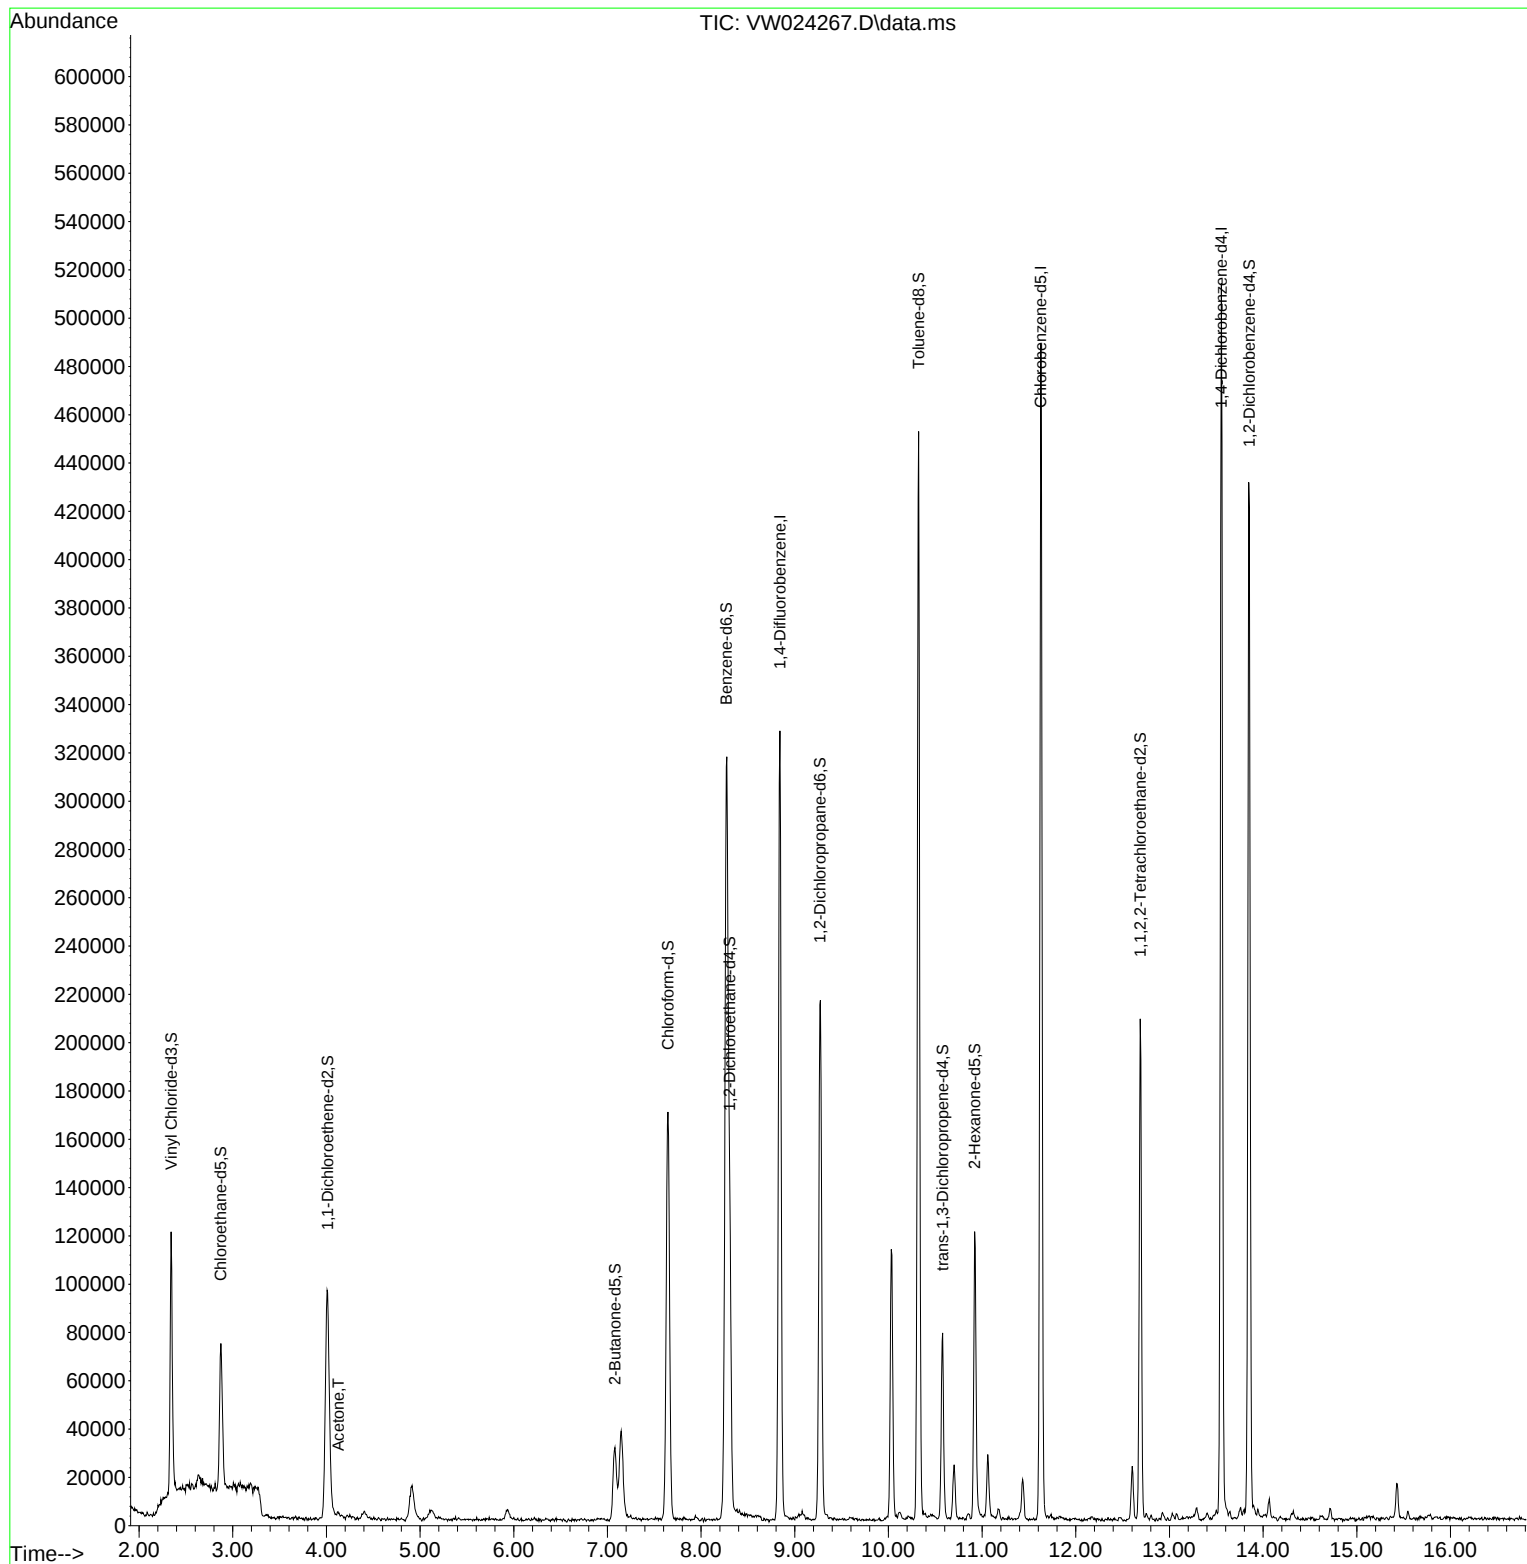

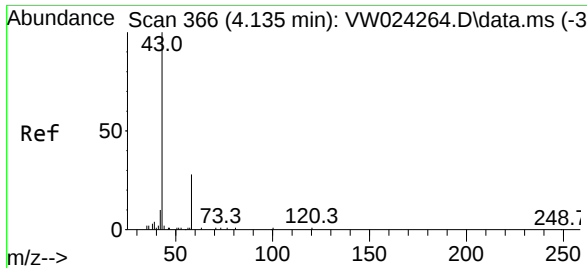

#13
 Acetone
 Concen: 3.733 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW024267.D
 Acq: 17 Aug 2022 12:05

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK535

Tgt Ion: 43 Resp: 2813
 Ion Ratio Lower Upper
 43 100
 58 18.0 0.0 31.8

