

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081822\
Data File : VW024272.D
Acq On : 18 Aug 2022 13:15
Operator : SY/VA
Sample : VW0818SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
VBLK579

Manual IntegrationsAPPROVED

Quant Time: Aug 18 21:05:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 18 01:04:13 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

08/22/2022
Supervised By :Mahesh
Dadoda

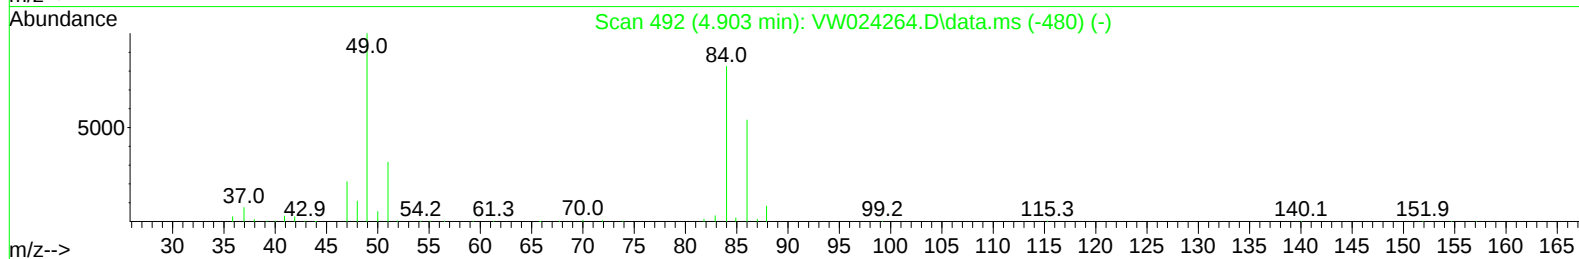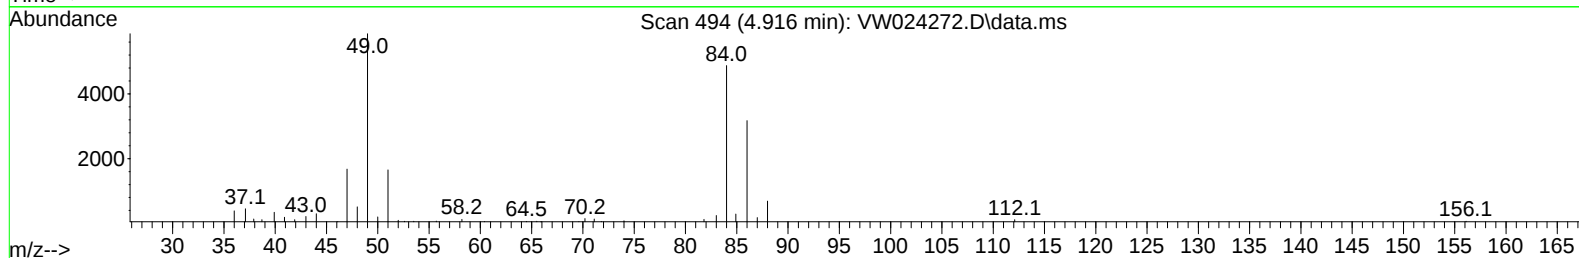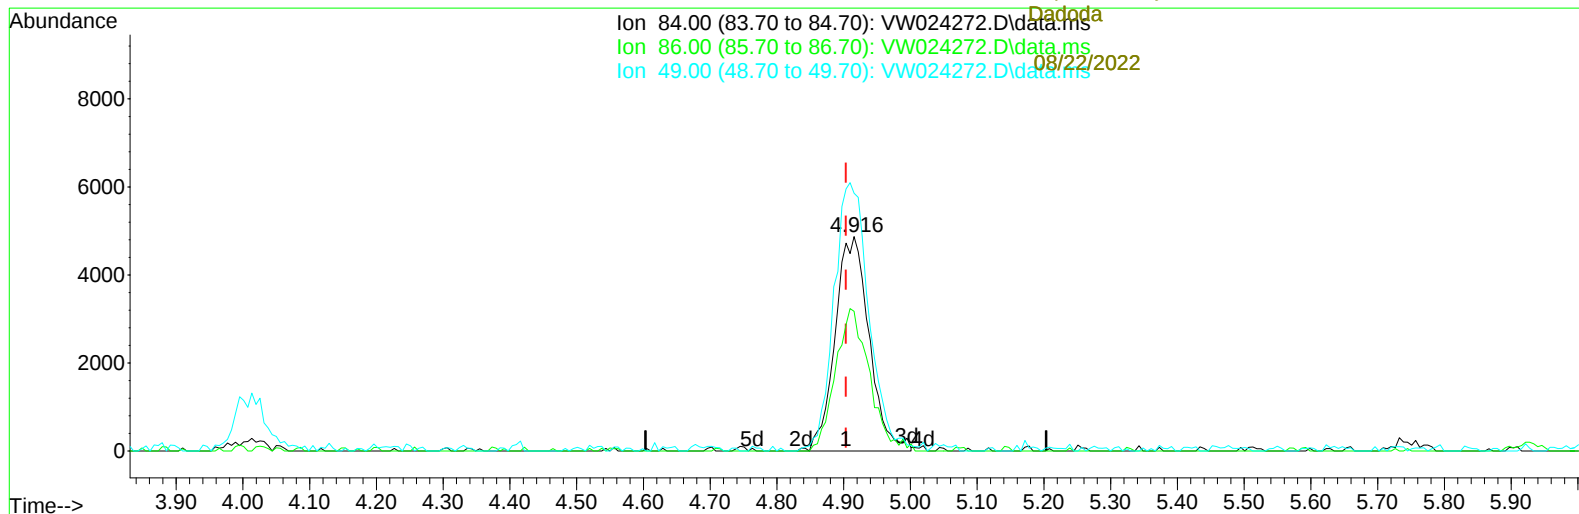

TIC: VW024272.D\data.ms

(16) Methylene chloride (T)

4.916min (+ 0.012) 3.86 ug/L m

response 17294

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	65.13
49.00	121.80	120.21
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081822\
Data File : VW024272.D
Acq On : 18 Aug 2022 13:15
Operator : SY/VA
Sample : VW0818SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
VBLK579

Manual IntegrationsAPPROVED

Quant Time: Aug 18 21:05:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 18 01:04:13 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

08/22/2022
Supervised By :Mahesh
Dadoda

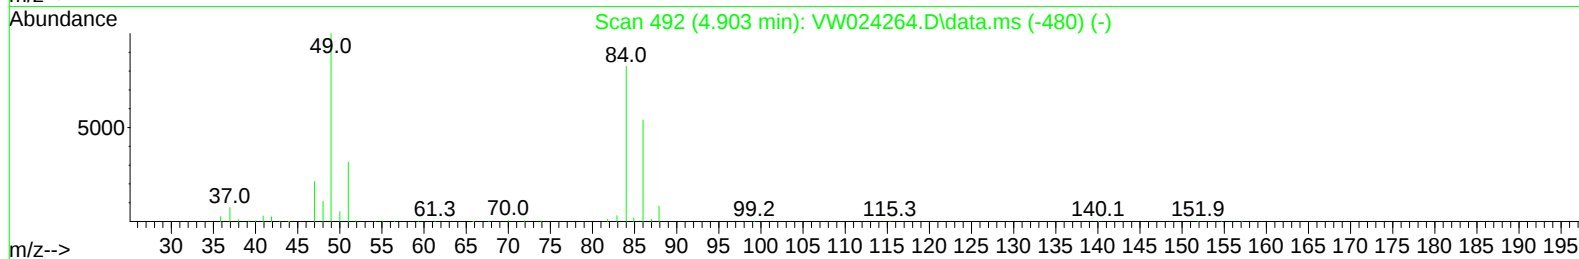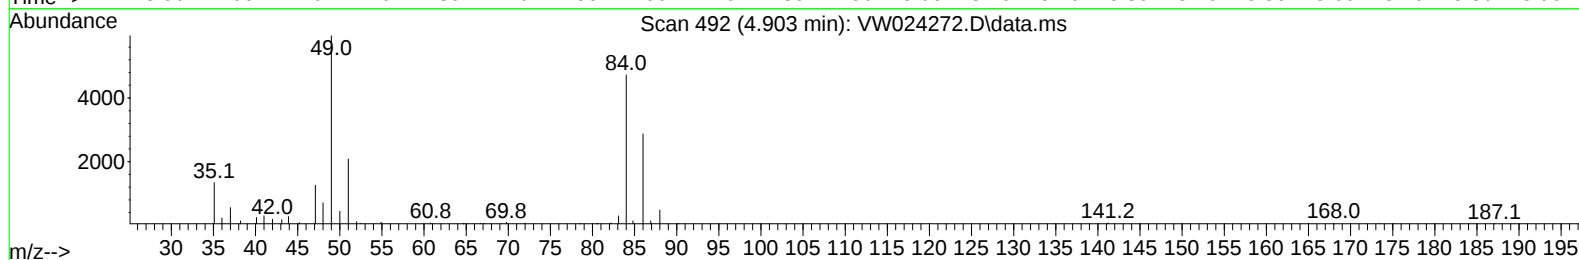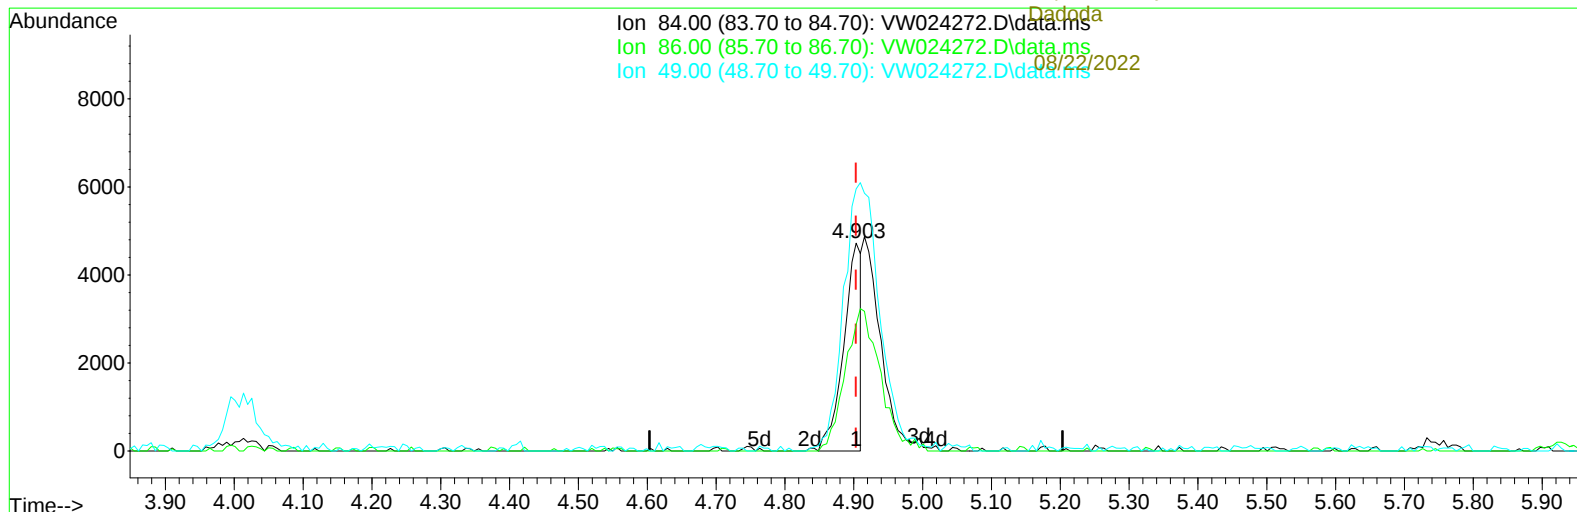

TIC: VW024272.D\data.ms

(16) Methylene chloride (T)

4.903min (+ 0.000) 1.88 ug/L

response 8404

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	60.82
49.00	121.80	126.06
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081822\
 Data File : VW024272.D
 Acq On : 18 Aug 2022 13:15
 Operator : SY/VA
 Sample : VW0818SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK579

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

08/22/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Aug 18 21:05:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 18 01:04:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	254043	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	246931	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	121253	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	108667	20.464	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.840%
7) Chloroethane-d5	2.873	69	72601	21.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	4.007	63	93866	15.511	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.040%
21) 2-Butanone-d5	7.080	46	50326	50.941	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.880%
24) Chloroform-d	7.647	84	173251	22.539	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.160%
26) 1,2-Dichloroethane-d4	8.305	65	99892	23.407	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.640%
32) Benzene-d6	8.269	84	320341	21.997	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.000%
36) 1,2-Dichloropropane-d6	9.275	67	96938	22.545	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.160%
41) Toluene-d8	10.323	98	286488	21.047	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	10.579	79	40530	21.520	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.080%
47) 2-Hexanone-d5	10.921	63	36380	45.807	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.620%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	95664	22.932	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.720%
66) 1,2-Dichlorobenzene-d4	13.847	152	109900	24.768	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.080%
Target Compounds						
16) Methylene chloride	4.916	84	17294m	3.860	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081822\
Data File : VW024272.D
Acq On : 18 Aug 2022 13:15
Operator : SY/VA
Sample : VW0818SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK579

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

08/22/2022
Supervised By :Mahesh
Dadoda

08/22/2022

