

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081918\
 Data File : VW004752.D
 Acq On : 18 Aug 2018 00:04
 Operator : SY/AP
 Sample : J4460-03RE
 Misc : 5.01G/5ML/MSVOA W/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 RA-081018-SW-003RE

Quant Time: Aug 18 05:01:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 18 01:49:53 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	465914	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	672336	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	442428	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	101215	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	272898	60.58	ug/l	0.00
Spiked Amount 50.000			Recovery	=	121.16%	
35) Dibromofluoromethane	7.88	113	261841	60.93	ug/l	0.00
Spiked Amount 50.000			Recovery	=	121.86%	
50) Toluene-d8	10.33	98	681095	40.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	81.20%	
62) 4-Bromofluorobenzene	12.62	95	115768	19.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	38.36%	
Target Compounds						
20) Methylene Chloride	4.91	84	33843	2.33	ug/l	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081918\
Data File : VW004752.D
Acq On : 18 Aug 2018 00:04
Operator : SY/AP
Sample : J4460-03RE
Misc : 5.01G/5ML/MSVOA W/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
RA-081018-SW-003RE

Quant Time: Aug 18 05:01:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 18 01:49:53 2018
Response via : Initial Calibration

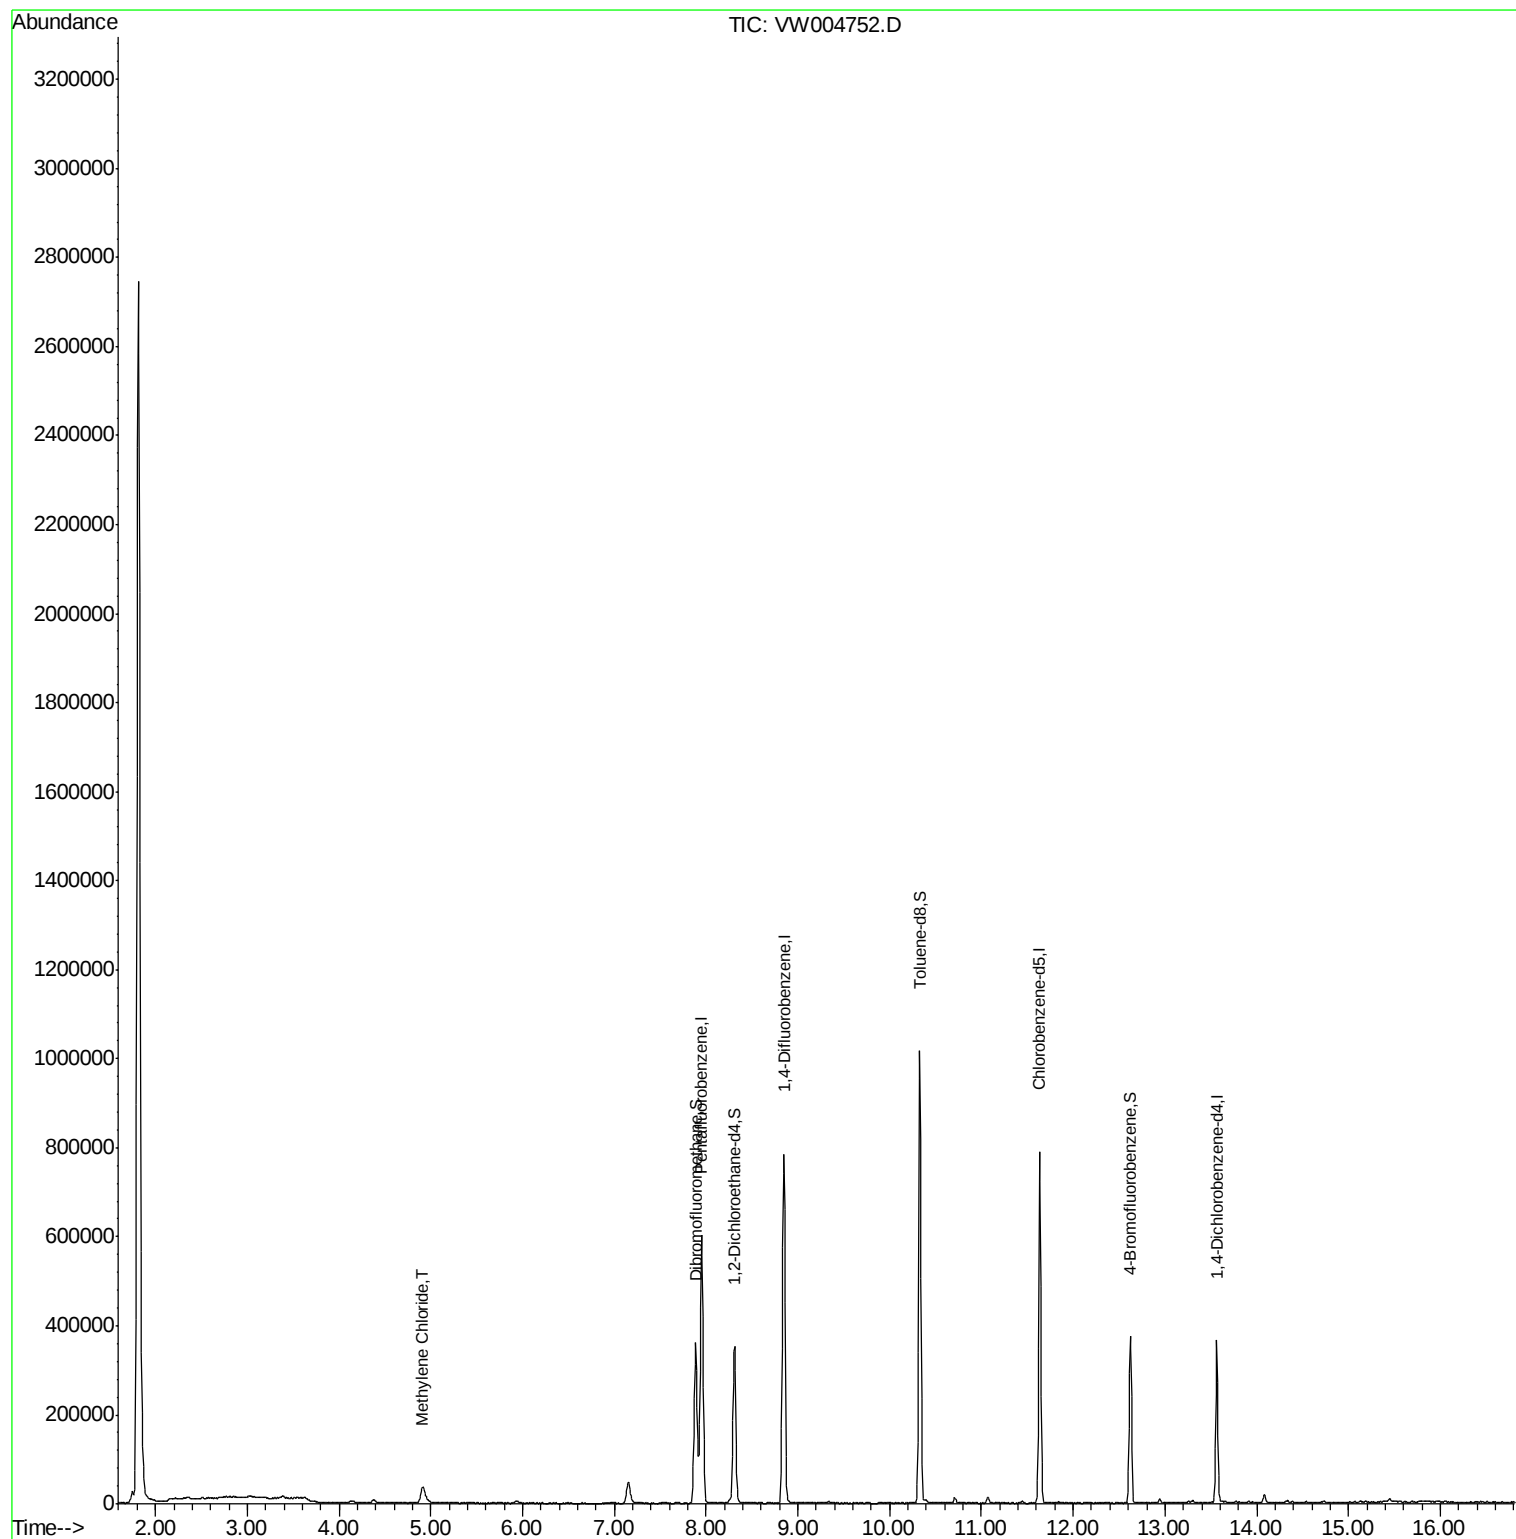

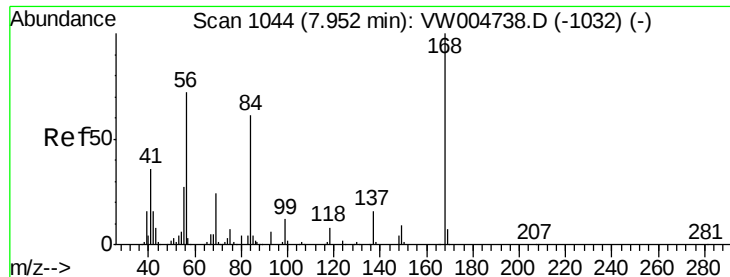

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1044

Delta R.T. -0.00 min

Lab File: VW004752.D

Acq: 18 Aug 2018 00:04

Instrument :

MSVOA_W

ClientSampleId :


RA-081018-SW-003RE

Tot Ion:168 Resp: 465914

Ion Ratio Lower Upper

168 100

99 53.1 41.0 61.4

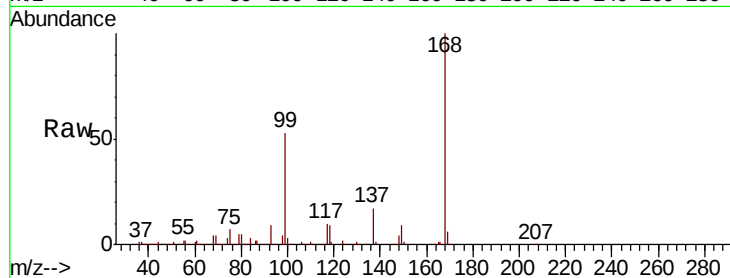

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

200000



150000

100000

50000

0

Time-->

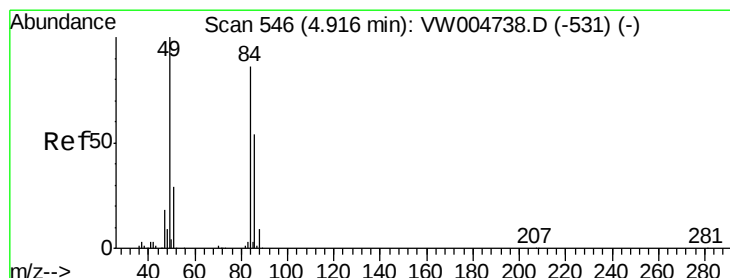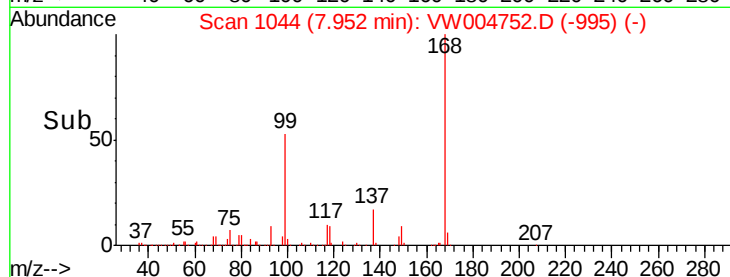

#20

Methylene Chloride

Concen: 2.33 ug/l

RT: 4.91 min Scan# 545

Delta R.T. -0.01 min

Lab File: VW004752.D

Acq: 18 Aug 2018 00:04

Tgt Ion: 84 Resp: 33843


Ion Ratio Lower Upper

84 100

49 128.4 93.2 139.8

51 40.5 27.4 41.0

86 64.2 50.6 75.8

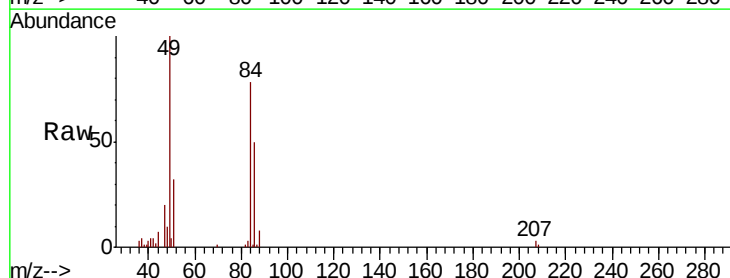

Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

4.91


15000


10000

5000

0

Time-->




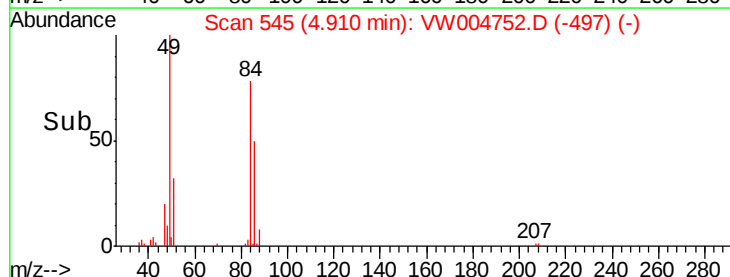


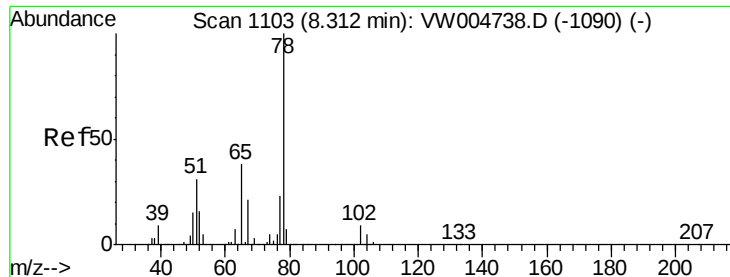

#33
 1,2-Dichloroethane-d4
 Concen: 60.58 ug/l
 RT: 8.31 min Scan# 1103
 Delta R.T. -0.00 min
 Lab File: VW004752.D
 Acq: 18 Aug 2018 00:04




Instrument :
 MSVOA_W
 ClientSampleId :
 RA-081018-SW-003RE


Tot Ion: 65 Resp: 272898
 Ion Ratio Lower Upper
 65 100
 67 53.8 0.0 109.4

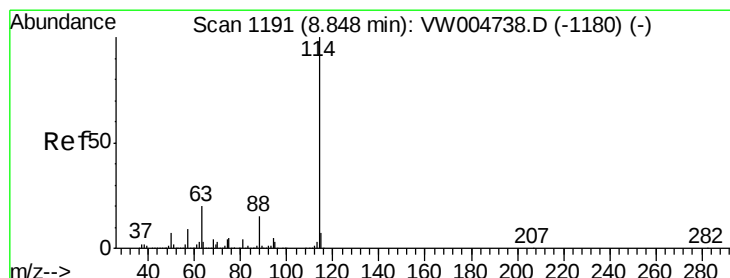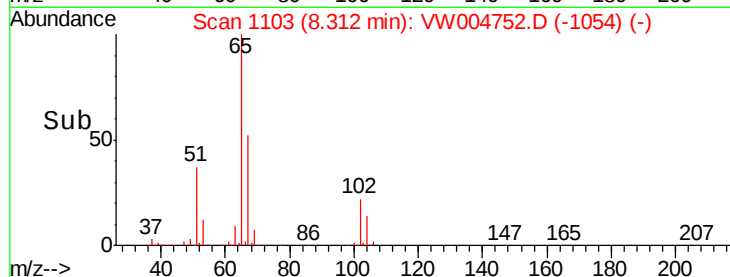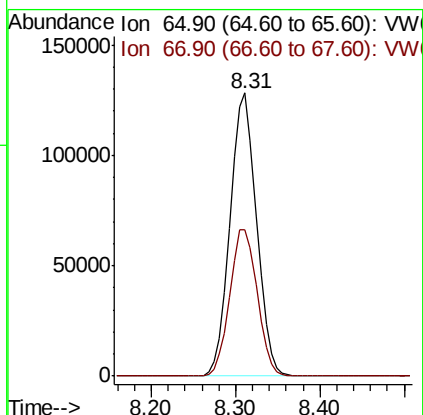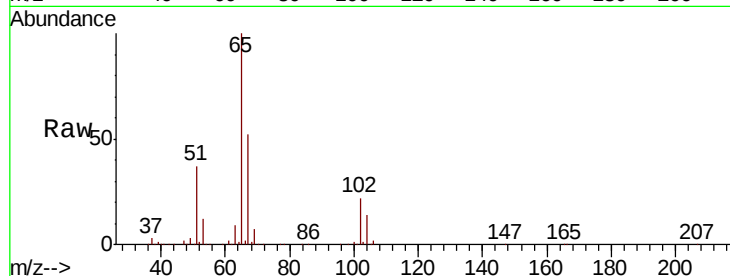

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: VW004752.D
 Acq: 18 Aug 2018 00:04

Tgt Ion: 114 Resp: 672336
 Ion Ratio Lower Upper
 114 100
 63 20.8 0.0 39.0
 88 15.8 0.0 30.0


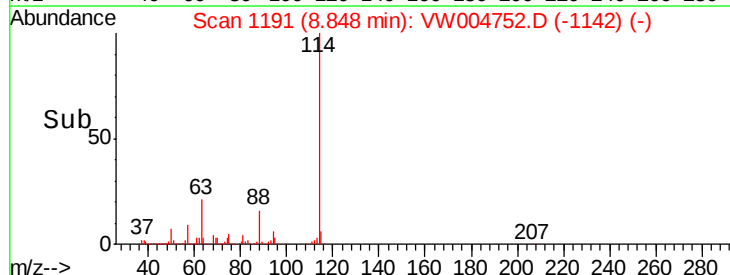
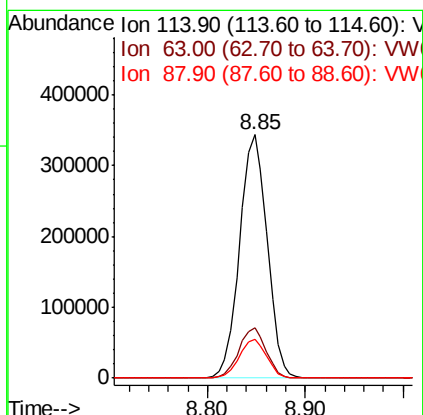
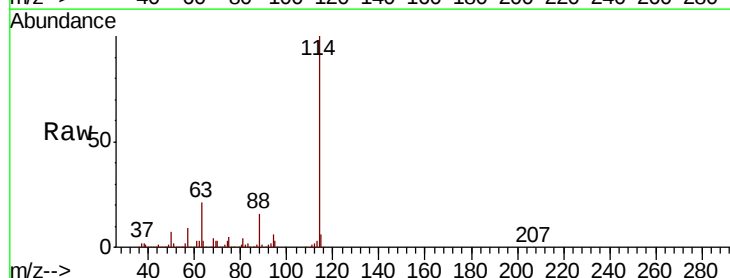


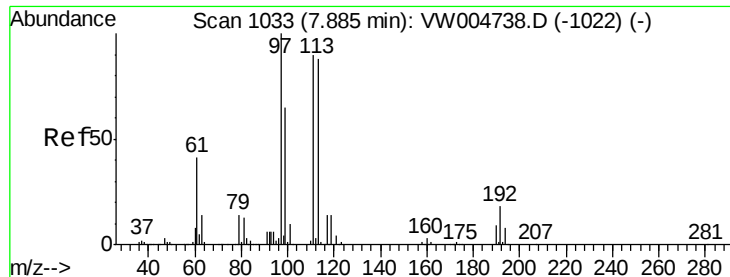

#35
 Dibromofluoromethane
 Concen: 60.93 ug/l
 RT: 7.88 min Scan# 1033
 Delta R.T. -0.00 min
 Lab File: VW004752.D
 Acq: 18 Aug 2018 00:04




Instrument :
 MSVOA_W
 ClientSampleId :
 RA-081018-SW-003RE


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.3	82.4	123.6
192	21.1	16.7	25.1

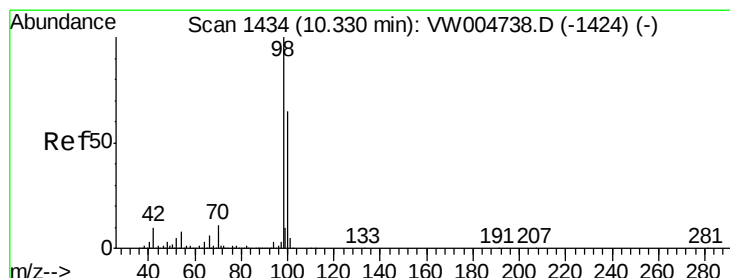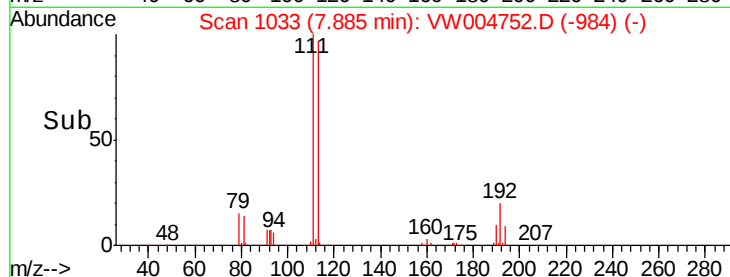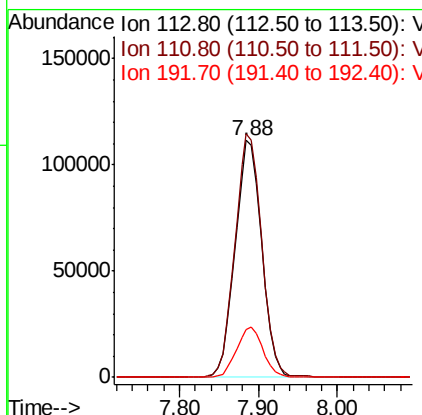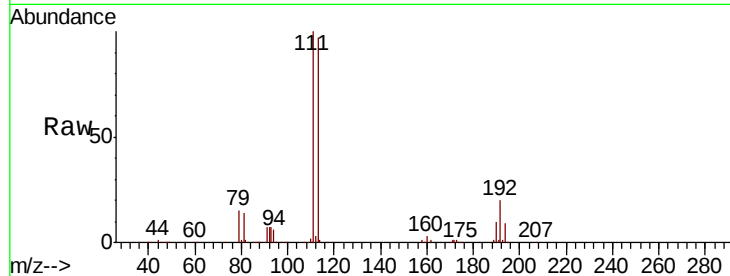

#50
 Toluene-d8
 Concen: 40.60 ug/l
 RT: 10.33 min Scan# 1434
 Delta R.T. -0.00 min
 Lab File: VW004752.D
 Acq: 18 Aug 2018 00:04

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.4	51.8	77.8


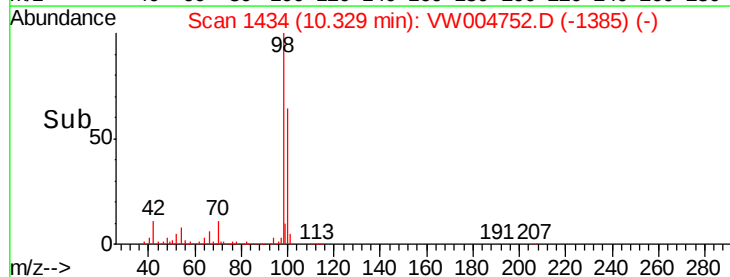
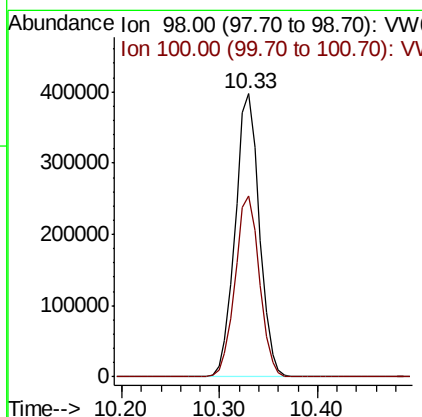
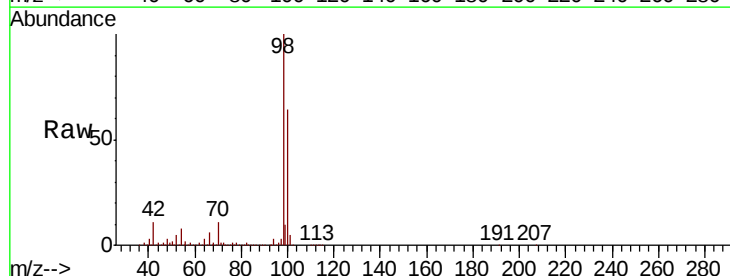


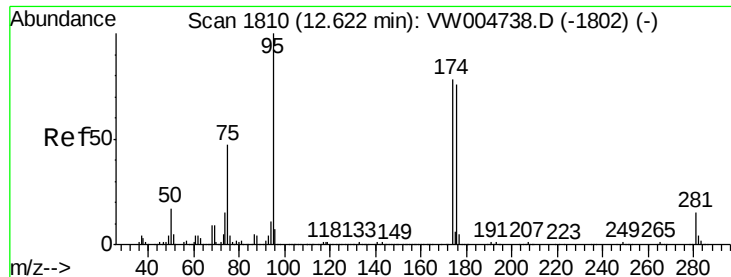

#62
4-Bromofluorobenzene
Concen: 19.18 ug/l
RT: 12.62 min Scan# 1810
Delta R.T. -0.00 min
Lab File: VW004752.D
Acq: 18 Aug 2018 00:04




Instrument :
MSVOA_W
ClientSampleId :
RA-081018-SW-003RE


Tot Ion: 95 Resp: 115768
Ion Ratio Lower Upper
95 100
174 85.4 0.0 165.8
176 80.2 0.0 159.8

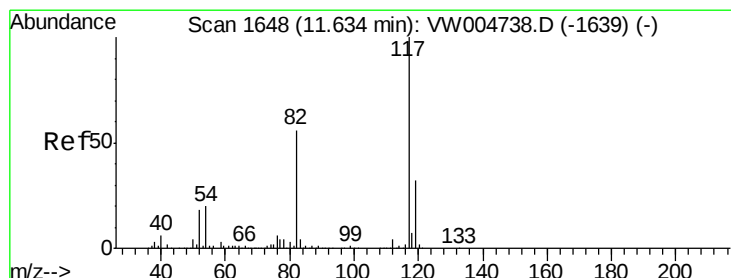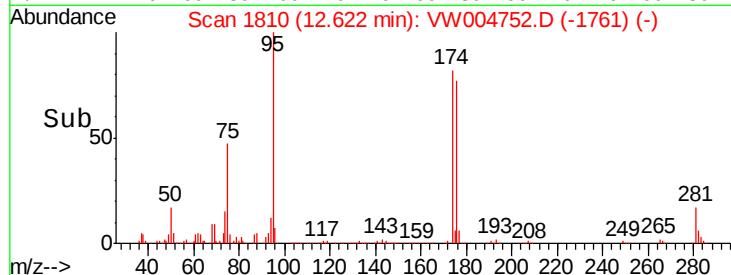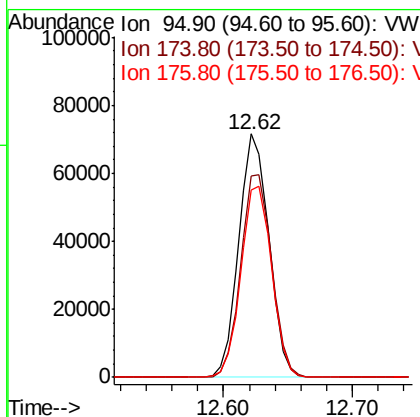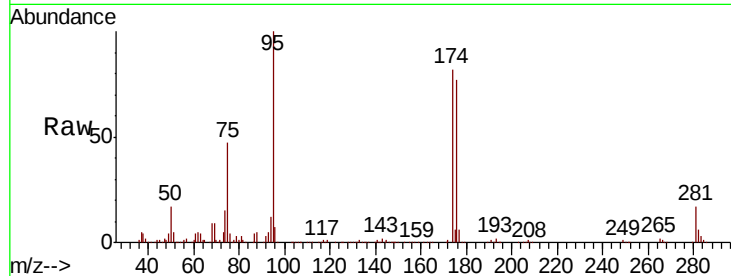

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.63 min Scan# 1648
Delta R.T. -0.00 min
Lab File: VW004752.D
Acq: 18 Aug 2018 00:04

Tgt Ion: 117 Resp: 442428
Ion Ratio Lower Upper
117 100
82 55.7 44.6 67.0
119 31.3 25.6 38.4

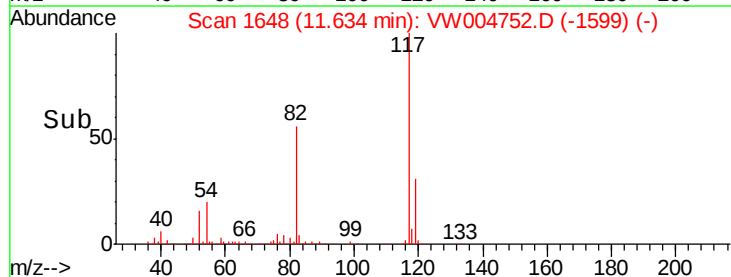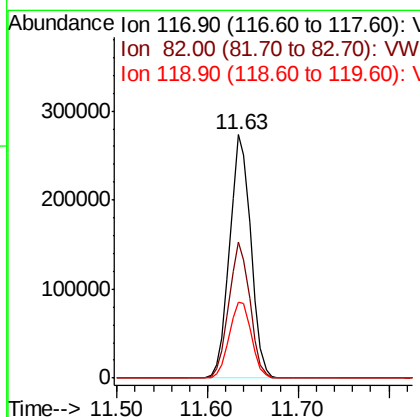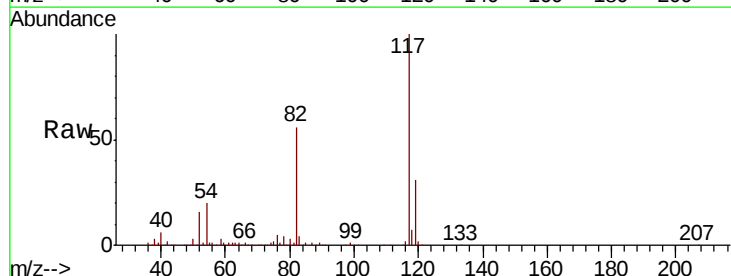

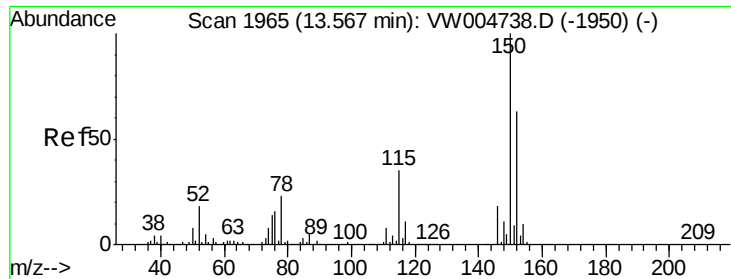

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.57 min Scan# 1965

Delta R.T. -0.00 min

Lab File: VW004752.D

Acq: 18 Aug 2018 00:04

Instrument :

MSVOA_W

ClientSampleId :

RA-081018-SW-003RE


Tot Ion:152 Resp: 101215

Ion Ratio Lower Upper

152 100

115 54.5 28.5 85.5

150 155.6 0.0 344.8

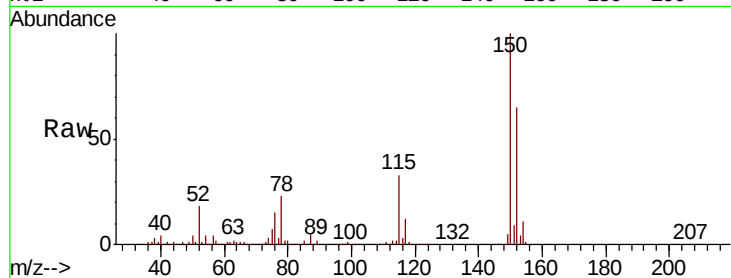

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

