

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081918\
 Data File : VW004765.D
 Acq On : 18 Aug 2018 07:22
 Operator : SY/AP
 Sample : J4500-09
 Misc : 4.28G/5ML/MSVOA W/SOIL
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 TP-6

Quant Time: Aug 20 01:16:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 18 01:49:53 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	566185	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	1023366	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	946924	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	428881	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	338318	61.81	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	123.62%	
35) Dibromofluoromethane	7.89	113	96824	14.80	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	29.60%	
50) Toluene-d8	10.33	98	1199289	46.97	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	93.94%	
62) 4-Bromofluorobenzene	12.62	95	379722	41.34	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	82.68%	
Target Compounds						
16) Acetone	4.14	43	64995	46.51	ug/l	96
20) Methylene Chloride	4.92	84	61334	5.80	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081918\
 Data File : VW004765.D
 Acq On : 18 Aug 2018 07:22
 Operator : SY/AP
 Sample : J4500-09
 Misc : 4.28G/5ML/MSVOA W/SOIL
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleID :
 TP-6

Quant Time: Aug 20 01:16:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 18 01:49:53 2018
 Response via : Initial Calibration




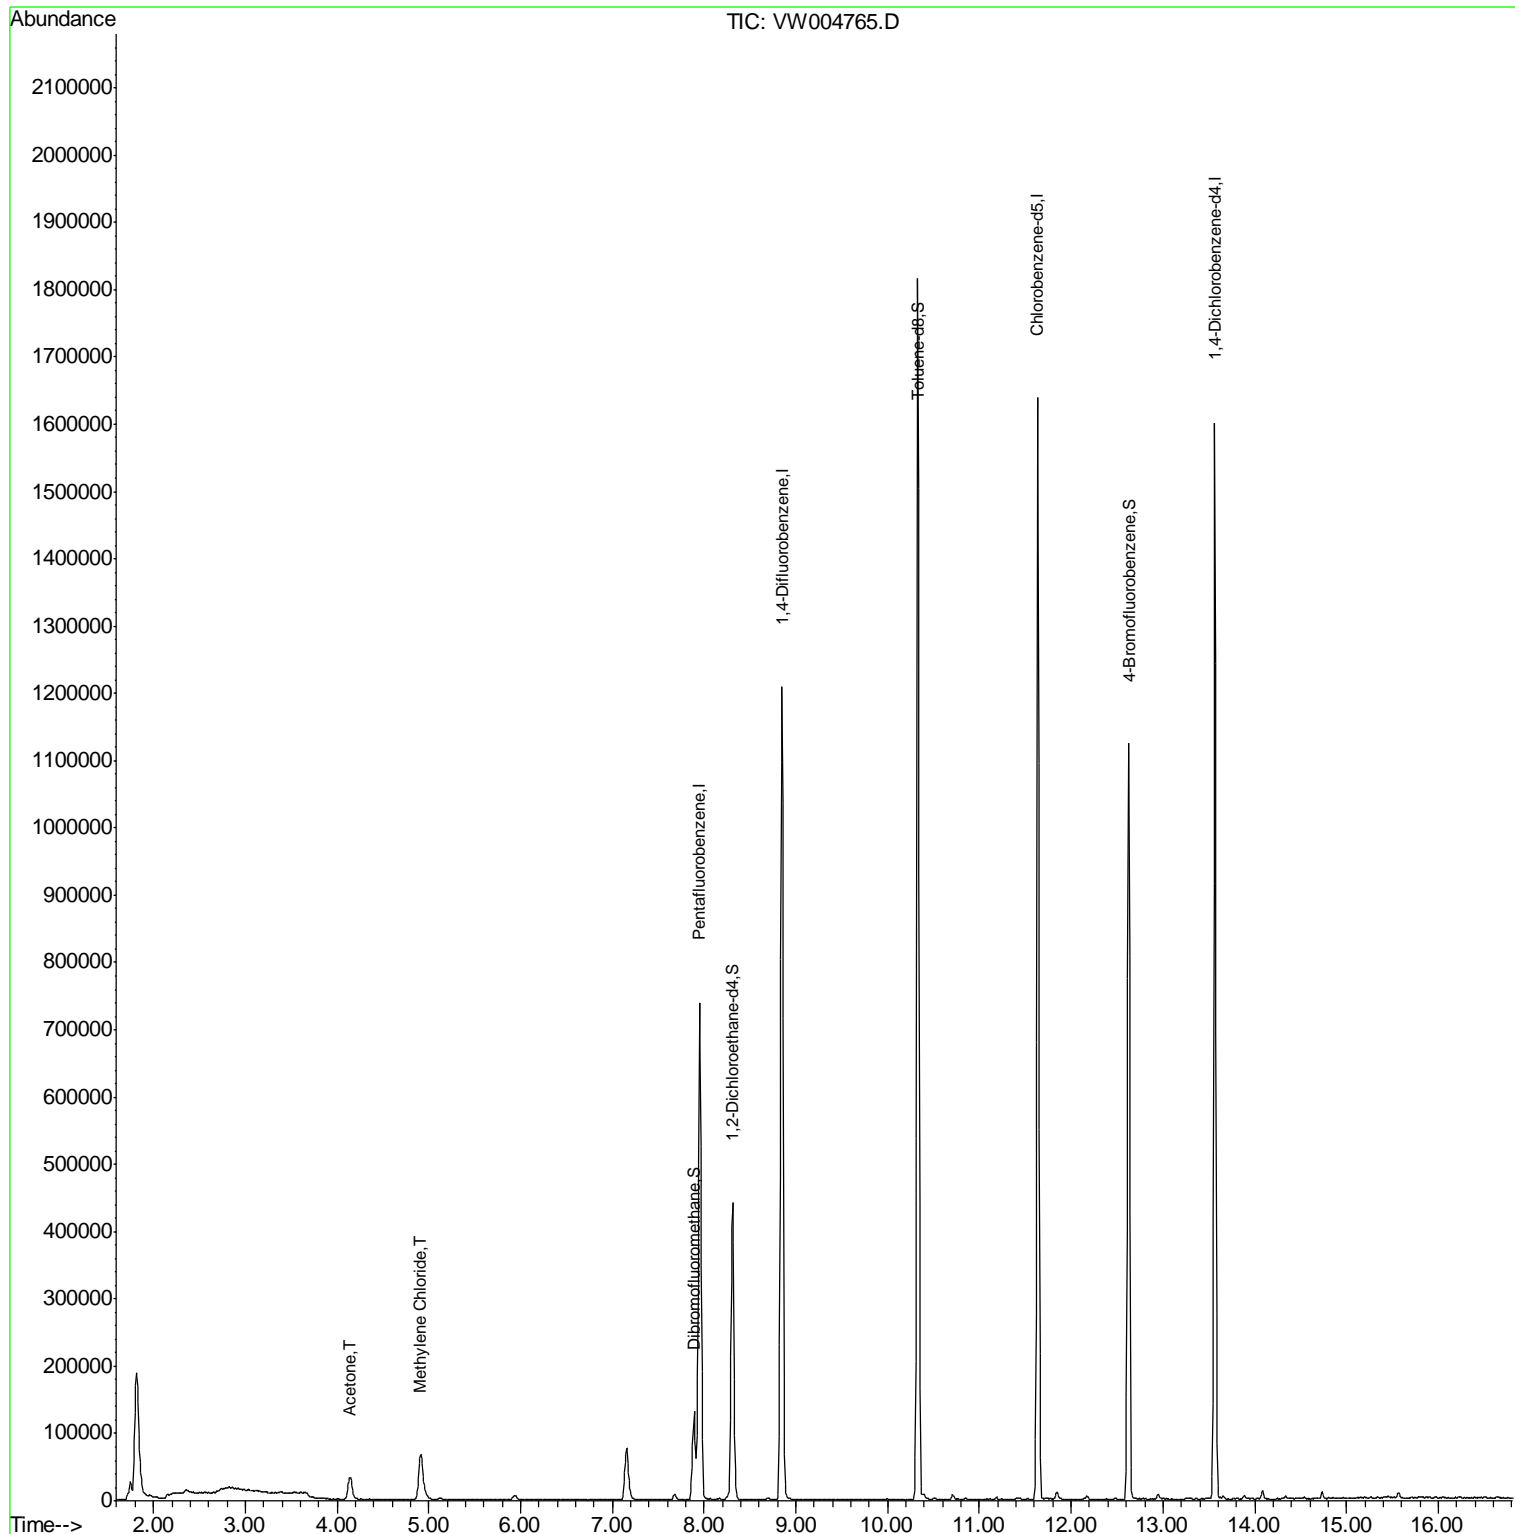


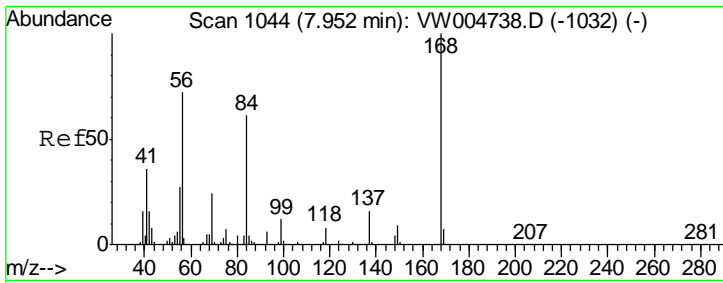

#1
 Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 7.95 min Scan# 1044
 Delta R.T. -0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22




Instrument : MSVOA_W
 ClientSampled : TP-6


Tgt Ion	Resp	Lower	Upper
168	100		
99	54.8	41.0	61.4

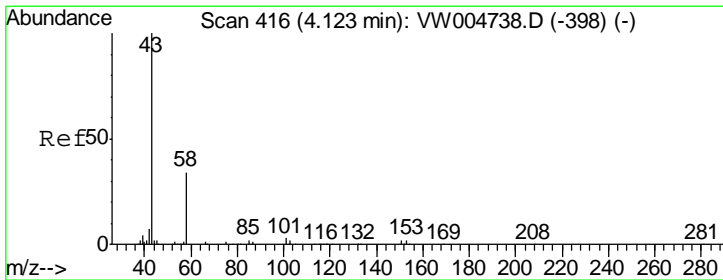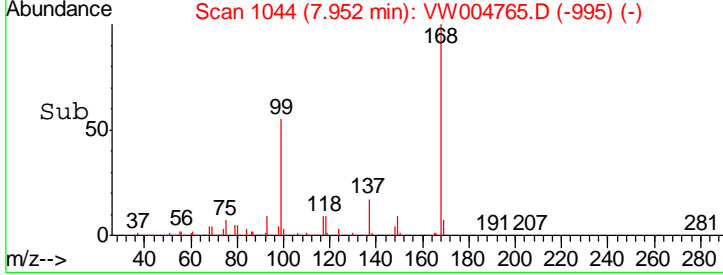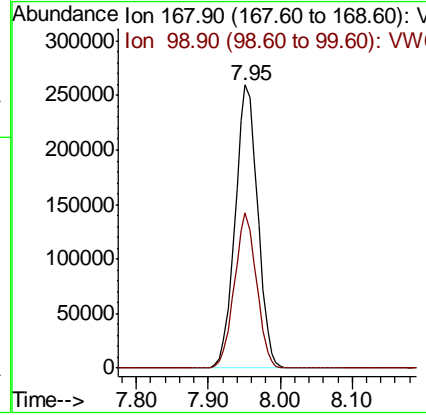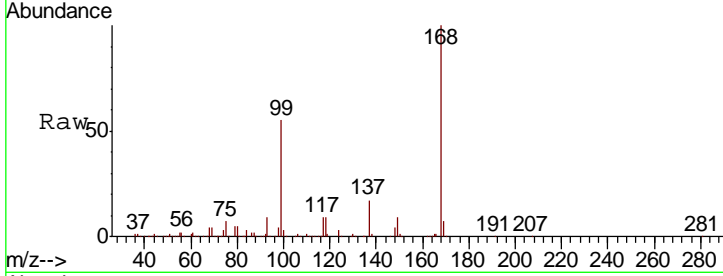

#16
 Acetone
 Concen: 46.51 ug/l
 RT: 4.14 min Scan# 418
 Delta R.T. 0.01 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22

Tgt Ion	Resp	Lower	Upper
43	100		
58	36.5	27.3	40.9


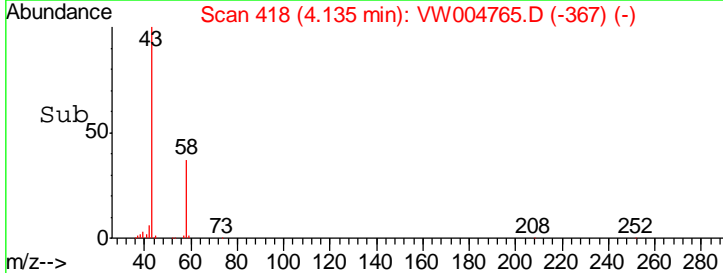
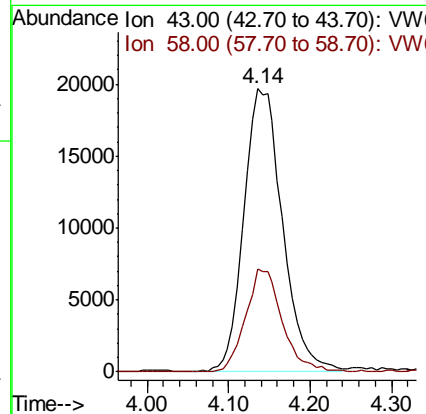
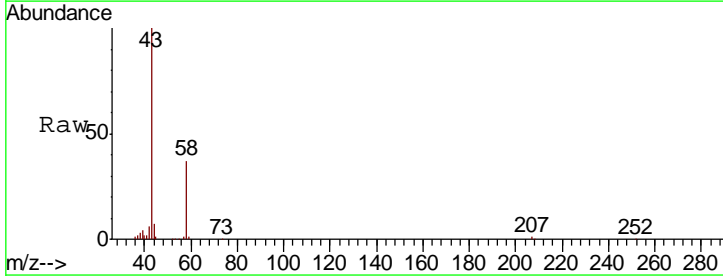


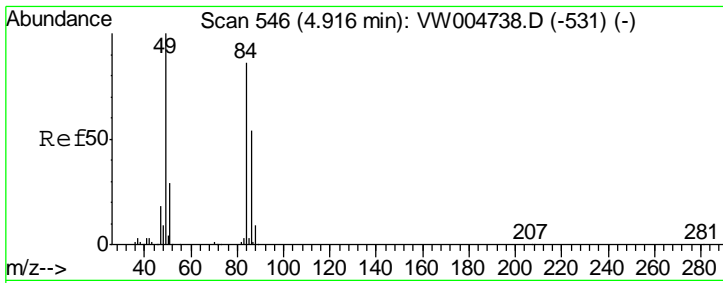

#20
 Methylene Chloride
 Concen: 5.80 ug/l
 RT: 4.92 min Scan# 546
 Delta R.T. 0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22




Instrument :
 MSVOA_W
 ClientSampled :
 TP-6


Tgt Ion	Resp	Lower	Upper
84	100		
49	113.6	93.2	139.8
51	33.5	27.4	41.0
86	59.1	50.6	75.8

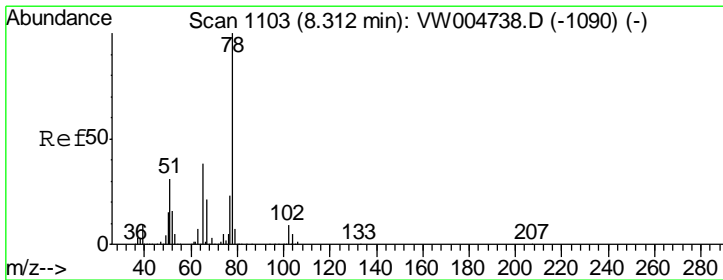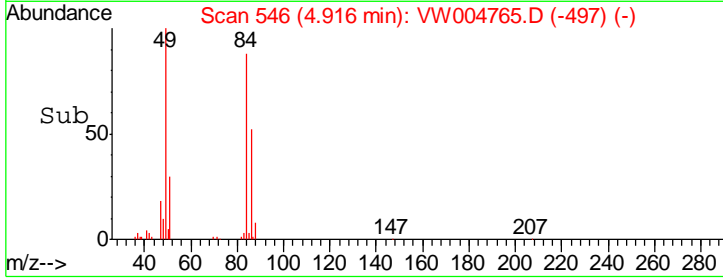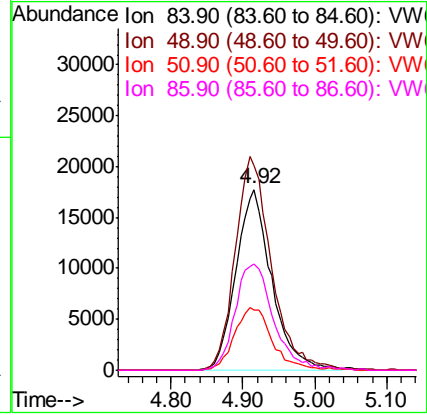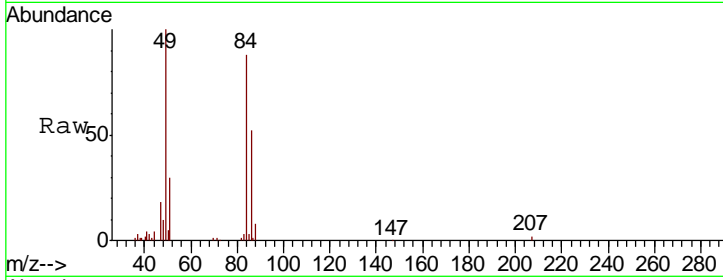

#33
 1,2-Dichloroethane-d4
 Concen: 61.81 ug/l
 RT: 8.31 min Scan# 1103
 Delta R.T. -0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22

Tgt Ion	Resp	Lower	Upper
65	100		
67	54.5	0.0	109.4


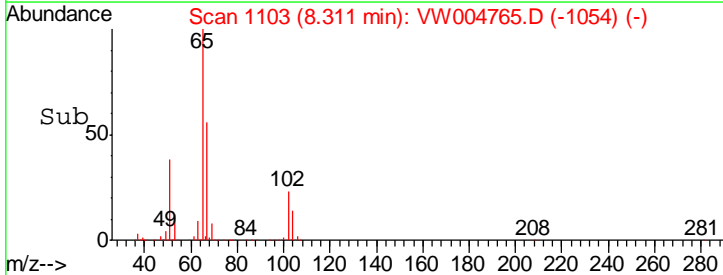
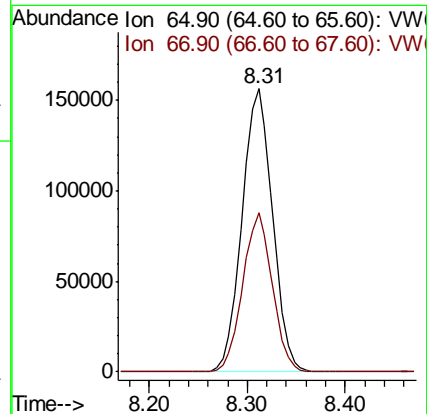
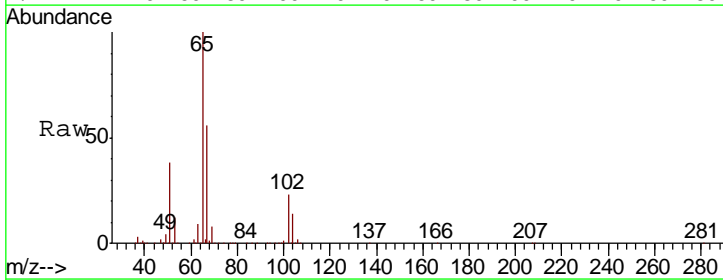


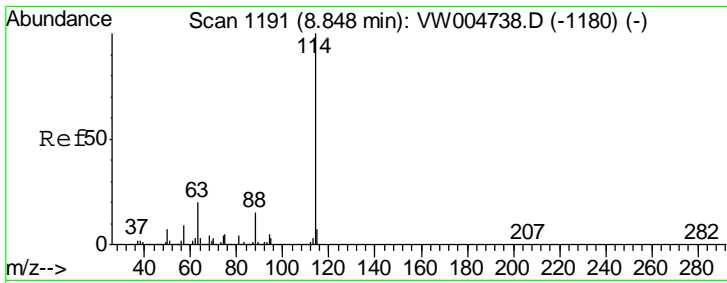

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22




Instrument :
 MSVOA_W
 ClientSampled :
 TP-6


Tgt Ion	Resp	Lower	Upper
114	1023366		
63	20.1	0.0	39.0
88	15.8	0.0	30.0

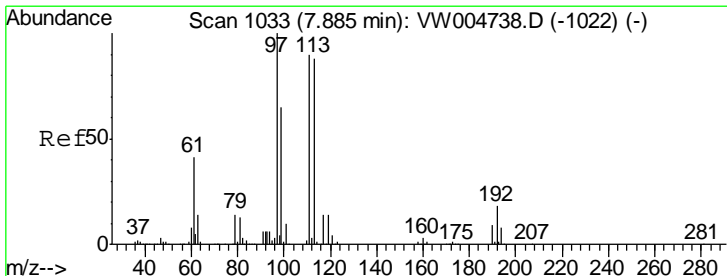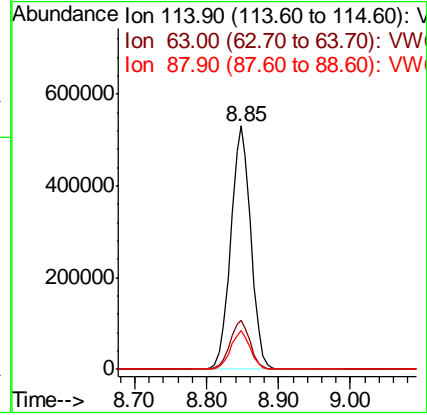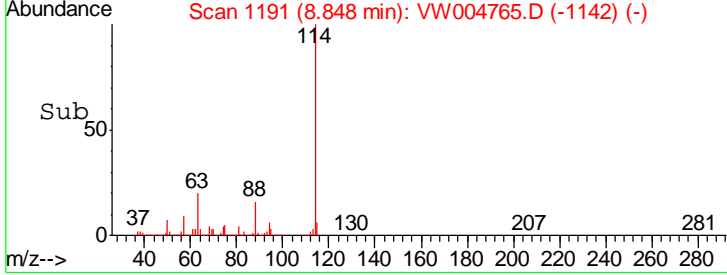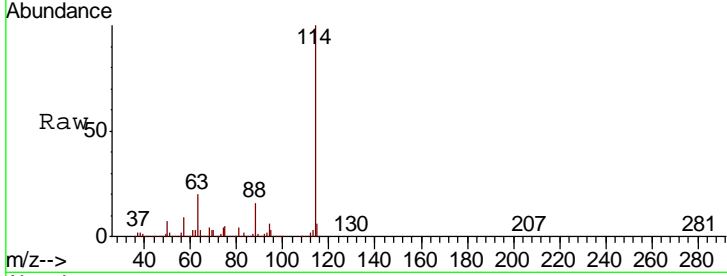

#35
 Dibromofluoromethane
 Concen: 14.80 ug/l
 RT: 7.89 min Scan# 1034
 Delta R.T. 0.01 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22

Tgt Ion	Resp	Lower	Upper
113	96824		
111	100.6	82.4	123.6
192	21.0	16.7	25.1


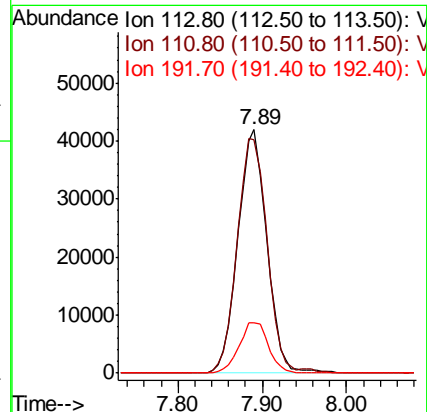
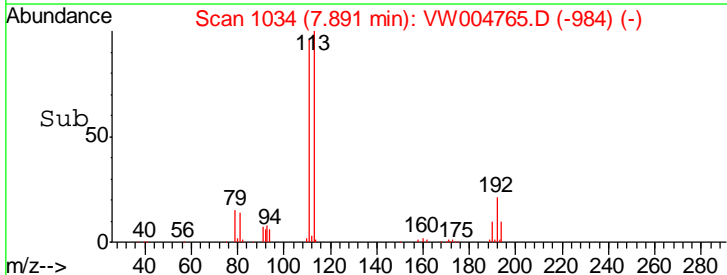
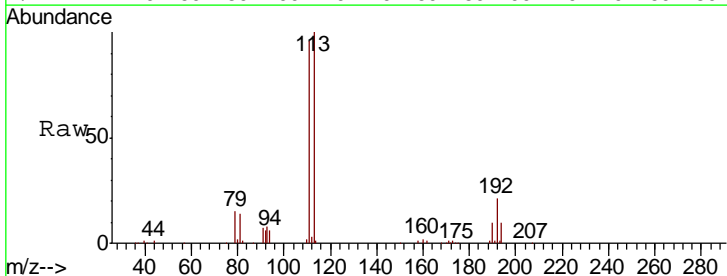


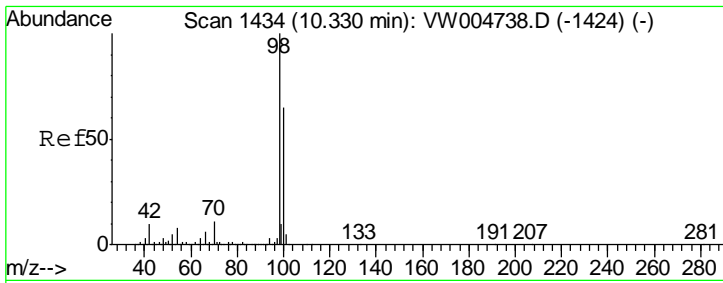

#50
 Toluene-d8
 Concen: 46.97 ug/l
 RT: 10.33 min Scan# 1434
 Delta R.T. -0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22




Instrument : MSVOA_W
 ClientSampled : TP-6


Tgt Ion	Resp	Lower	Upper
98	1199289		
100	63.9	51.8	77.8

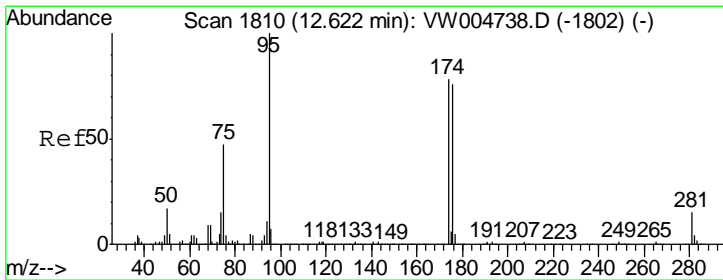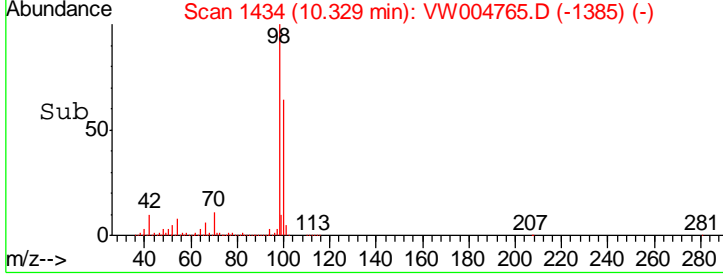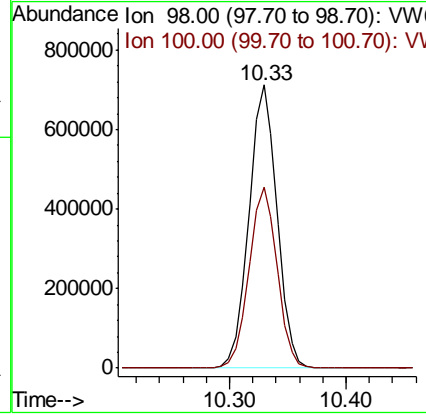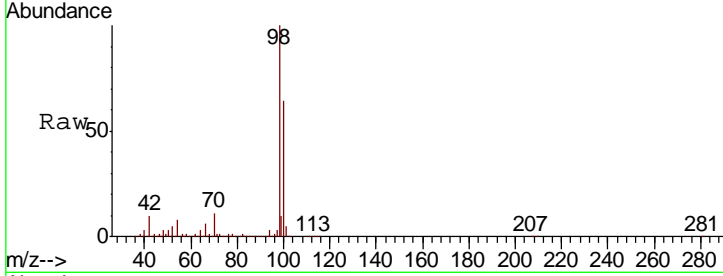

#62
 4-Bromofluorobenzene
 Concen: 41.34 ug/l
 RT: 12.62 min Scan# 1810
 Delta R.T. -0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22

Tgt Ion	Resp	Lower	Upper
95	379722		
174	83.6	0.0	165.8
176	82.0	0.0	159.8


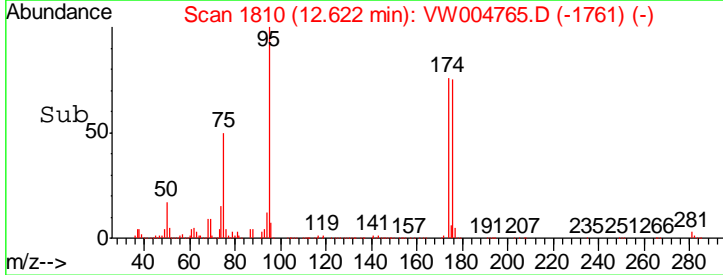
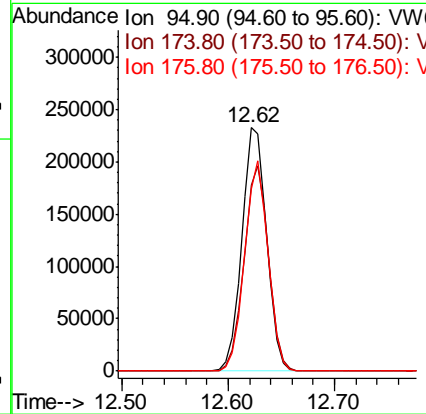
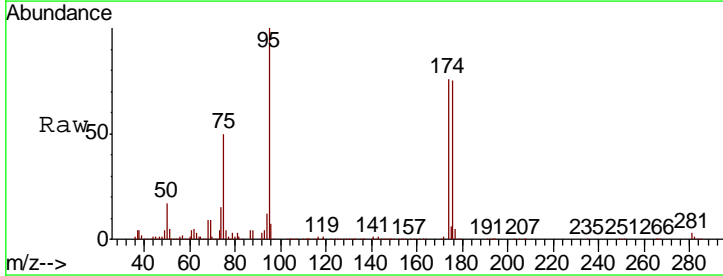


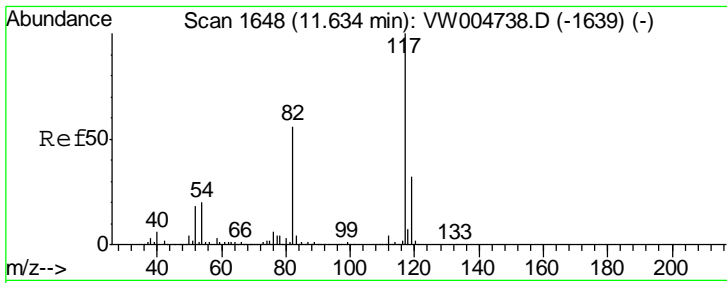

#63
 Chlorobenzene-d5
 Concen: 50.00 ug/l
 RT: 11.63 min Scan# 1648
 Delta R.T. -0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22

Instrument : MSVOA_W
 ClientSampled : TP-6

Tgt Ion	Resp	Lower	Upper
117	100		
82	53.2	44.6	67.0
119	32.1	25.6	38.4

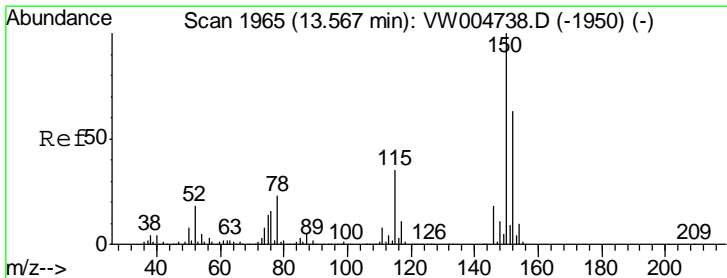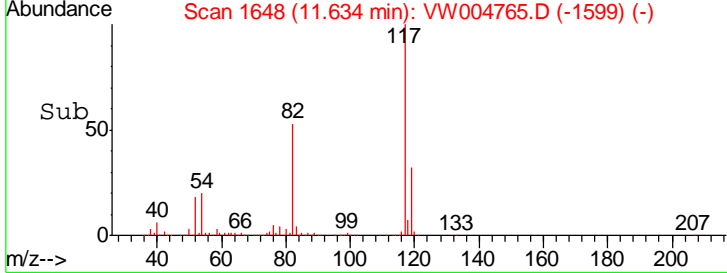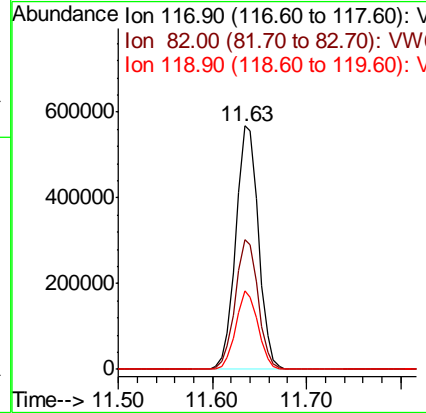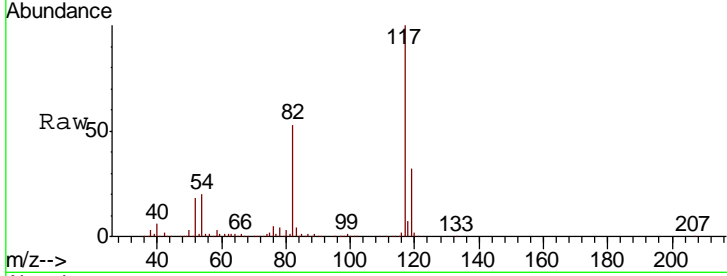

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.57 min Scan# 1965
 Delta R.T. -0.00 min
 Lab File: VW004765.D
 Acq: 18 Aug 2018 07:22

Tgt Ion	Resp	Lower	Upper
152	100		
115	57.0	28.5	85.5
150	154.7	0.0	344.8

