


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081918\
 Data File : VW004758.D
 Acq On : 18 Aug 2018 03:31
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
 Title : SW846 8260
 Last Update : Sat Aug 18 01:49:53 2018

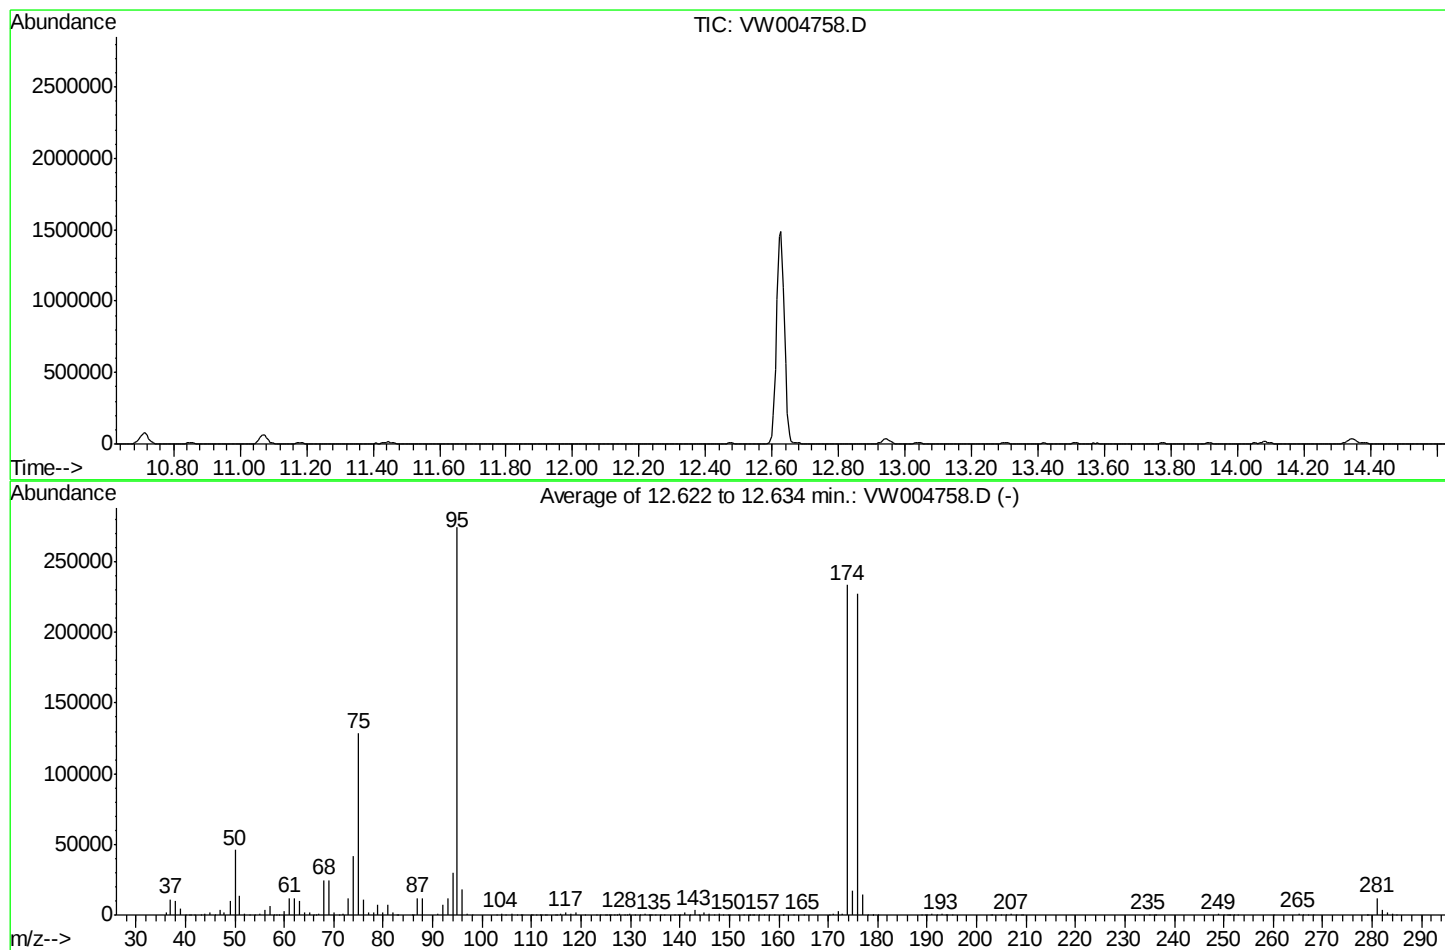

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	45829	PASS
75	95	30	60	46.8	128522	PASS
95	95	100	100	100.0	274346	PASS
96	95	5	9	6.5	17826	PASS
173	174	0.00	2	0.3	764	PASS
174	95	50	100	85.1	233365	PASS
175	174	5	9	7.4	17240	PASS
176	174	95	101	97.4	227306	PASS
177	176	5	9	6.5	14748	PASS