

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081921\
 Data File : VW019805.D
 Acq On : 19 Aug 2021 13:50
 Operator : SY/VA
 Sample : M3458-12
 Misc : 6.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AT8

Quant Time: Aug 20 00:45:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 20 00:38:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	329991	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	308265	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	111718	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	142180	27.808	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.240%
7) Chloroethane-d5	2.898	69	118787	26.469	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.880%
11) 1,1-Dichloroethene-d2	4.025	63	152212	17.157	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.640%
21) 2-Butanone-d5	7.086	46	33539	32.295	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.580%
24) Chloroform-d	7.653	84	210518	23.197	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	8.311	65	114952	23.505	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	8.281	84	414664	23.592	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.360%
36) 1,2-Dichloropropane-d6	9.281	67	125944	23.662	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.640%
41) Toluene-d8	10.323	98	360819	22.401	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	10.579	79	46394	21.099	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.400%
47) 2-Hexanone-d5	10.927	63	23193	31.279	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.560%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	89335	20.622	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.480%
66) 1,2-Dichlorobenzene-d4	13.853	152	96518	25.186	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.760%
Target Compounds						
16) Methylene chloride	4.928	84	8570	1.513	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081921\
Data File : VW019805.D
Acq On : 19 Aug 2021 13:50
Operator : SY/VA
Sample : M3458-12
Misc : 6.09g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AT8


Quant Time: Aug 20 00:45:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 20 00:38:38 2021
Response via : Initial Calibration

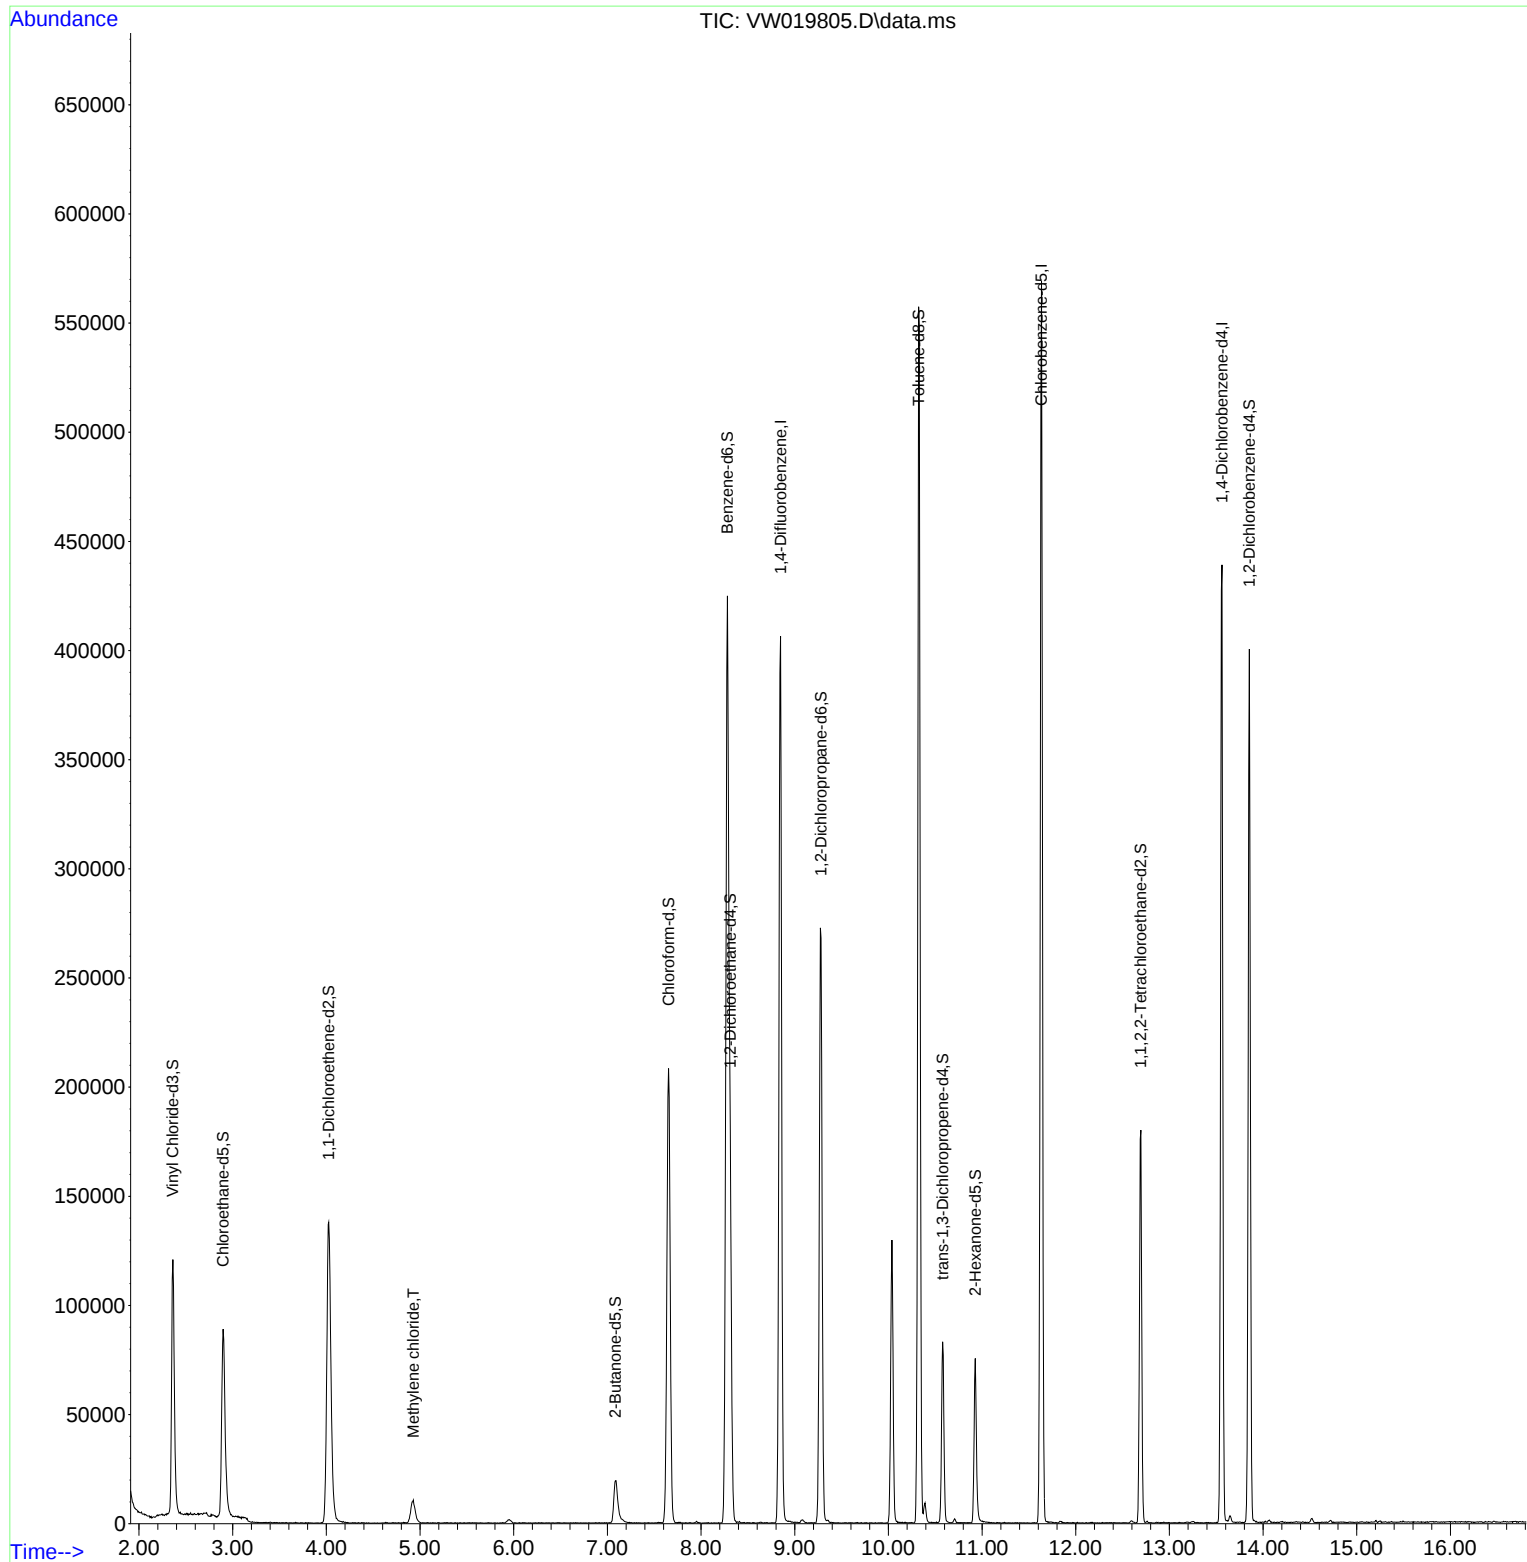

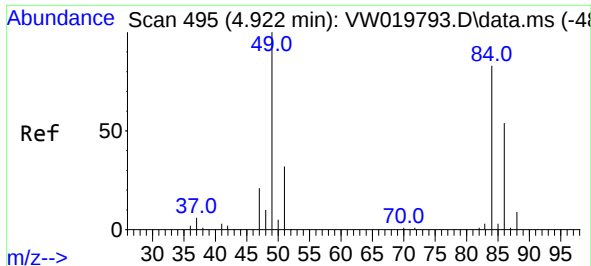

#16
Methylene chloride
Concen: 1.513 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW019805.D
Acq: 19 Aug 2021 13:50

Instrument :
MSVOA_W
ClientSampleId :
C0AT8

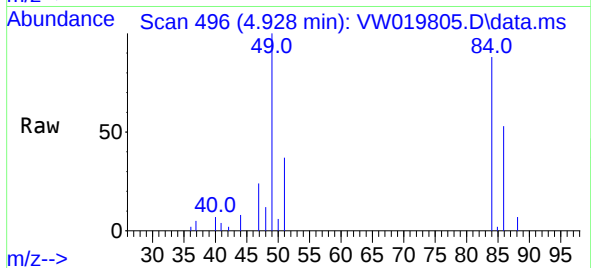

Tgt Ion:	84	Resp:	8570
Ion	Ratio	Lower	Upper
84	100		
86	59.9	45.3	84.1
49	113.5	86.6	160.8

