

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082018\
 Data File : VW004798.D
 Acq On : 20 Aug 2018 18:19
 Operator : SY/AP
 Sample : J4499-02
 Misc : 5.08G/5ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 LSB-02(0-1)

Quant Time: Aug 21 01:29:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 18 01:49:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	541508	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	881659	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	663206	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	187203	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	337661	64.50	ug/l	0.00
Spiked Amount			Recovery	=	129.00%	
35) Dibromofluoromethane	7.89	113	328932	58.37	ug/l	0.00
Spiked Amount			Recovery	=	116.74%	
50) Toluene-d8	10.33	98	1017693	46.27	ug/l	0.00
Spiked Amount			Recovery	=	92.54%	
62) 4-Bromofluorobenzene	12.62	95	242740	30.67	ug/l	0.00
Spiked Amount			Recovery	=	61.34%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
20) Methylene Chloride	4.91	84	59685	5.98	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW082018\
Data File : VW004798.D
Acq On : 20 Aug 2018 18:19
Operator : SY/AP
Sample : J4499-02
Misc : 5.08G/5ML/MSVOA W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
LSB-02(0-1)

Quant Time: Aug 21 01:29:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 18 01:49:53 2018
Response via : Initial Calibration

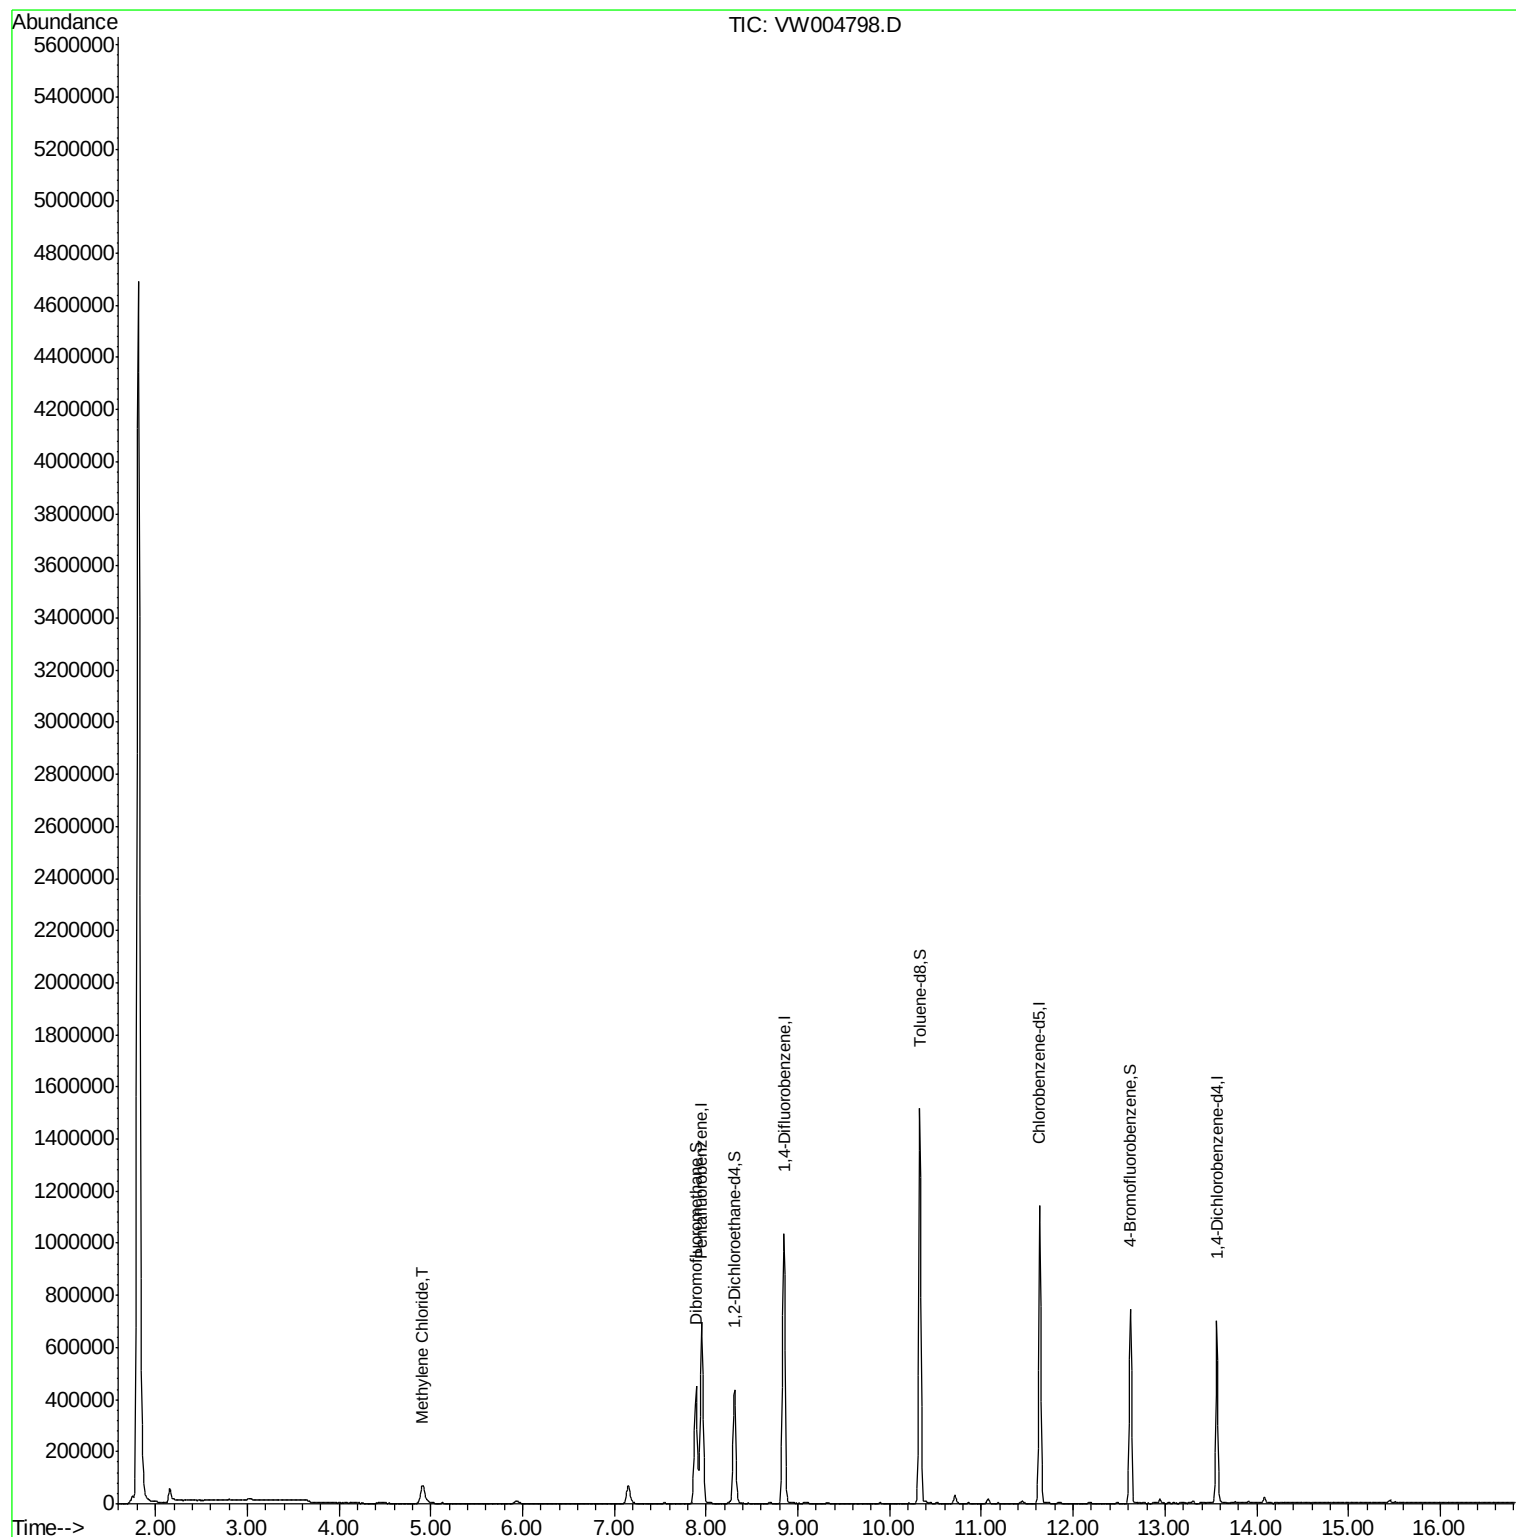

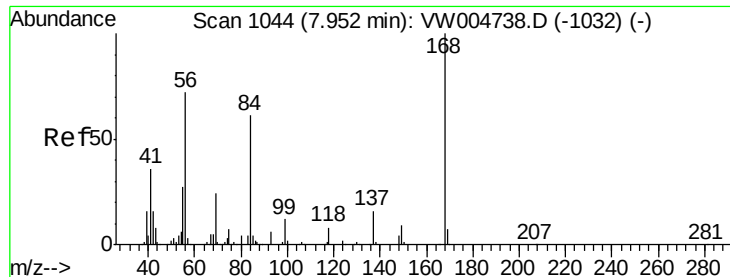

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1044

Delta R.T. -0.00 min

Lab File: VW004798.D

Acq: 20 Aug 2018 18:19

Instrument :

MSVOA_W

ClientSampled :


LSB-02(0-1)

Tot Ion:168 Resp: 541508

Ion Ratio Lower Upper

168 100

99 53.0 41.0 61.4

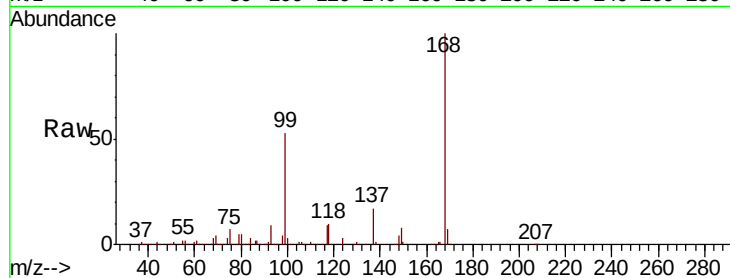

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

250000

200000



150000

100000

50000

0

Time--> 7.80 7.90 8.00 8.10

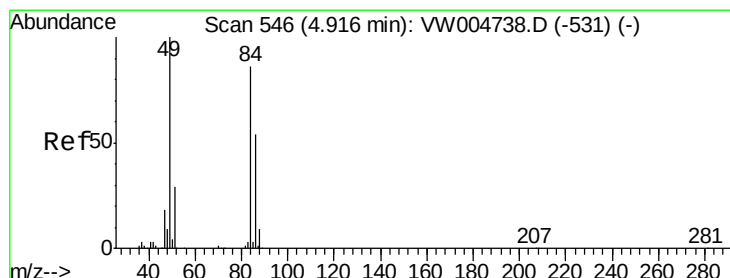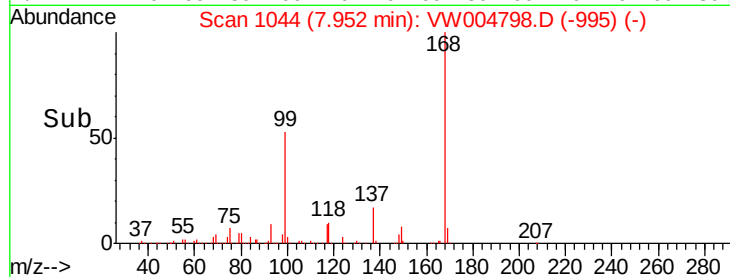

#20

Methylene Chloride

Concen: 5.98 ug/l

RT: 4.91 min Scan# 545

Delta R.T. -0.01 min

Lab File: VW004798.D

Acq: 20 Aug 2018 18:19

Tgt Ion: 84 Resp: 59685


Ion Ratio Lower Upper

84 100

49 112.3 93.2 139.8

51 34.2 27.4 41.0

86 62.0 50.6 75.8

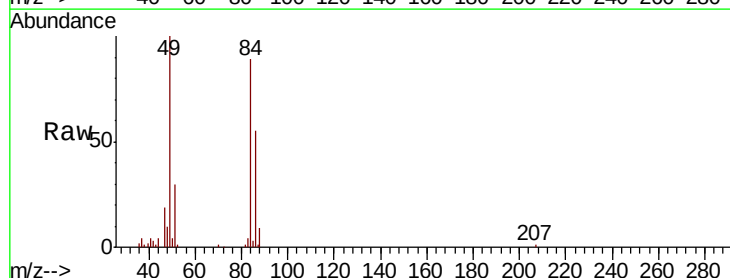

Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

4.91

30000

25000

20000


15000


10000

5000

0

Time--> 4.80 4.90 5.00




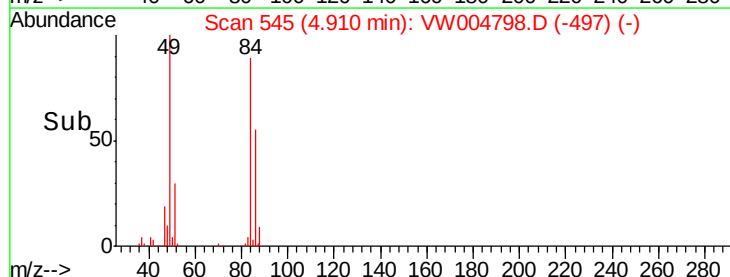


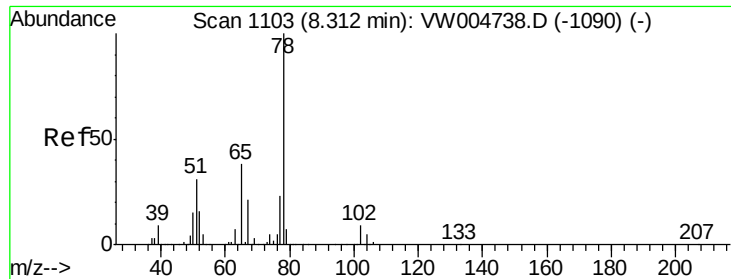

#33
 1,2-Dichloroethane-d4
 Concen: 64.50 ug/l
 RT: 8.31 min Scan# 1103
 Delta R.T. -0.00 min
 Lab File: VW004798.D
 Acq: 20 Aug 2018 18:19




Instrument :
 MSVOA_W
 ClientSampleId :
 LSB-02(0-1)


Tot Ion: 65 Resp: 337661
 Ion Ratio Lower Upper
 65 100
 67 54.0 0.0 109.4

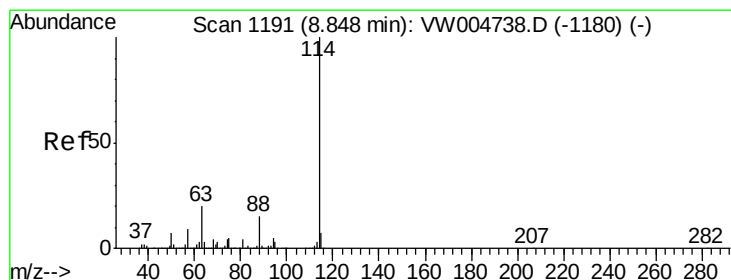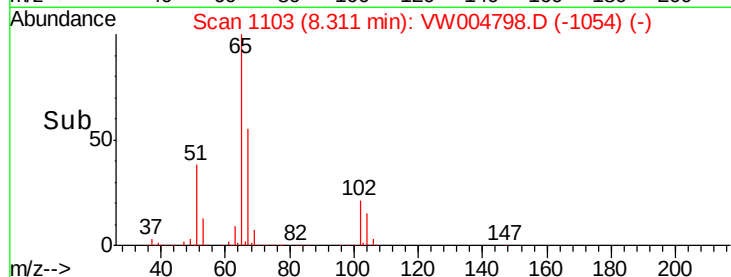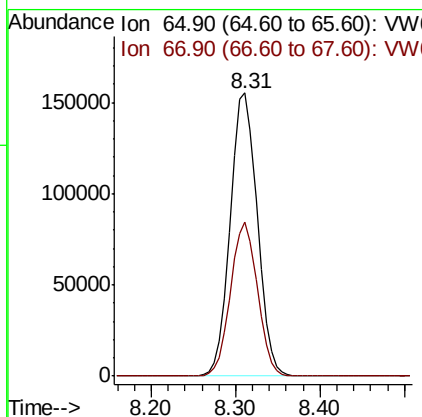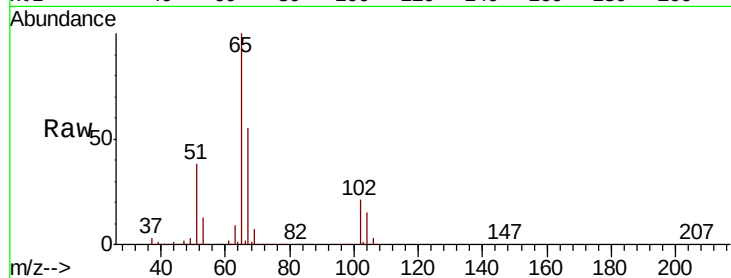

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: VW004798.D
 Acq: 20 Aug 2018 18:19

Tgt Ion: 114 Resp: 881659
 Ion Ratio Lower Upper
 114 100
 63 20.4 0.0 39.0
 88 15.6 0.0 30.0

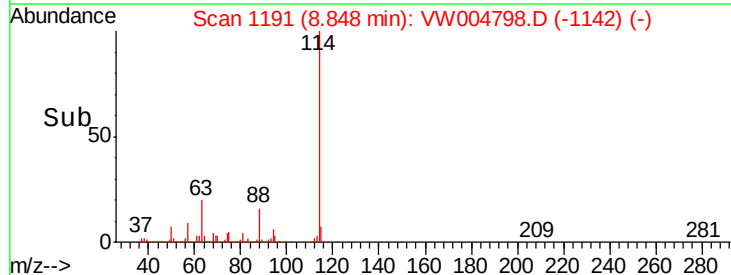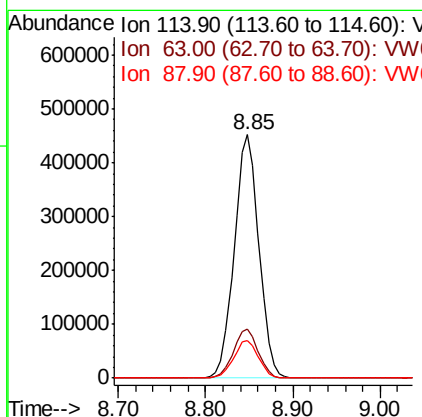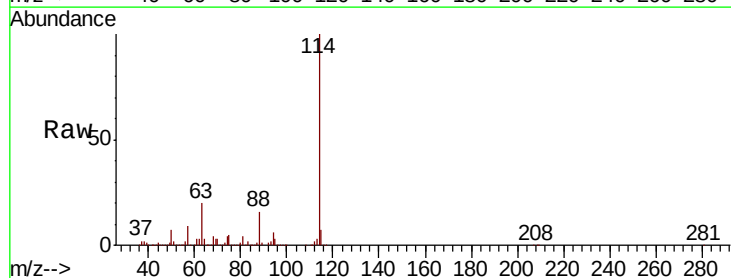


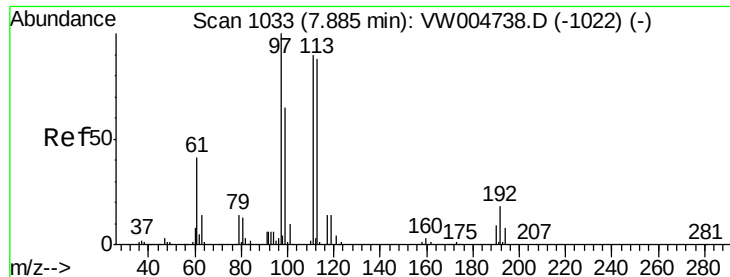




#35
 Dibromofluoromethane
 Concen: 58.37 ug/l
 RT: 7.89 min Scan# 1034
 Delta R.T. 0.01 min
 Lab File: VW004798.D
 Acq: 20 Aug 2018 18:19

Instrument :
 MSVOA_W
 ClientSampleId :
 LSB-02(0-1)

Tot Ion	Ratio	Lower	Upper
113	100		
111	103.0	82.4	123.6
192	21.1	16.7	25.1

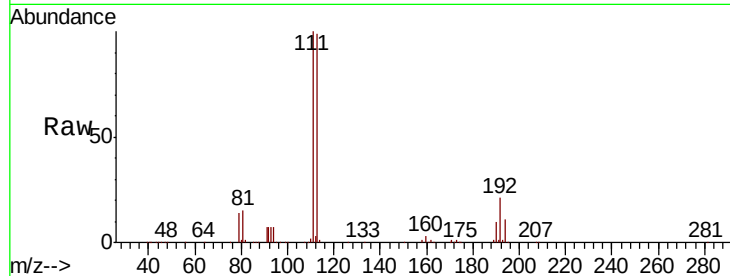


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

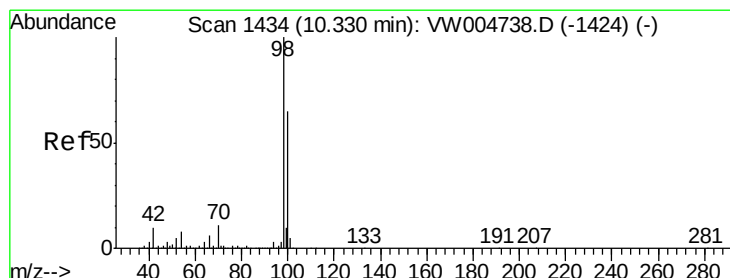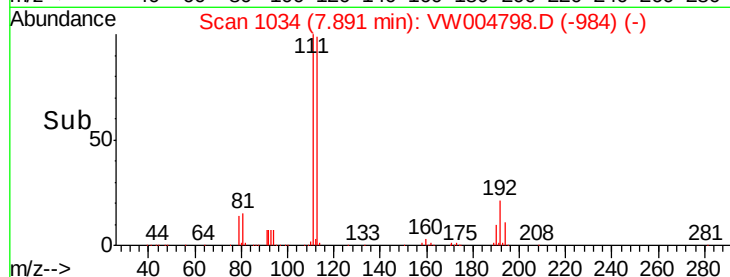
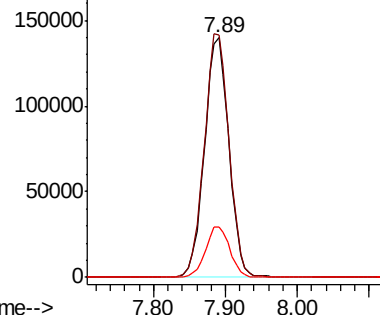



#50
 Toluene-d8
 Concen: 46.27 ug/l
 RT: 10.33 min Scan# 1434
 Delta R.T. -0.00 min
 Lab File: VW004798.D
 Acq: 20 Aug 2018 18:19

Tgt Ion	Ratio	Lower	Upper
98	100		
100	63.8	51.8	77.8

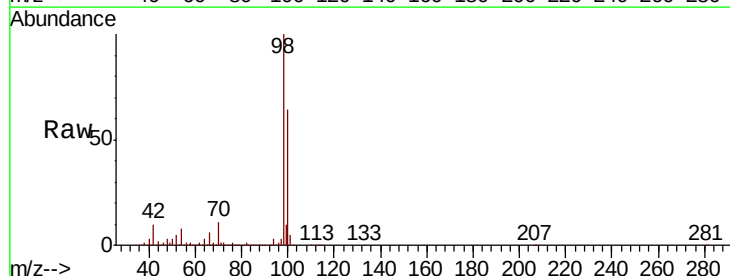

Abundance Ion 98.00 (97.70 to 98.70): VW
 Ion 100.00 (99.70 to 100.70): VW



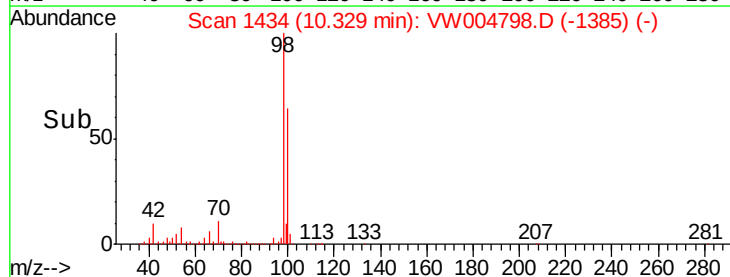
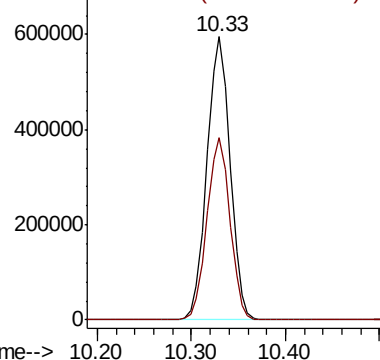


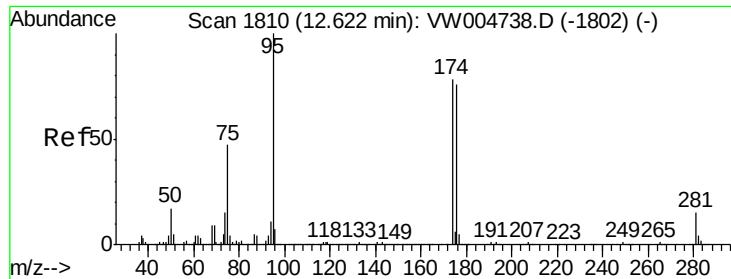

#62
4-Bromofluorobenzene
Concen: 30.67 ug/l
RT: 12.62 min Scan# 1810
Delta R.T. -0.00 min
Lab File: VW004798.D
Acq: 20 Aug 2018 18:19




Instrument :
MSVOA_W
ClientSampled :
LSB-02(0-1)


Tot Ion: 95 Resp: 242740
Ion Ratio Lower Upper
95 100
174 83.2 0.0 165.8
176 79.8 0.0 159.8

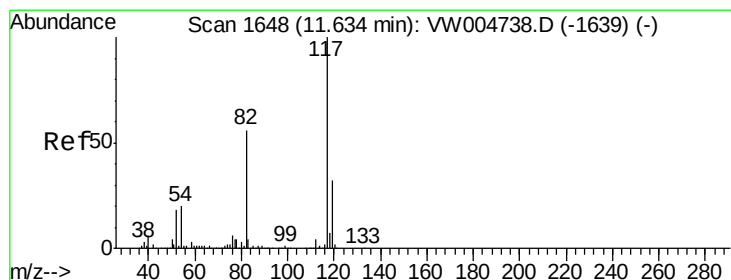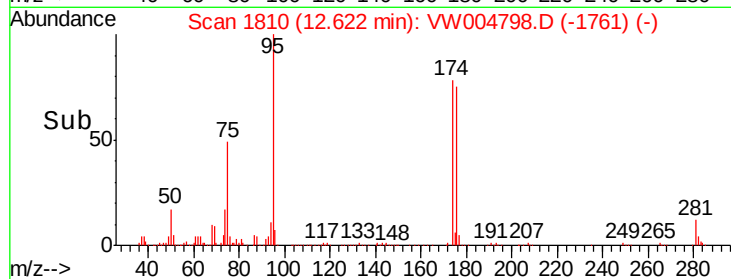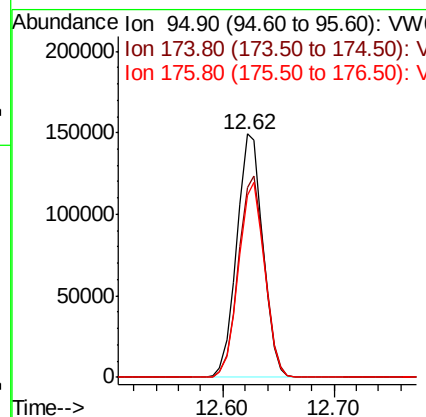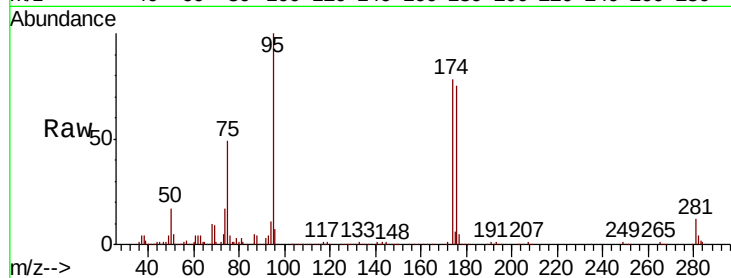

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.63 min Scan# 1648
Delta R.T. -0.00 min
Lab File: VW004798.D
Acq: 20 Aug 2018 18:19

Tgt Ion: 117 Resp: 663206
Ion Ratio Lower Upper
117 100
82 56.1 44.6 67.0
119 32.2 25.6 38.4

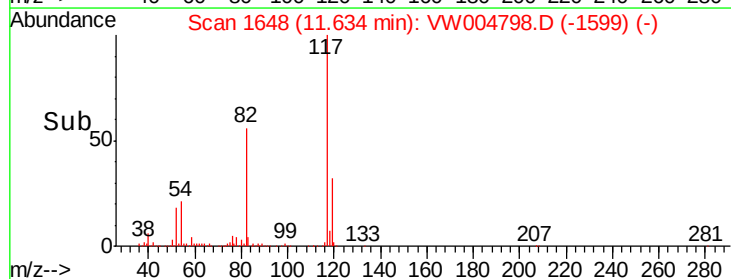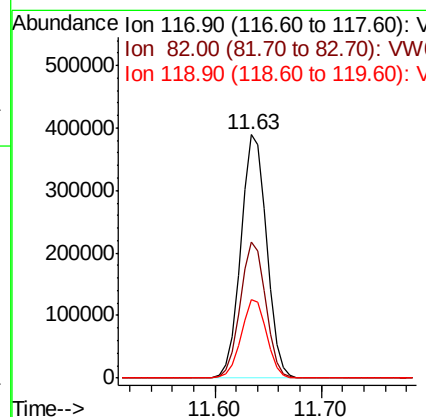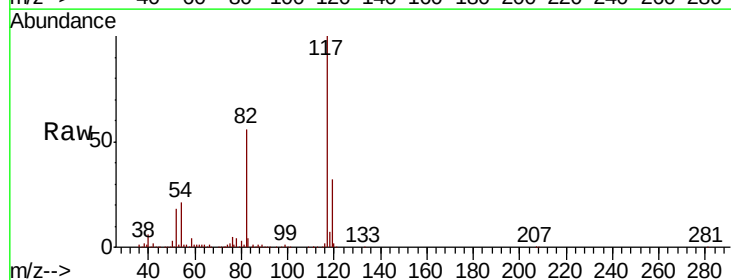

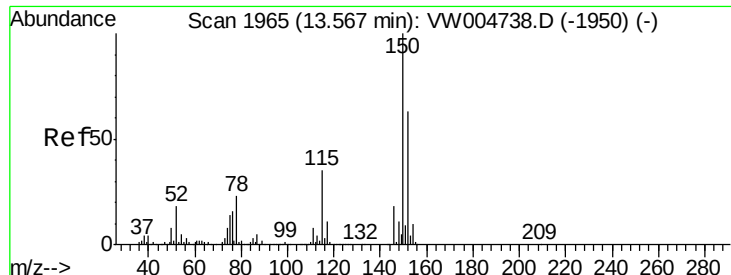

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.57 min Scan# 1965

Delta R.T. -0.00 min

Lab File: VW004798.D

Acq: 20 Aug 2018 18:19

Instrument :

MSVOA_W

ClientSampleId :

LSB-02(0-1)


Tot Ion:152 Resp: 187203

Ion Ratio Lower Upper

152 100

115 57.8 28.5 85.5

150 157.5 0.0 344.8

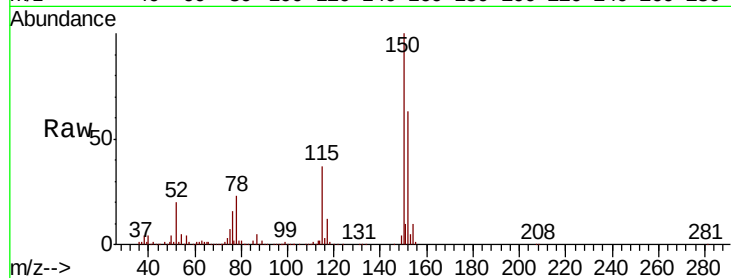

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

