


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW082018\
Data File : VW004806.D
Acq On : 20 Aug 2018 22:36
Operator : SY/AP
Sample : BFB
Misc : 5.05G/5ML/MSVOA W/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081918S.M
Title : SW846 8260
Last Update : Sat Aug 18 01:49:53 2018

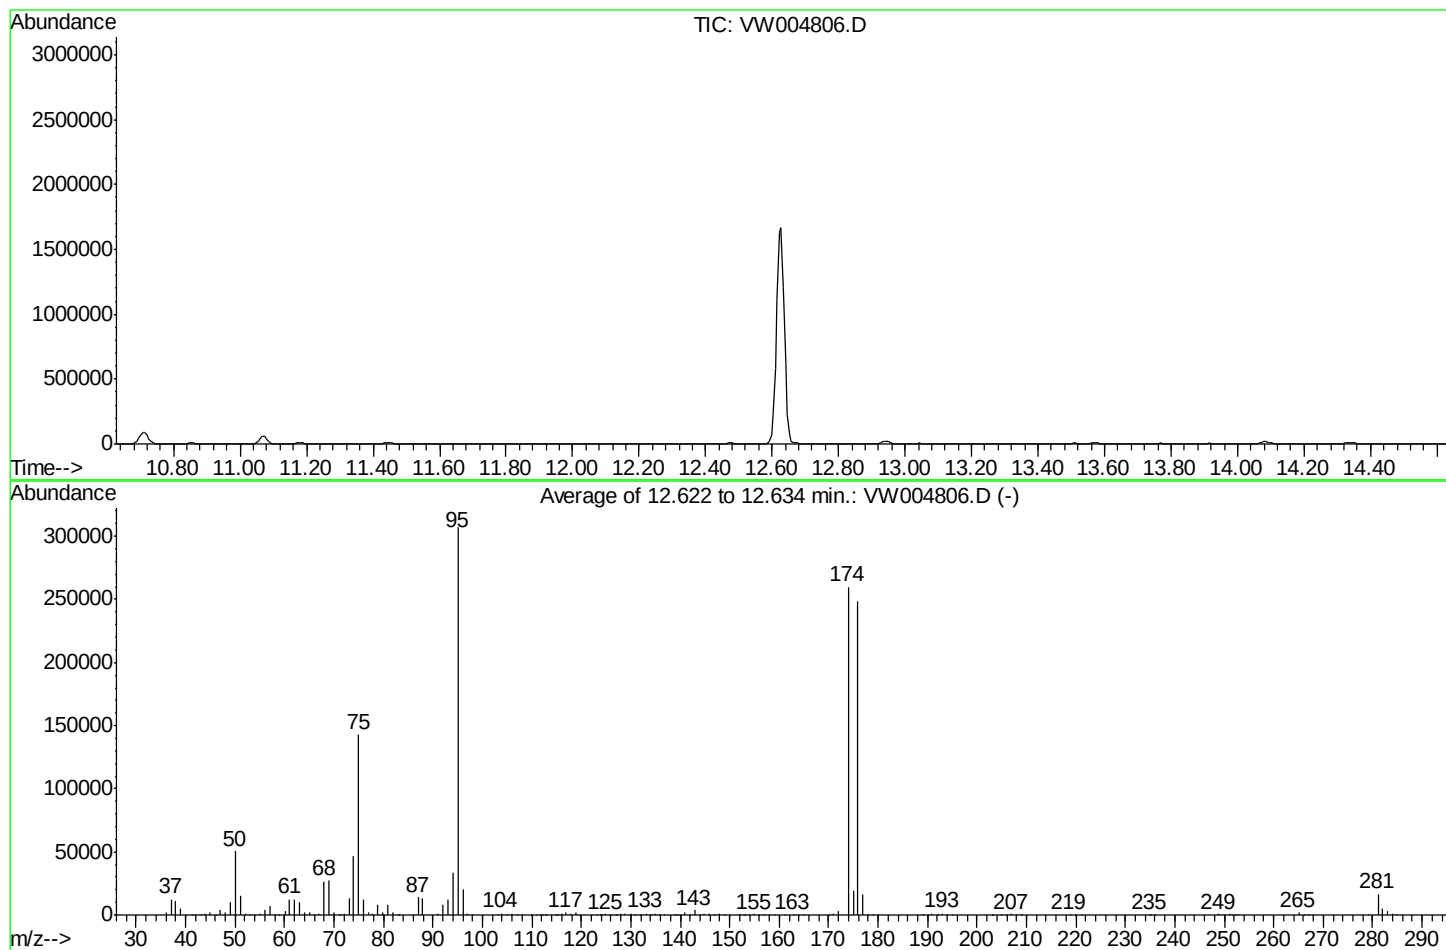

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	50309	PASS
75	95	30	60	46.4	142528	PASS
95	95	100	100	100.0	307093	PASS
96	95	5	9	6.5	20001	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.6	259904	PASS
175	174	5	9	7.4	19170	PASS
176	174	95	101	95.5	248170	PASS
177	176	5	9	6.7	16679	PASS