

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082020\
 Data File : VW016273.D
 Acq On : 20 Aug 2020 17:57
 Operator : SY/VA
 Sample : L3767-14
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Quant Time: Aug 21 04:57:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 21 03:27:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	338738	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	323241	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	144446	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	68341	16.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.08%
7) Chloroethane-d5	2.89	69	56804	17.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.28%
10) 1,1-Dichloroethene-d2	4.02	63	123351	13.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.32%
20) 2-Butanone-d5	7.08	46	56606	51.22	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.44%
24) Chloroform-d	7.65	84	196870	21.66	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.64%
26) 1,2-Dichloroethane-d4	8.31	65	106374	22.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.12%
29) Benzene-d6	8.28	84	384444	21.86	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.44%
33) 1,2-Dichloropropane-d6	9.27	67	113578	21.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.84%
37) Toluene-d8	10.32	98	347366	21.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.16%
38) trans-1,3-Dichloropropene-	10.58	79	48766	20.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.92%
39) 2-Hexanone-d5	10.93	63	46306	51.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.82%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	107413	25.52	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.08%
61) 1,2-Dichlorobenzene-d4	13.85	152	128394	25.08	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.32%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	24602	4.600 ug/L	90




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW082020\
Data File : VW016273.D
Acq On : 20 Aug 2020 17:57
Operator : SY/VA
Sample : L3767-14
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Aug 21 04:57:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 21 03:27:50 2020
Response via : Initial Calibration

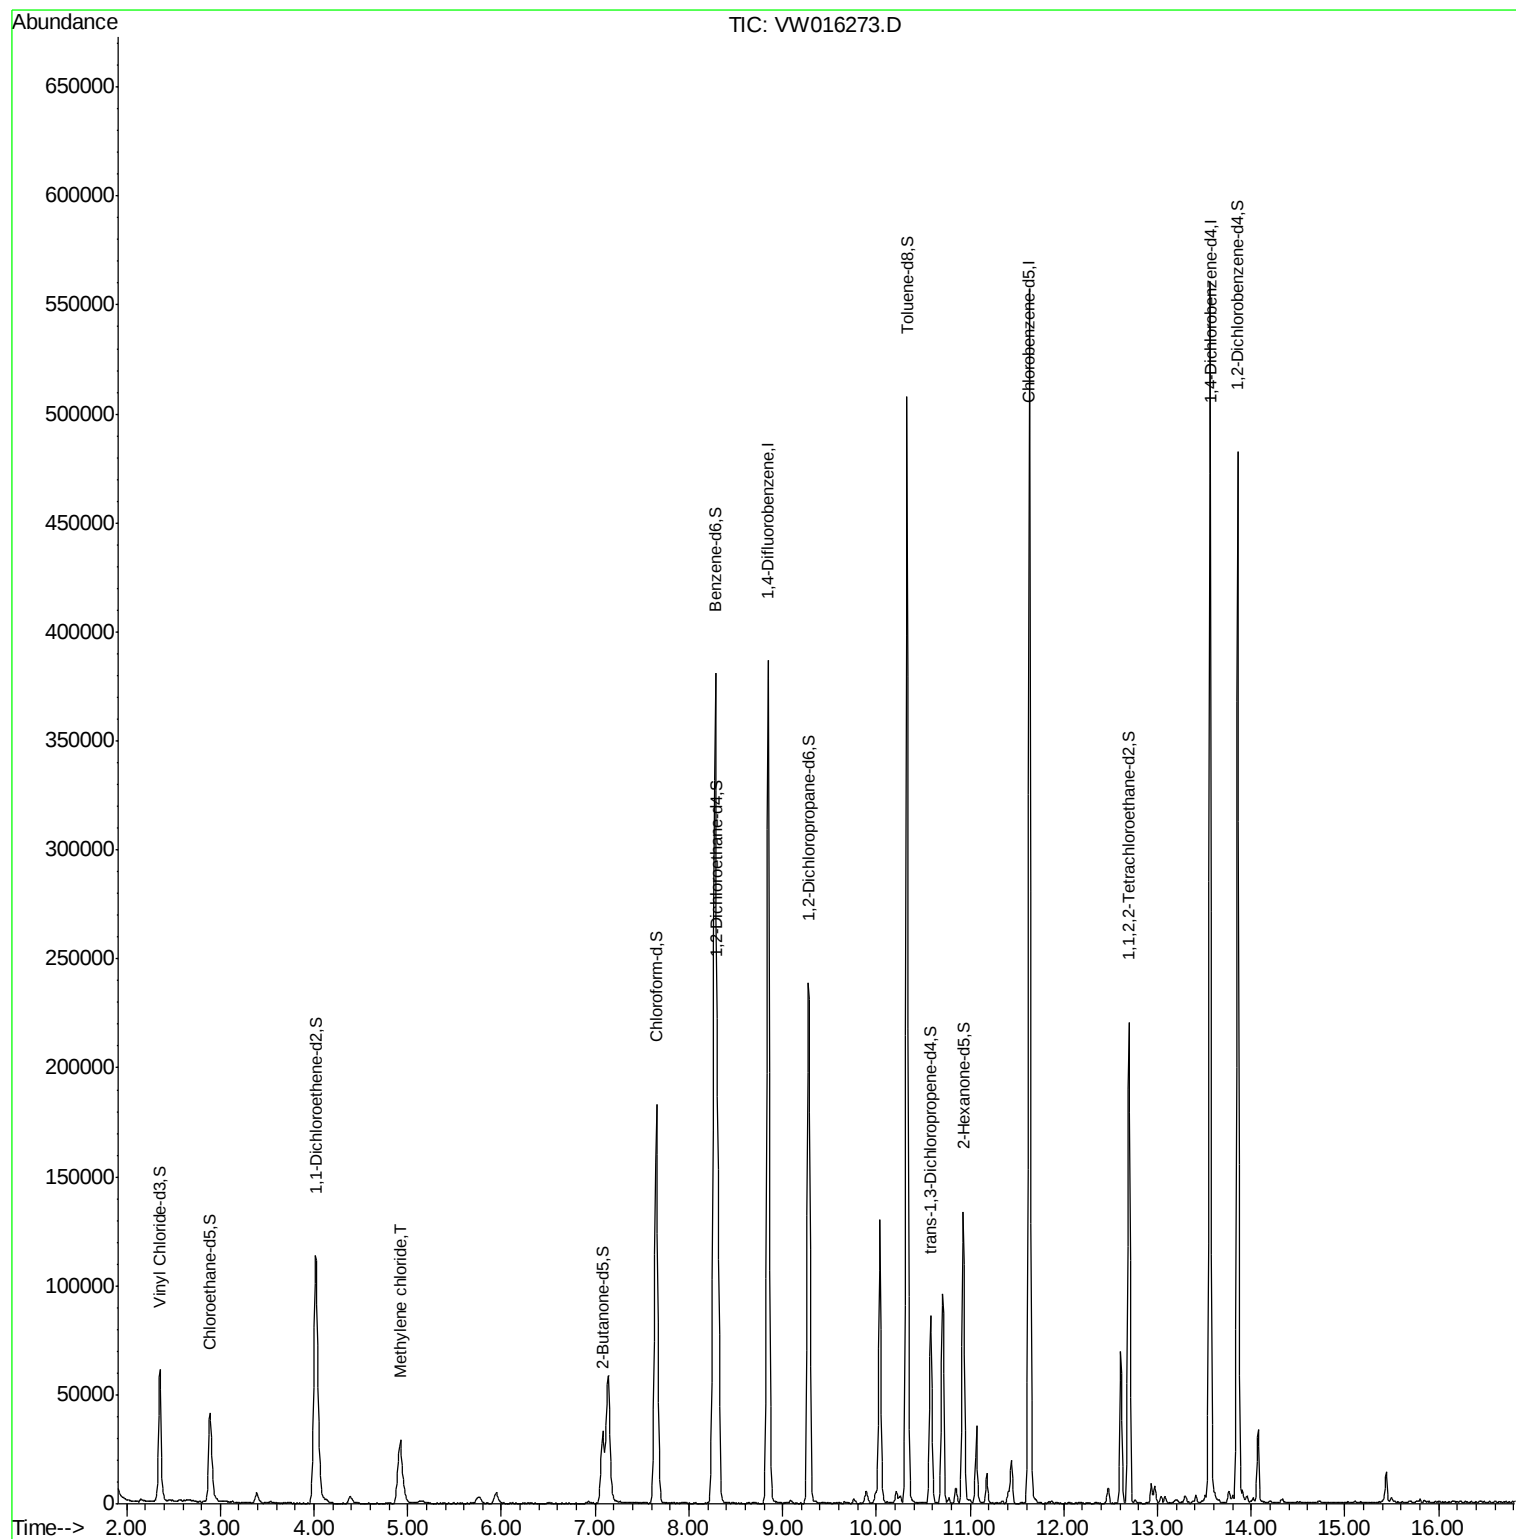

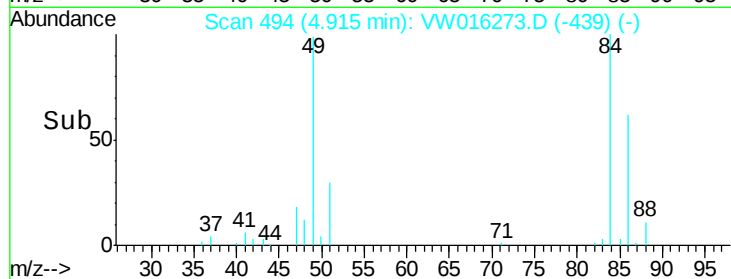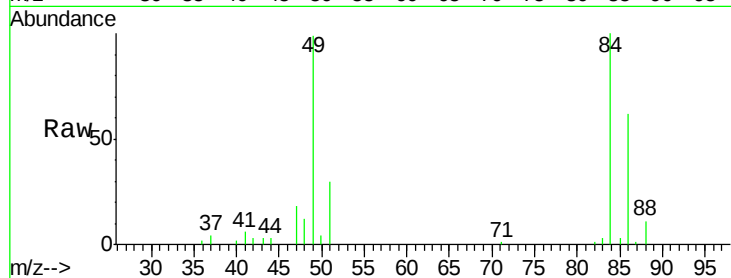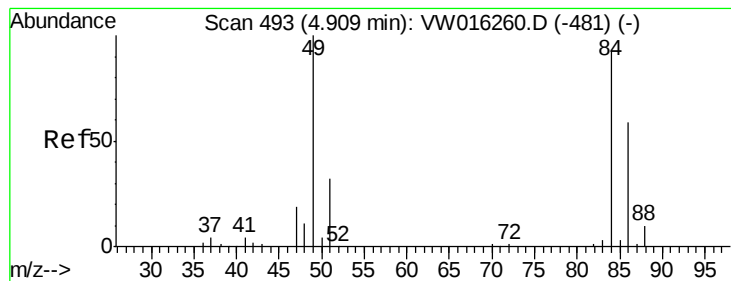

#16
Methylene chloride
Concen: 4.600 ug/L
RT: 4.92 min Scan# 494
Delta R.T. 0.01 min
Lab File: VW016273.D
Acq: 20 Aug 2020 17:57

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Tot Ion: 84 Resp: 24602

Ion	Ratio	Lower	Upper
84	100		
49	98.9	80.4	149.4
86	61.8	43.8	81.3

