

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082219\
 Data File : VW012118.D
 Acq On : 22 Aug 2019 18:26
 Operator : SY/VA
 Sample : K4461-17
 Misc : 5.01G/5ML/MSVOA W/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-09-5.5-6.0

Quant Time: Aug 23 08:20:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 00:23:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	13389	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	20243	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	14538	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	2620	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	7707	50.13	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.26%	
35) Dibromofluoromethane	7.89	113	6565	57.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	115.62%	
50) Toluene-d8	10.32	98	23695	50.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.92%	
62) 4-Bromofluorobenzene	12.62	95	4820	29.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	58.16%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW082219\
Data File : VW012118.D
Acq On : 22 Aug 2019 18:26
Operator : SY/VA
Sample : K4461-17
Misc : 5.01G/5ML/MSVOA W/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-09-5.5-6.0

Quant Time: Aug 23 08:20:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 00:23:30 2019
Response via : Initial Calibration

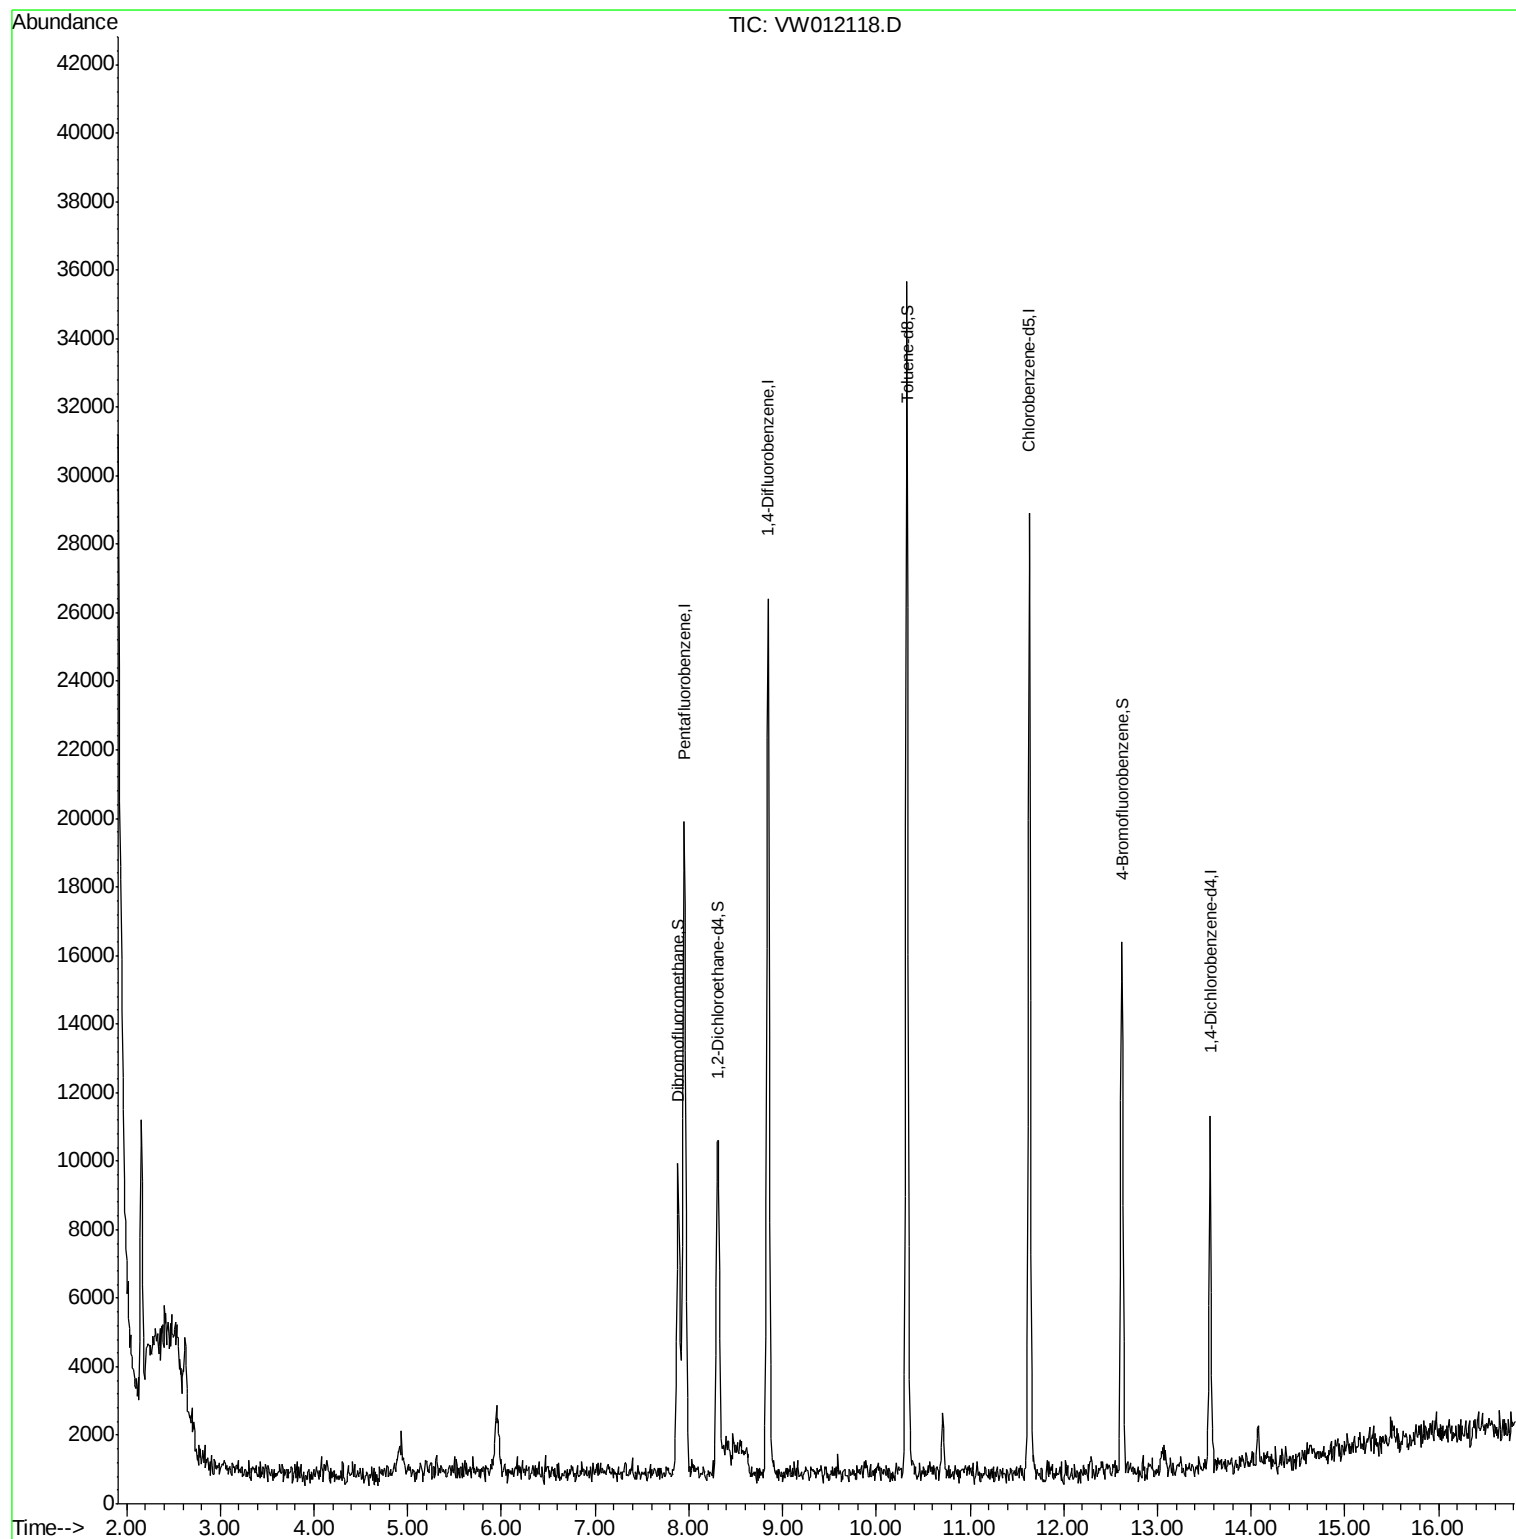

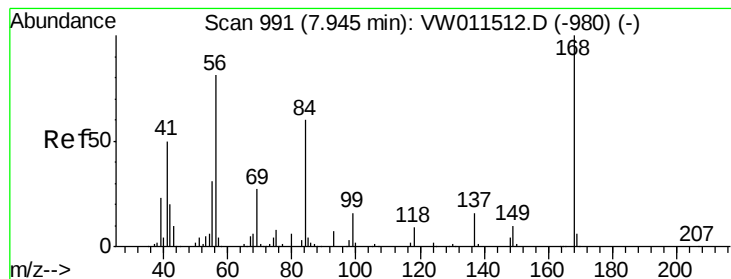

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.01 min

Lab File: VW012118.D

Acq: 22 Aug 2019 18:26

Instrument :

MSVOA_W

ClientSampleId :


SB-09-5.5-6.0

Tot Ion:168 Resp: 13389

Ion Ratio Lower Upper




168 100

99 63.5 48.2 72.4

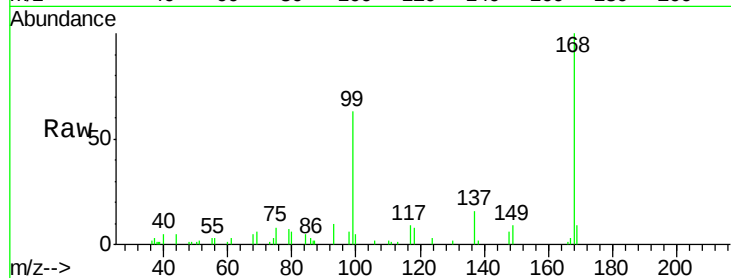

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

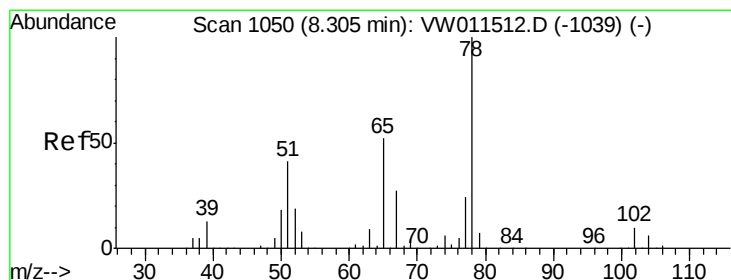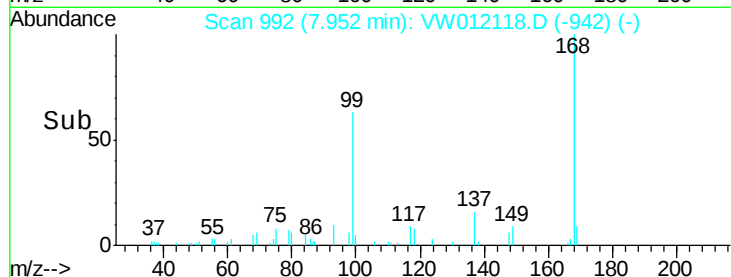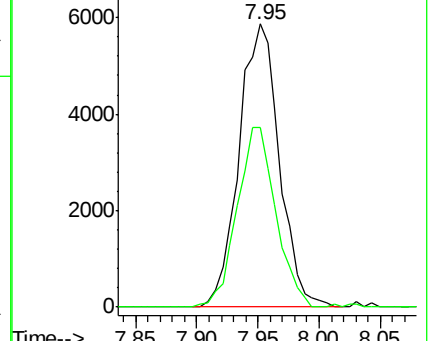

#33

1,2-Dichloroethane-d4

Concen: 50.129 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW012118.D


Acq: 22 Aug 2019 18:26

Tgt Ion: 65 Resp: 7707

Ion Ratio Lower Upper



65 100


67 53.6 0.0 105.2

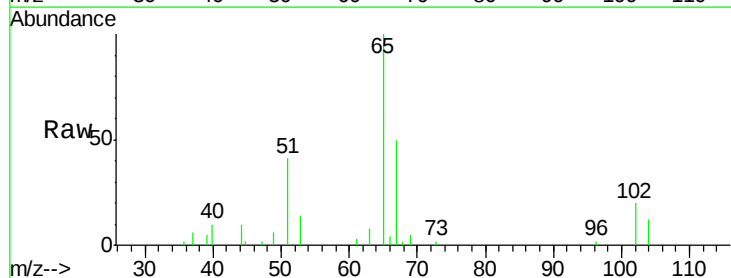

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

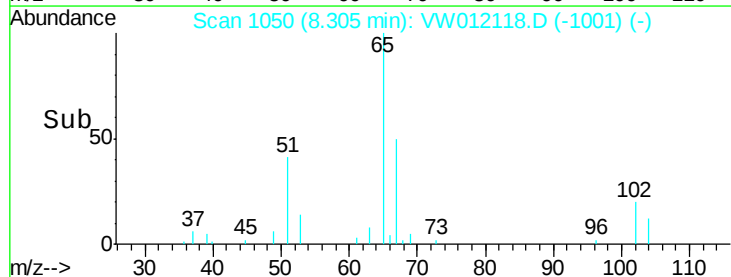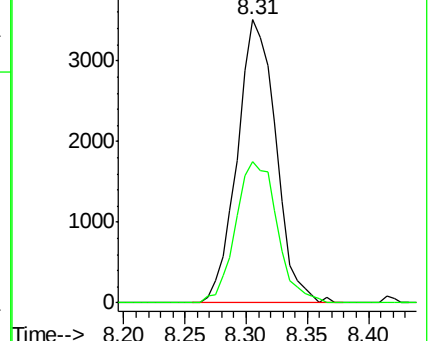


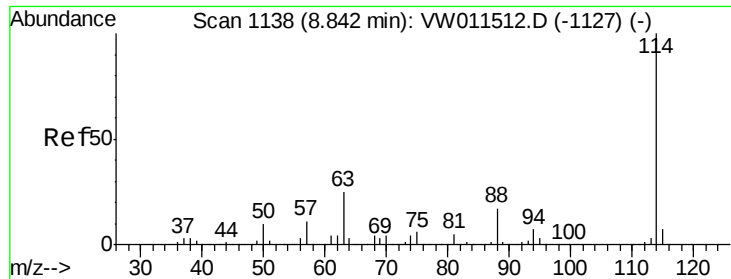




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW012118.D
 Acq: 22 Aug 2019 18:26

Instrument :
 MSVOA_W
 ClientSampled :
 SB-09-5.5-6.0

Tot Ion:114 Resp: 20243
 Ion Ratio Lower Upper
 114 100
 63 25.5 0.0 49.2
 88 16.4 0.0 33.8

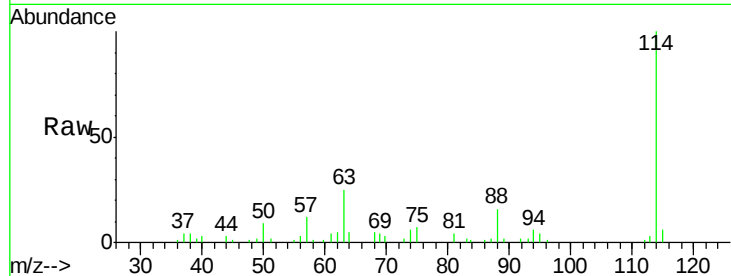


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

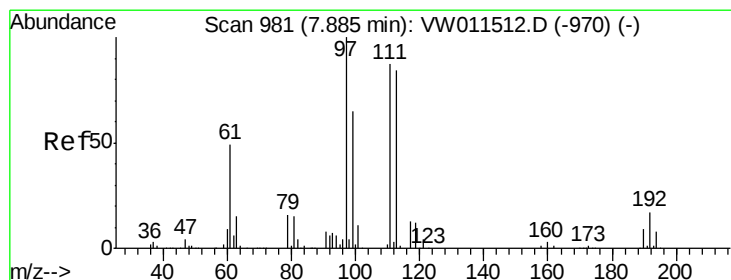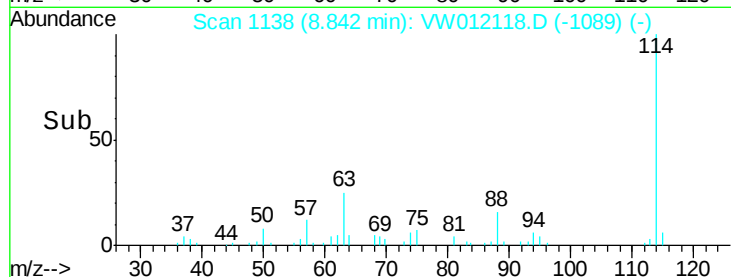
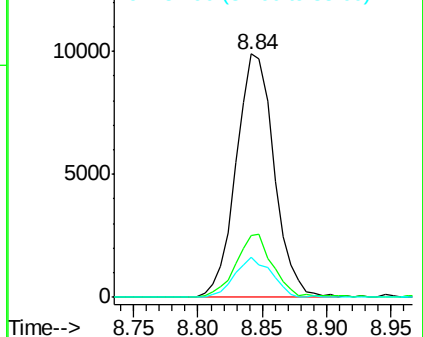



#35
 Dibromofluoromethane
 Concen: 57.807 ug/l
 RT: 7.89 min Scan# 982
 Delta R.T. 0.01 min
 Lab File: VW012118.D
 Acq: 22 Aug 2019 18:26

Tgt Ion:113 Resp: 6565
 Ion Ratio Lower Upper
 113 100
 111 103.0 82.7 124.1
 192 21.9 16.1 24.1

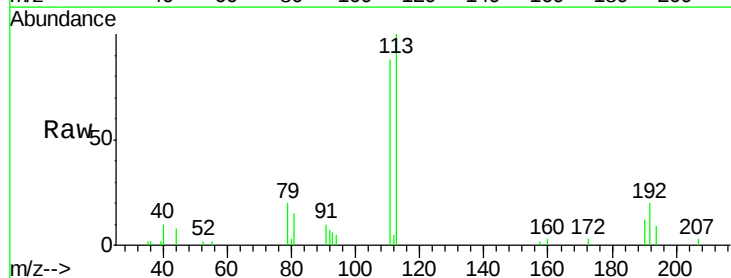

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

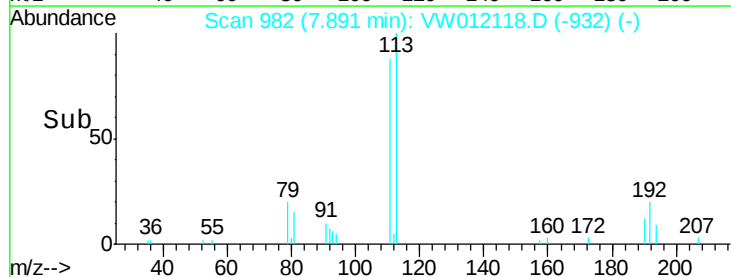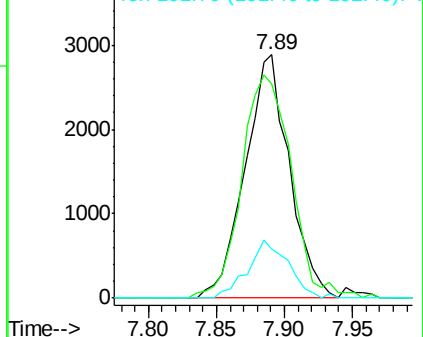

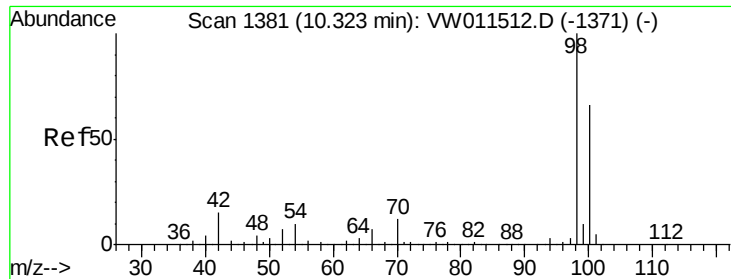

#50

Toluene-d8

Concen: 50.960 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW012118.D

Acq: 22 Aug 2019 18:26

Instrument :

MSVOA_W

ClientSampleId :





SB-09-5.5-6.0

Tot Ion: 98 Resp: 23695

Ion Ratio Lower Upper

98 100

100 62.7 52.7 79.1

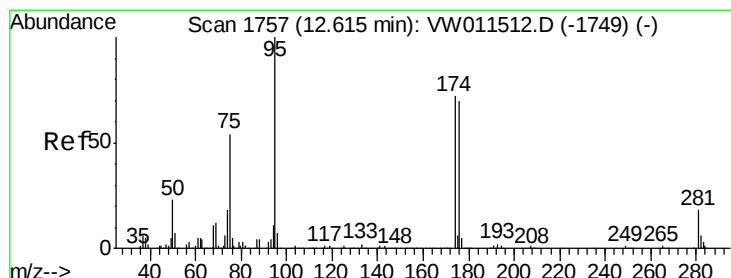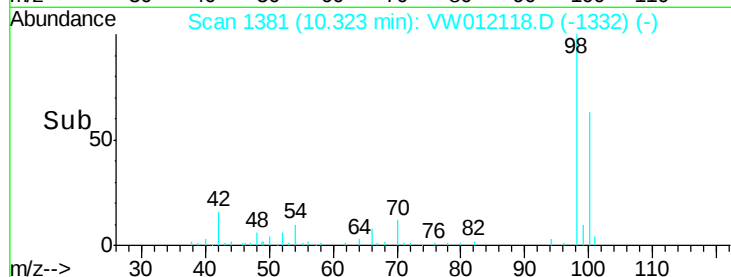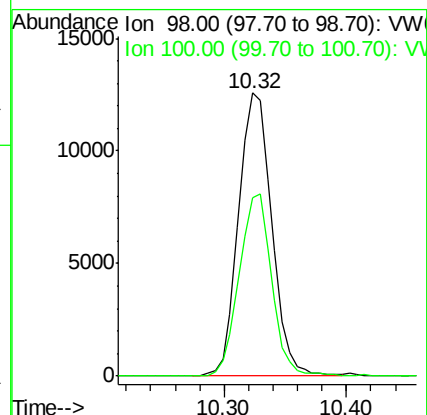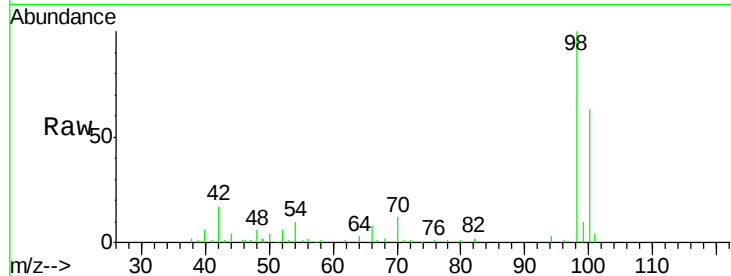

#62

4-Bromofluorobenzene

Concen: 29.076 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.01 min

Lab File: VW012118.D

Acq: 22 Aug 2019 18:26




Tgt Ion: 95 Resp: 4820


Ion Ratio Lower Upper

95 100

174 75.8 0.0 150.2

176 72.3 0.0 144.4


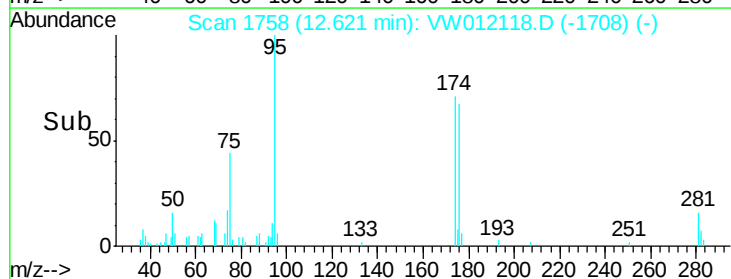
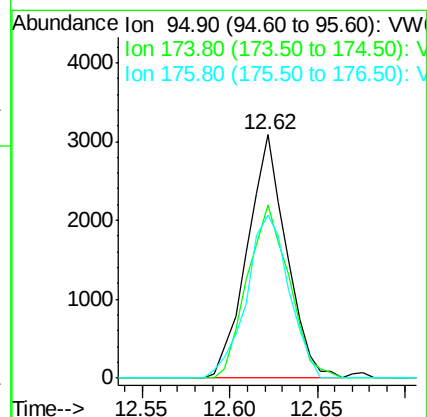
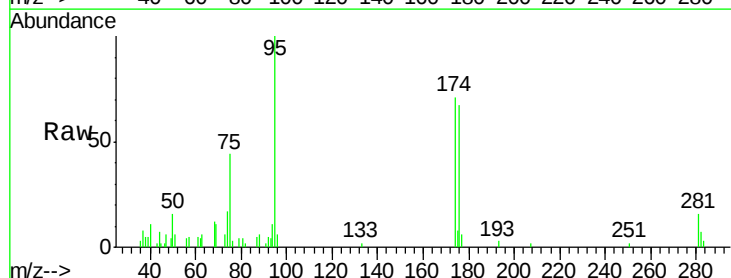


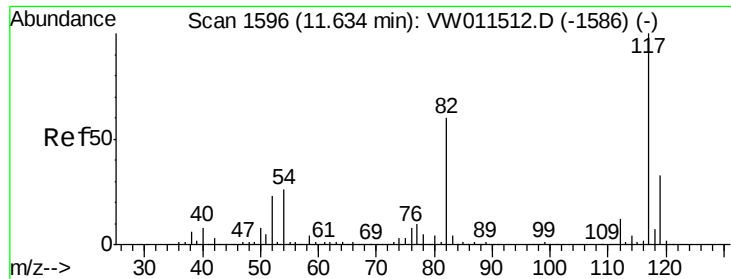

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW012118.D
Acq: 22 Aug 2019 18:26

Instrument :
MSVOA_W
ClientSampleId :
SB-09-5.5-6.0

Tot Ion:117 Resp: 14538
Ion Ratio Lower Upper
117 100
82 54.6 47.9 71.9
119 29.6 26.2 39.2

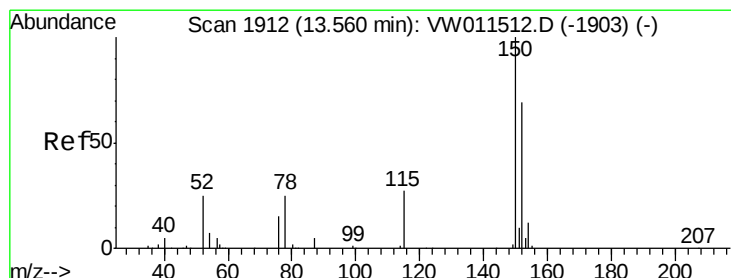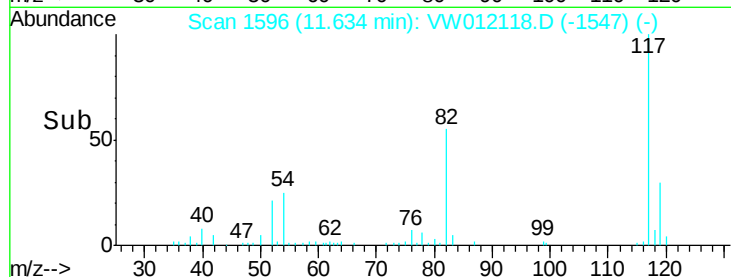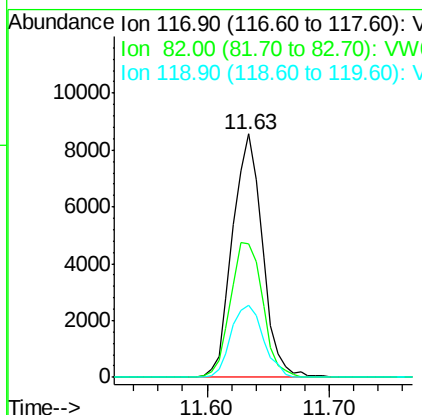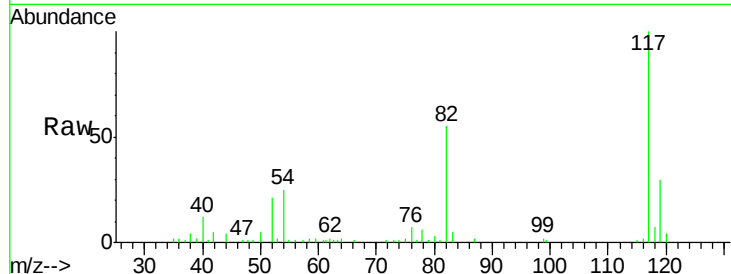

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW012118.D
Acq: 22 Aug 2019 18:26

Tgt Ion:152 Resp: 2620
Ion Ratio Lower Upper
152 100
115 55.1 30.5 91.5
150 144.4 0.0 352.6

