


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW082220\
Data File : VW016296.D
Acq On : 21 Aug 2020 08:49
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081420S.M
Title : SW846 8260
Last Update : Mon Aug 17 08:01:41 2020

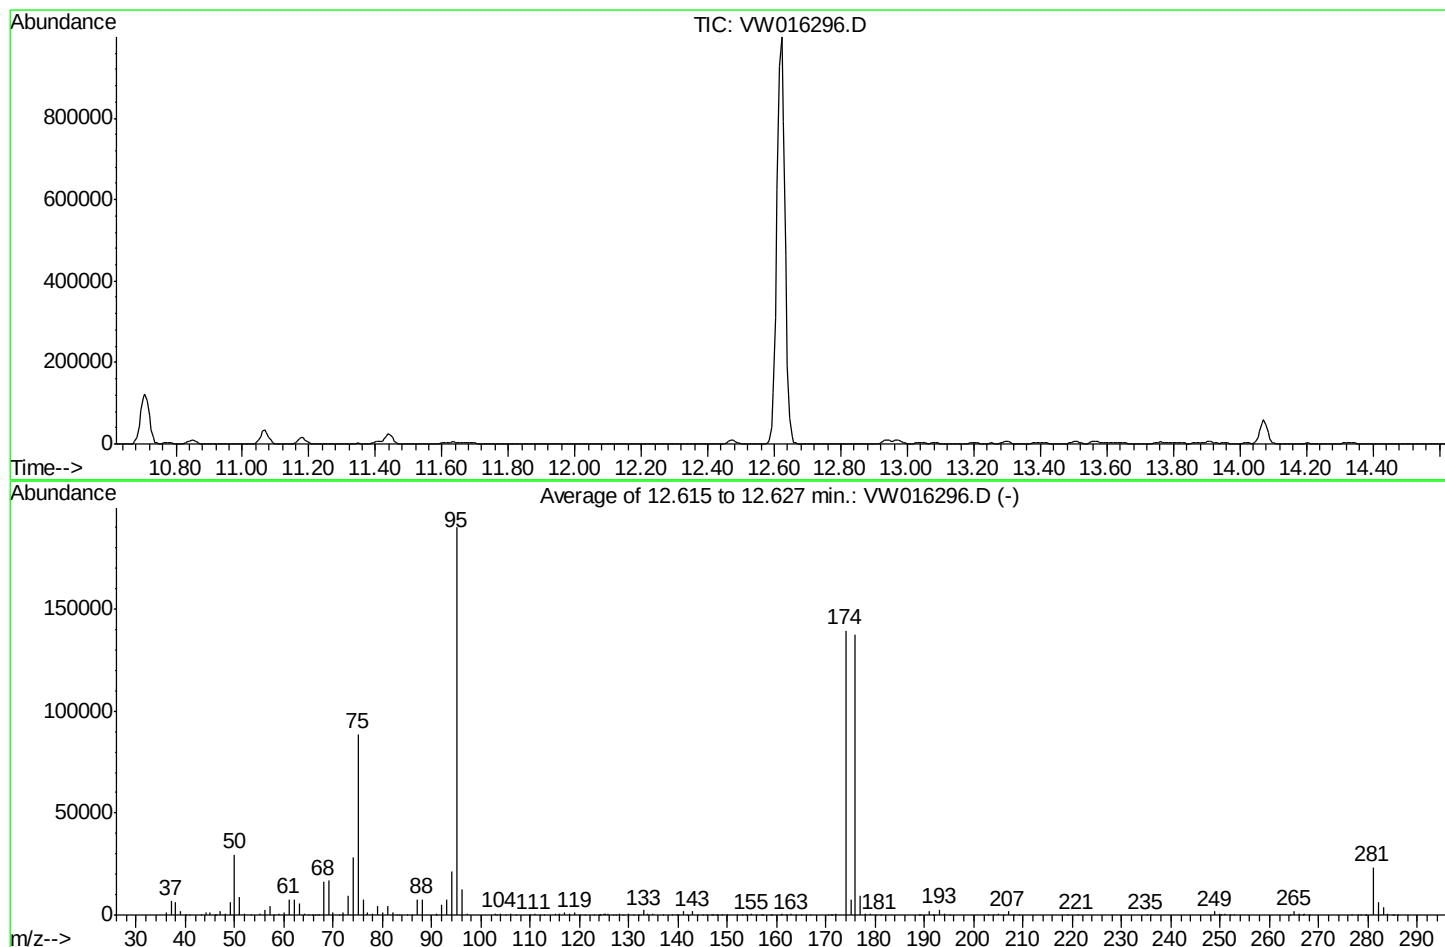

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	29570	PASS
75	95	30	60	46.7	88808	PASS
95	95	100	100	100.0	190208	PASS
96	95	5	9	6.5	12403	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.4	139584	PASS
175	174	5	9	5.5	7728	PASS
176	174	95	101	98.6	137672	PASS
177	176	5	9	6.8	9337	PASS