

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082318\
 Data File : VW004919.D
 Acq On : 24 Aug 2018 01:58
 Operator : SY/AP
 Sample : J4628-13
 Misc : 6.03G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 24 07:20:08 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 07:12:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	668140	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	717173	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	301892	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	294843	23.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.40%
7) Chloroethane-d5	2.89	69	233006	24.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.56%
10) 1,1-Dichloroethene-d2	4.02	63	296141	18.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.44%
20) 2-Butanone-d5	7.09	46	96303	37.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.94%
24) Chloroform-d	7.65	84	396071	26.70	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	8.31	65	218412	27.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.40%
29) Benzene-d6	8.28	84	860325	23.32	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.28%
33) 1,2-Dichloropropane-d6	9.28	67	262807	24.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.00%
37) Toluene-d8	10.33	98	910116	23.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.16%
38) trans-1,3-Dichloropropene-	10.58	79	100282	21.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.00%
39) 2-Hexanone-d5	10.93	63	96912	36.09	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.18%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	240685	22.10	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	318560	26.27	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.08%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.56	75	33308	3.863 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW082318\
Data File : VW004919.D
Acq On : 24 Aug 2018 01:58
Operator : SY/AP
Sample : J4628-13
Misc : 6.03G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 24 07:20:08 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 07:12:16 2018
Response via : Initial Calibration

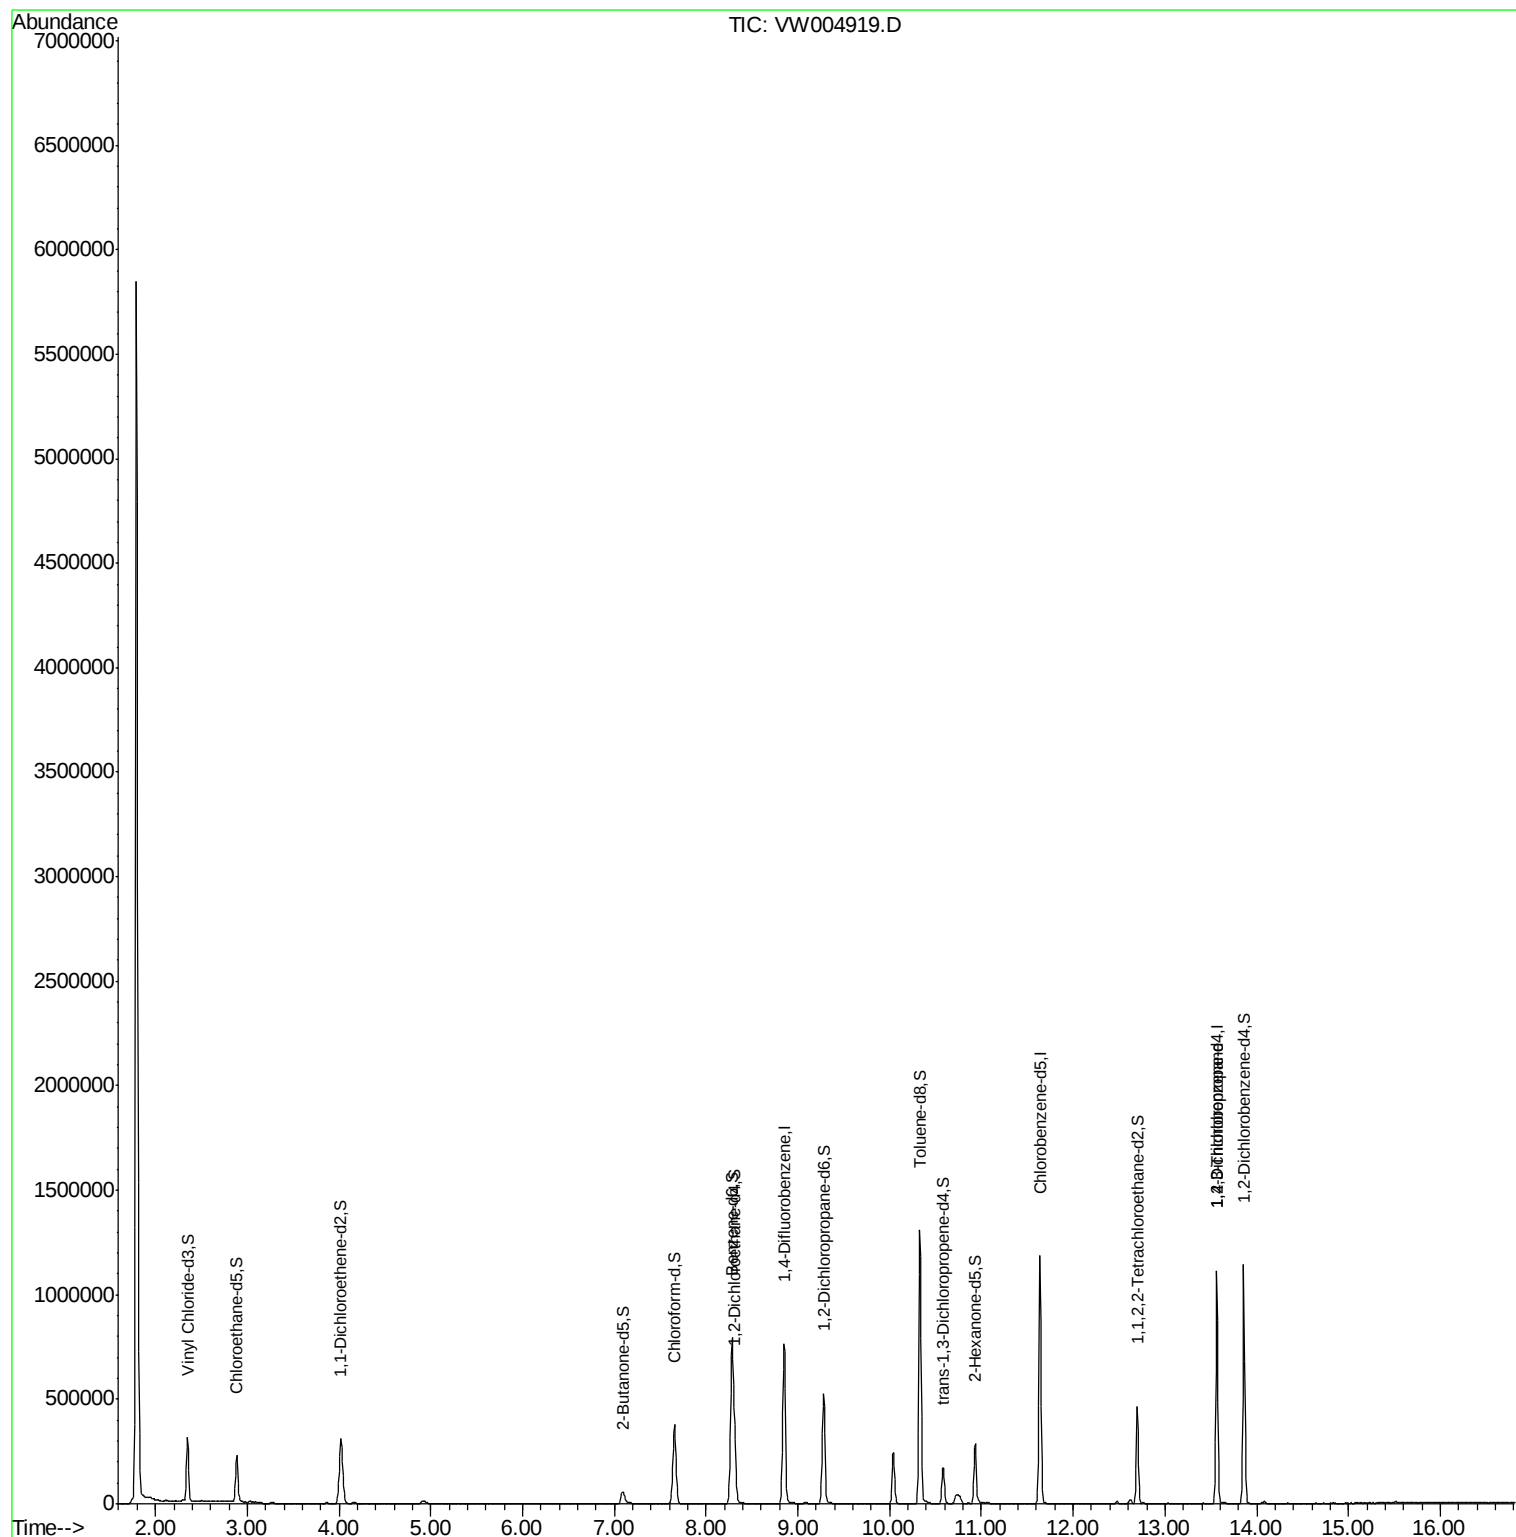

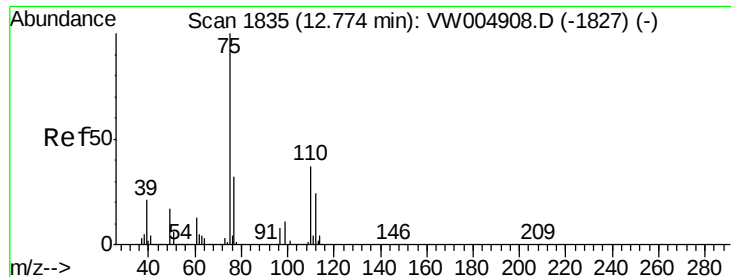

#59

1,2,3-Trichloropropane

Concen: 3.863 ug/L

RT: 13.56 min Scan# 1964

Delta R.T. 0.79 min

Lab File: VW004919.D

Acq: 24 Aug 2018 01:58

Instrument :

MSVOA_W


ClientSampleId :

Tot Ion: 75 Resp: 33308

Ion Ratio Lower Upper

75 100

77 37.0 25.3 37.9

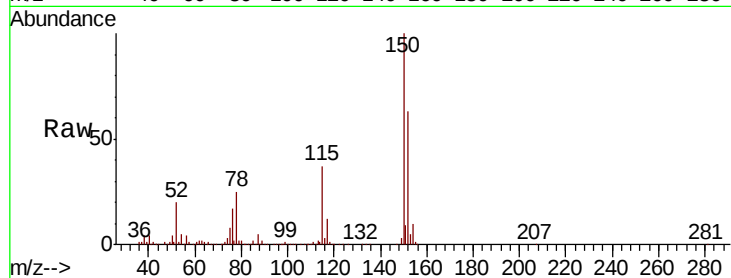

Abundance Ion 75.00 (74.70 to 75.70): VW

Ion 77.00 (76.70 to 77.70): VW

