

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082318\
 Data File : VW004934.D
 Acq On : 24 Aug 2018 14:17
 Operator : SY/AP
 Sample : J4634-08
 Misc : 6.85G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB3J4

Quant Time: Aug 24 23:10:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 08:18:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	681673	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	726399	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	332270	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	274582	21.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.24%
7) Chloroethane-d5	2.89	69	214520	22.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.84%
10) 1,1-Dichloroethene-d2	4.03	63	289521	17.60	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.40%
20) 2-Butanone-d5	7.09	46	93929	35.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.64%
24) Chloroform-d	7.66	84	371809	24.57	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.28%
26) 1,2-Dichloroethane-d4	8.31	65	199988	24.32	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.28%
29) Benzene-d6	8.28	84	820088	21.95	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.80%
33) 1,2-Dichloropropane-d6	9.28	67	249300	22.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.84%
37) Toluene-d8	10.33	98	879670	22.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.88%
38) trans-1,3-Dichloropropene-	10.59	79	99214	21.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.00%
39) 2-Hexanone-d5	10.93	63	92279	33.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.86%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	213329	19.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.36%
61) 1,2-Dichlorobenzene-d4	13.86	152	329129	24.66	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.64%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.15	43	10726	5.281	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW082318\
Data File : VW004934.D
Acq On : 24 Aug 2018 14:17
Operator : SY/AP
Sample : J4634-08
Misc : 6.85G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB3J4

Quant Time: Aug 24 23:10:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 08:18:56 2018
Response via : Initial Calibration

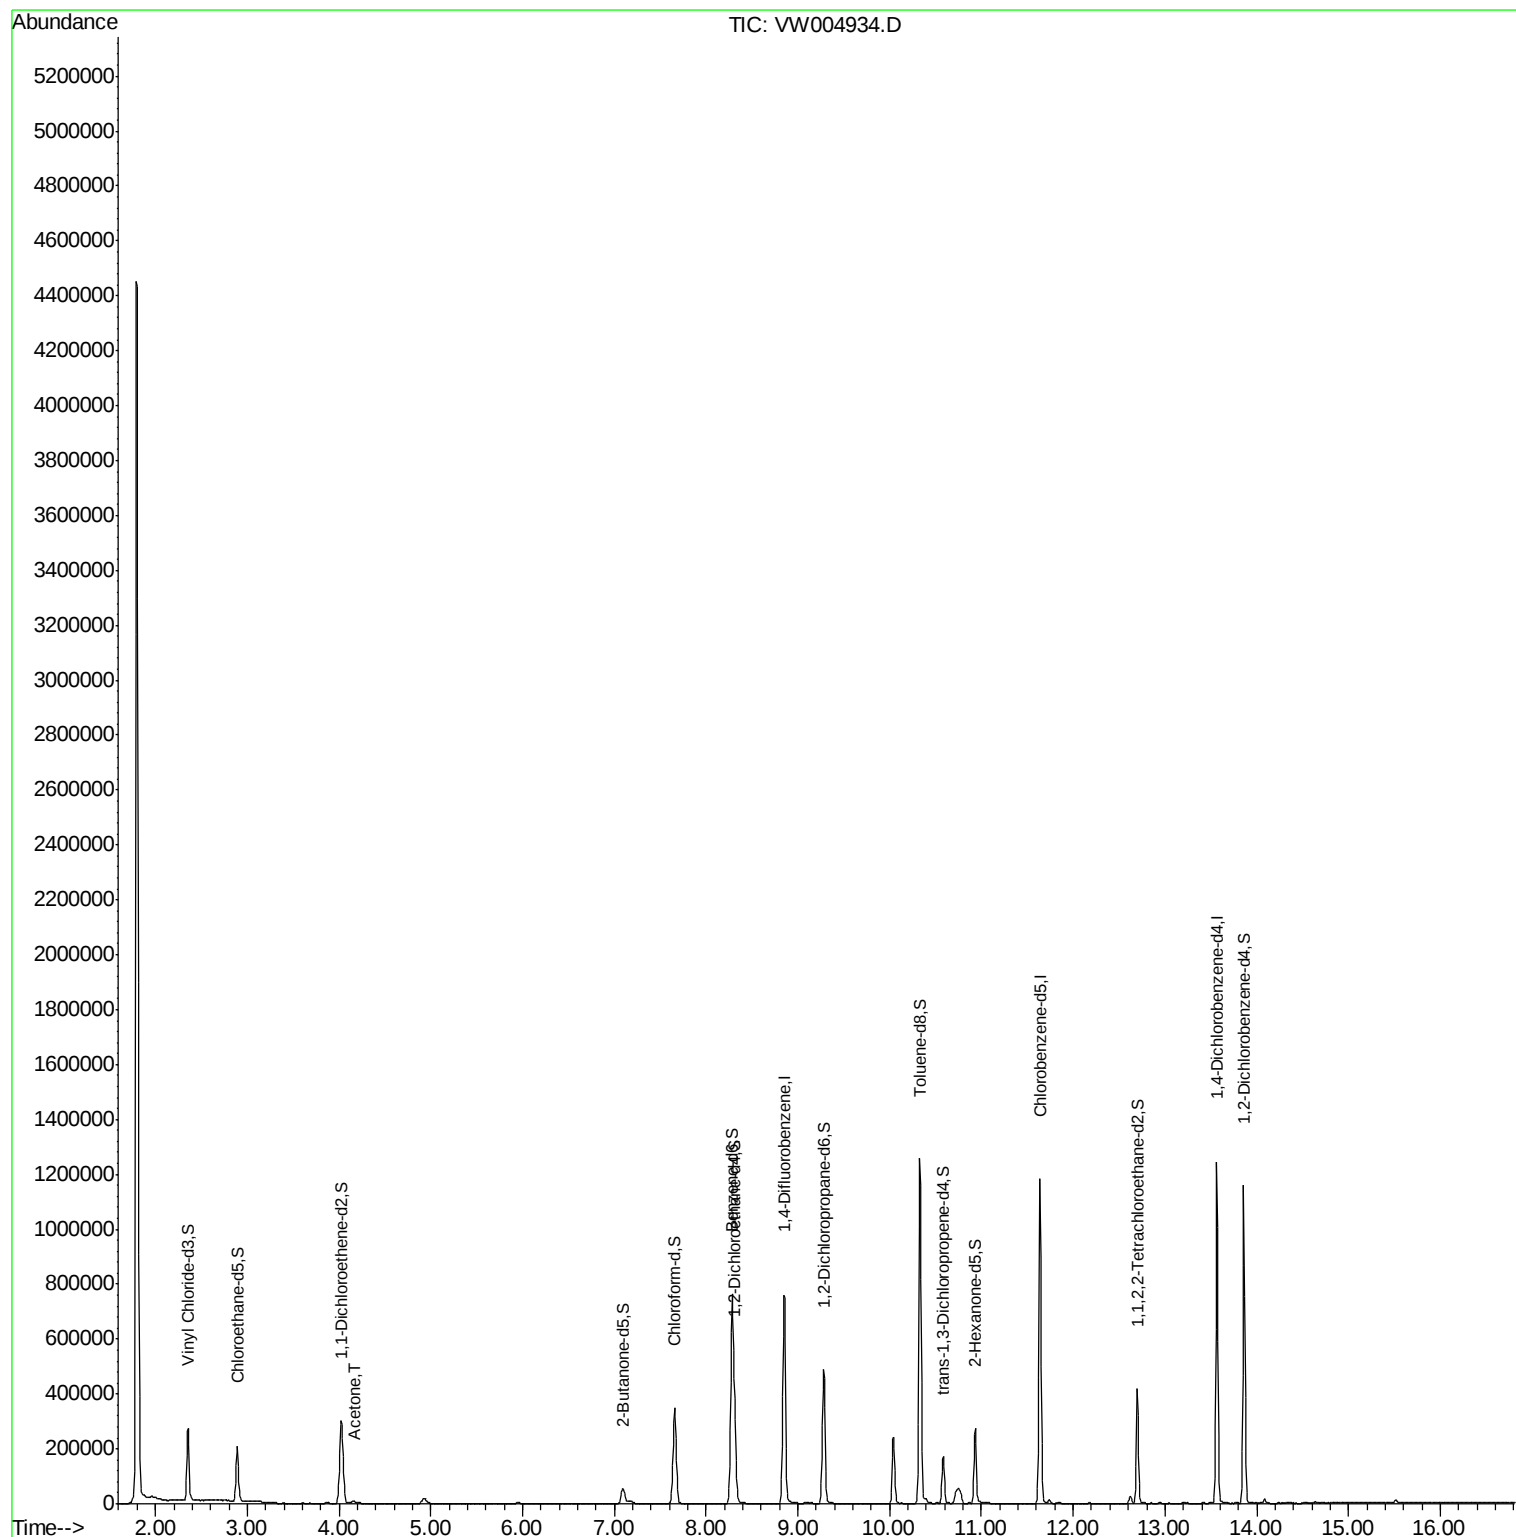

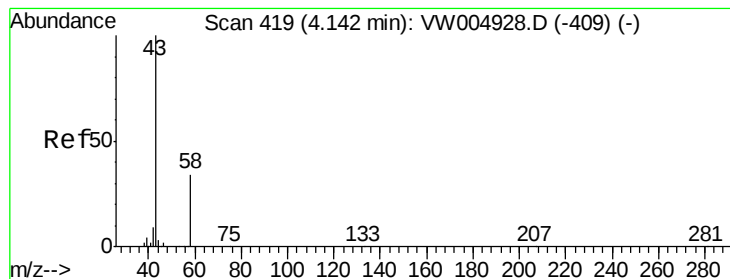

#13
 Acetone
 Concen: 5.281 ug/L
 RT: 4.15 min Scan# 421
 Delta R.T. 0.01 min
 Lab File: VW004934.D
 Acq: 24 Aug 2018 14:17

Instrument :
 MSVOA_W
 ClientSampleId :
 DB3J4

Tgt Ion: 43 Resp: 10726
 Ion Ratio Lower Upper
 43 100
 58 33.2 0.0 69.4

