

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082318\
 Data File : VW004935.D
 Acq On : 24 Aug 2018 14:43
 Operator : SY/AP
 Sample : J4634-09
 Misc : 6.92G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB3J5

Quant Time: Aug 24 23:10:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 08:18:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	722582	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	752694	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	312846	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	274635	20.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.44%
7) Chloroethane-d5	2.89	69	216382	21.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.48%
10) 1,1-Dichloroethene-d2	4.03	63	279555	16.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.12%
20) 2-Butanone-d5	7.09	46	88081	31.69	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.38%
24) Chloroform-d	7.65	84	360154	22.45	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	8.31	65	193929	22.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.00%
29) Benzene-d6	8.28	84	794174	20.51	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.04%
33) 1,2-Dichloropropane-d6	9.28	67	238952	21.01	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.04%
37) Toluene-d8	10.33	98	841753	20.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.08%
38) trans-1,3-Dichloropropene-	10.59	79	92324	18.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.44%
39) 2-Hexanone-d5	10.93	63	85724	30.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.84%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	200514	17.54	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	70.16%
61) 1,2-Dichlorobenzene-d4	13.86	152	281193	22.38	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.52%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.15	43	8196	3.807	ug/L	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW082318\
Data File : VW004935.D
Acq On : 24 Aug 2018 14:43
Operator : SY/AP
Sample : J4634-09
Misc : 6.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB3J5

Quant Time: Aug 24 23:10:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 08:18:56 2018
Response via : Initial Calibration

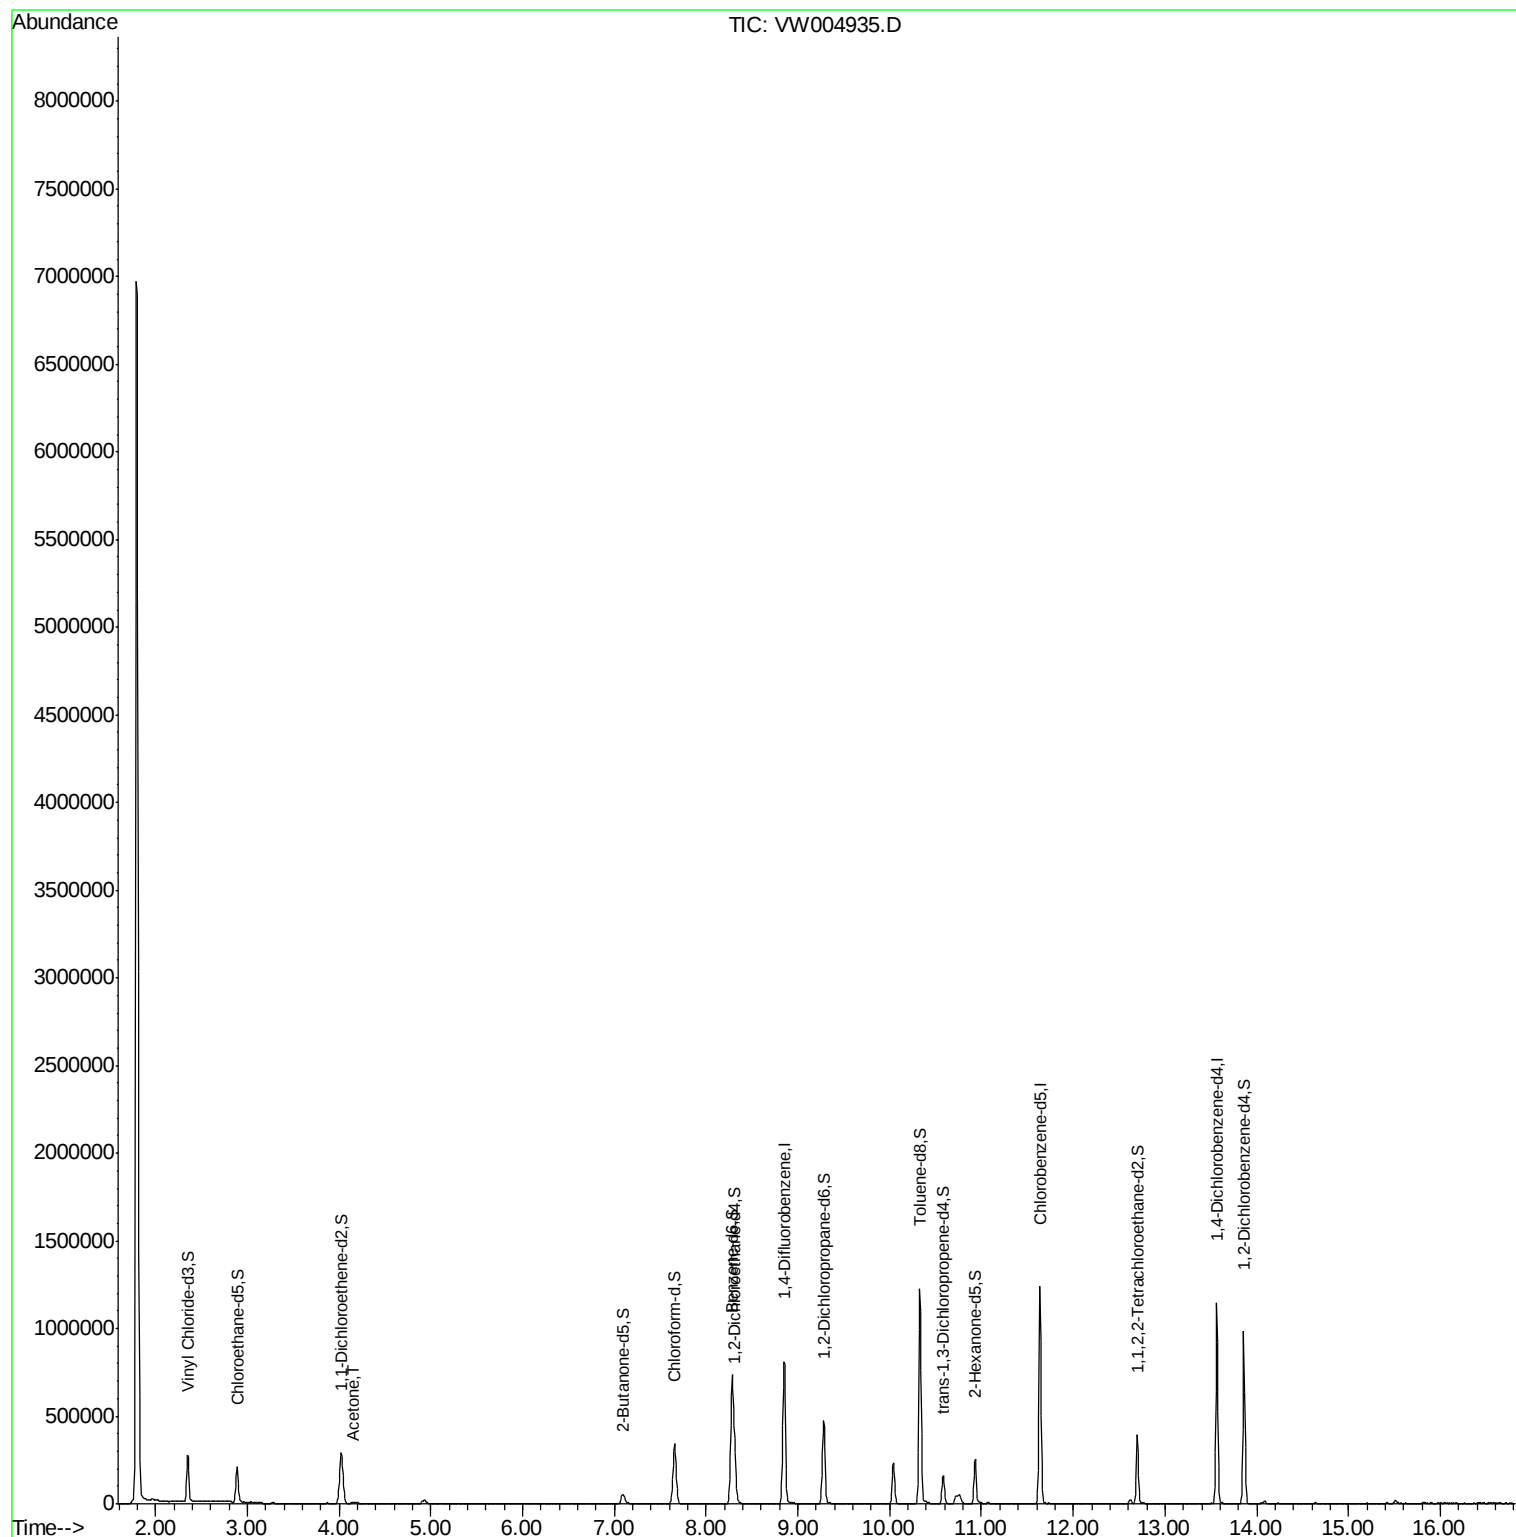

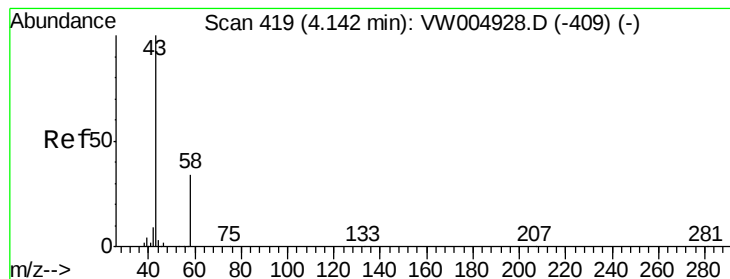

#13
 Acetone
 Concen: 3.807 ug/L
 RT: 4.15 min Scan# 420
 Delta R.T. 0.01 min
 Lab File: VW004935.D
 Acq: 24 Aug 2018 14:43

Instrument :
 MSVOA_W
 ClientSampleId :
 DB3J5

Tgt Ion: 43 Resp: 8196
 Ion Ratio Lower Upper
 43 100
 58 18.2 0.0 69.4

