

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082318\
 Data File : VW004936.D
 Acq On : 24 Aug 2018 15:08
 Operator : SY/AP
 Sample : J4624-08
 Misc : 5.66G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E4434

Quant Time: Aug 24 23:10:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 08:18:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	664160	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	731282	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	346749	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	277889	22.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.56%
7) Chloroethane-d5	2.89	69	215998	23.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.84%
10) 1,1-Dichloroethene-d2	4.25	63	110	0.01	ug/L	0.23
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.04%#
20) 2-Butanone-d5	7.09	46	82881	32.44	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.88%
24) Chloroform-d	7.65	84	362010	24.55	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.20%
26) 1,2-Dichloroethane-d4	8.31	65	190275	23.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.00%
29) Benzene-d6	8.28	84	805477	21.41	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.64%
33) 1,2-Dichloropropane-d6	9.28	67	237157	21.46	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.84%
37) Toluene-d8	10.33	98	877553	22.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.08%
38) trans-1,3-Dichloropropene-	10.59	79	93456	19.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.60%
39) 2-Hexanone-d5	10.93	63	79439	29.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.02%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	200373	18.04	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	72.16%
61) 1,2-Dichlorobenzene-d4	13.86	152	338699	24.32	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.28%


Target Compounds					Qvalue
13) Acetone	4.15	43	6785	3.429 ug/L	68
16) Methylene chloride	4.93	84	44210	3.433 ug/L	92
59) 1,2,3-Trichloropropane	13.57	75	37411	4.255 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW082318\
Data File : VW004936.D
Acq On : 24 Aug 2018 15:08
Operator : SY/AP
Sample : J4624-08
Misc : 5.66G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E4434

Quant Time: Aug 24 23:10:17 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 08:18:56 2018
Response via : Initial Calibration




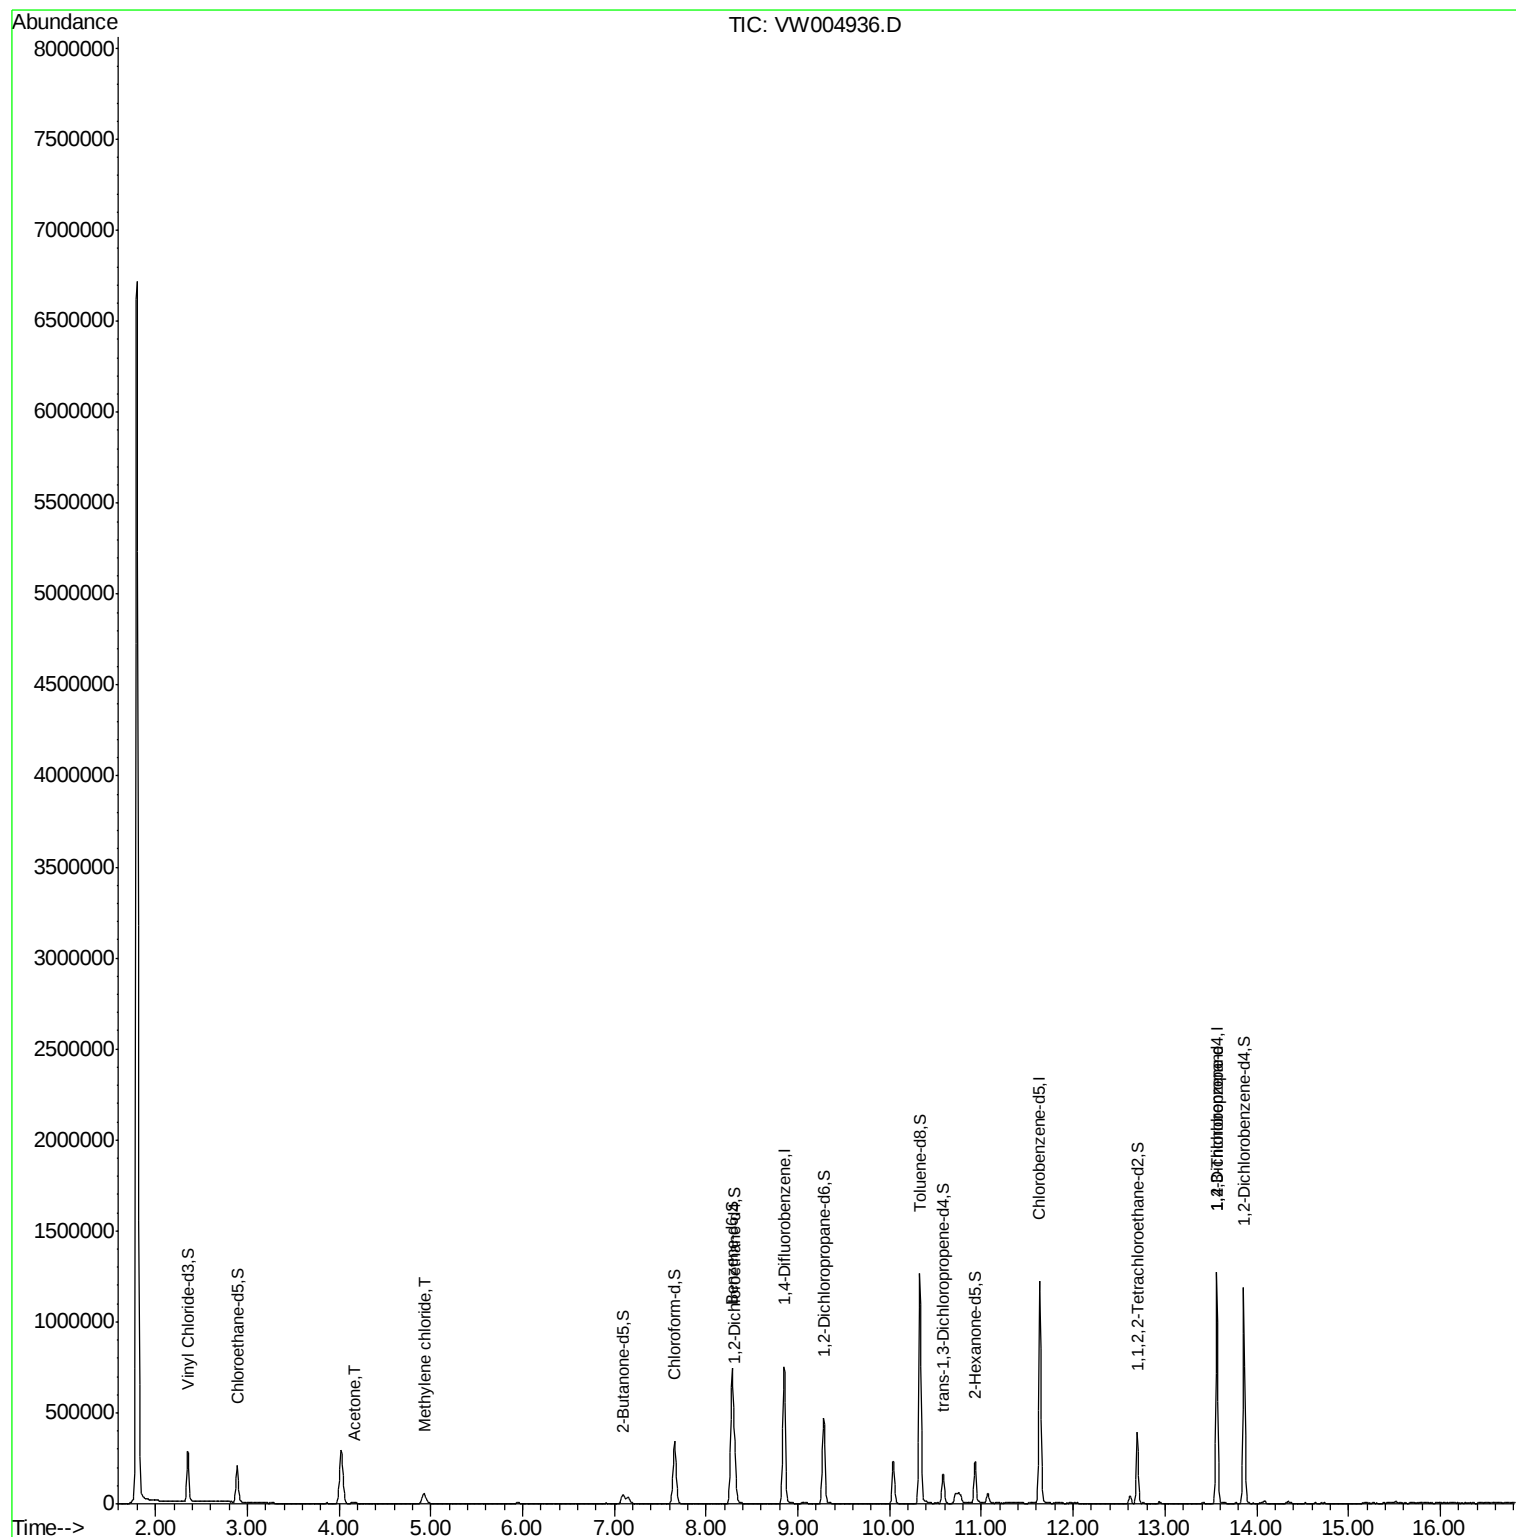


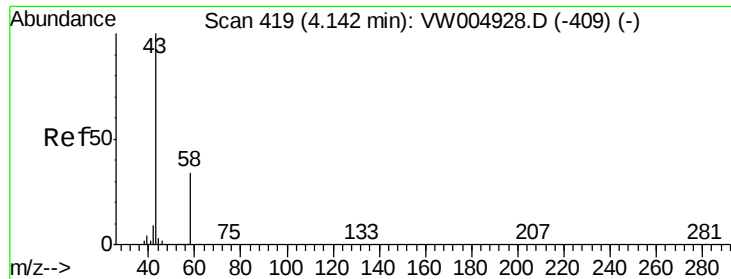

#13
Acetone
Concen: 3.429 ug/L
RT: 4.15 min Scan# 421
Delta R.T. 0.01 min
Lab File: VW004936.D
Acq: 24 Aug 2018 15:08




Instrument :
MSVOA_W
ClientSampleId :
E4434


Tgt Ion: 43 Resp: 6785
Ion Ratio Lower Upper
43 100
58 16.2 0.0 69.4

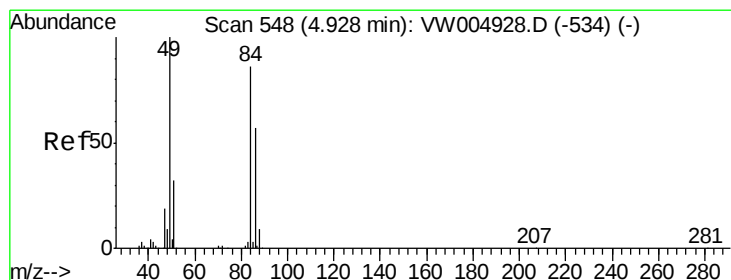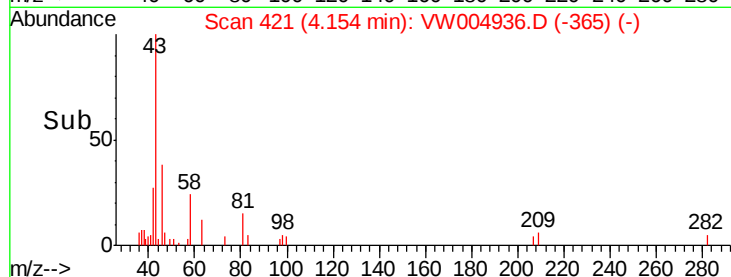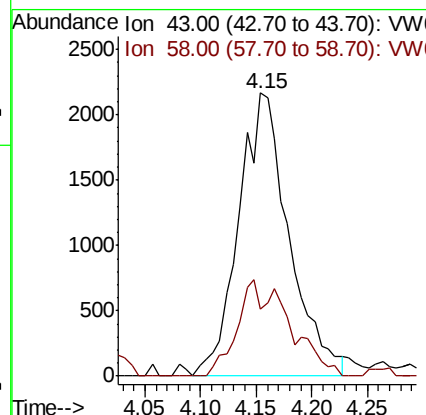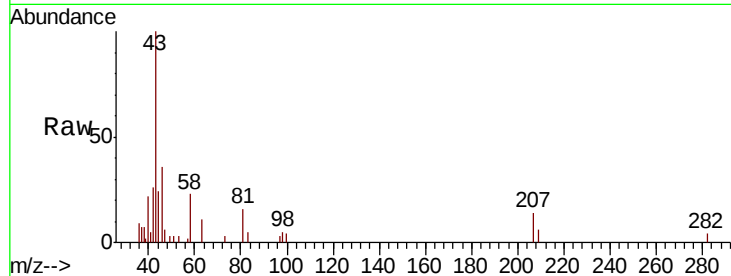

#16
Methylene chloride
Concen: 3.433 ug/L
RT: 4.93 min Scan# 548
Delta R.T. 0.00 min
Lab File: VW004936.D
Acq: 24 Aug 2018 15:08

Tgt Ion: 84 Resp: 44210
Ion Ratio Lower Upper
84 100
49 108.7 83.8 155.6
86 58.6 42.6 79.0

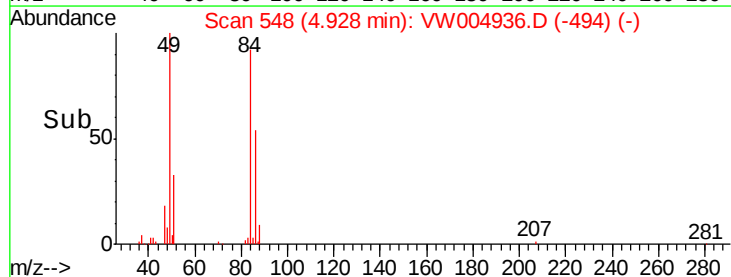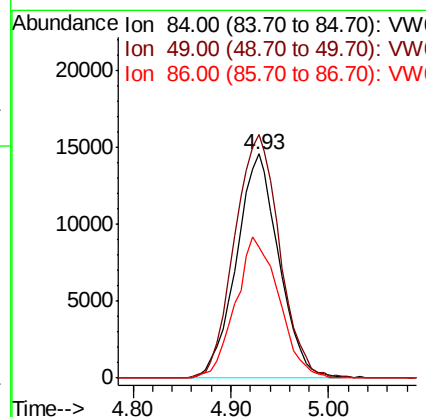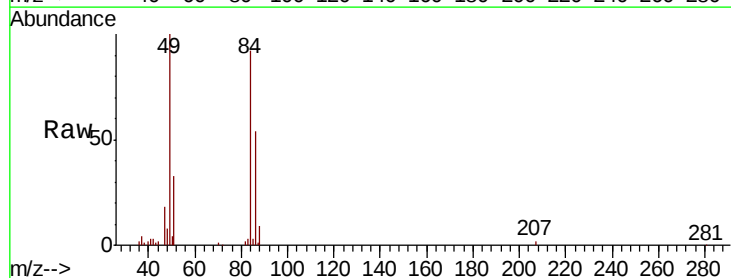

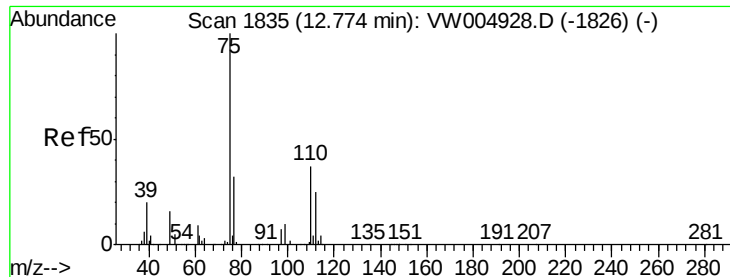

#59

1,2,3-Trichloropropane

Concen: 4.255 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW004936.D

Acq: 24 Aug 2018 15:08

Instrument :

MSVOA_W

ClientSampleId :

E4434

Tgt Ion: 75 Resp: 37411

Ion Ratio Lower Upper

75 100

77 37.3 25.3 37.9

