


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082318\
Data File : VW004894.D
Acq On : 23 Aug 2018 13:40
Operator : SY/AP
Sample : J4624-02
Misc : 6.22G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E4428

Manual Integrations
APPROVED

MMDadoda
8/27/2018 1:45:22 PM

Quant Time: Aug 24 05:18:07 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 05:01:02 2018
Response via : Initial Calibration

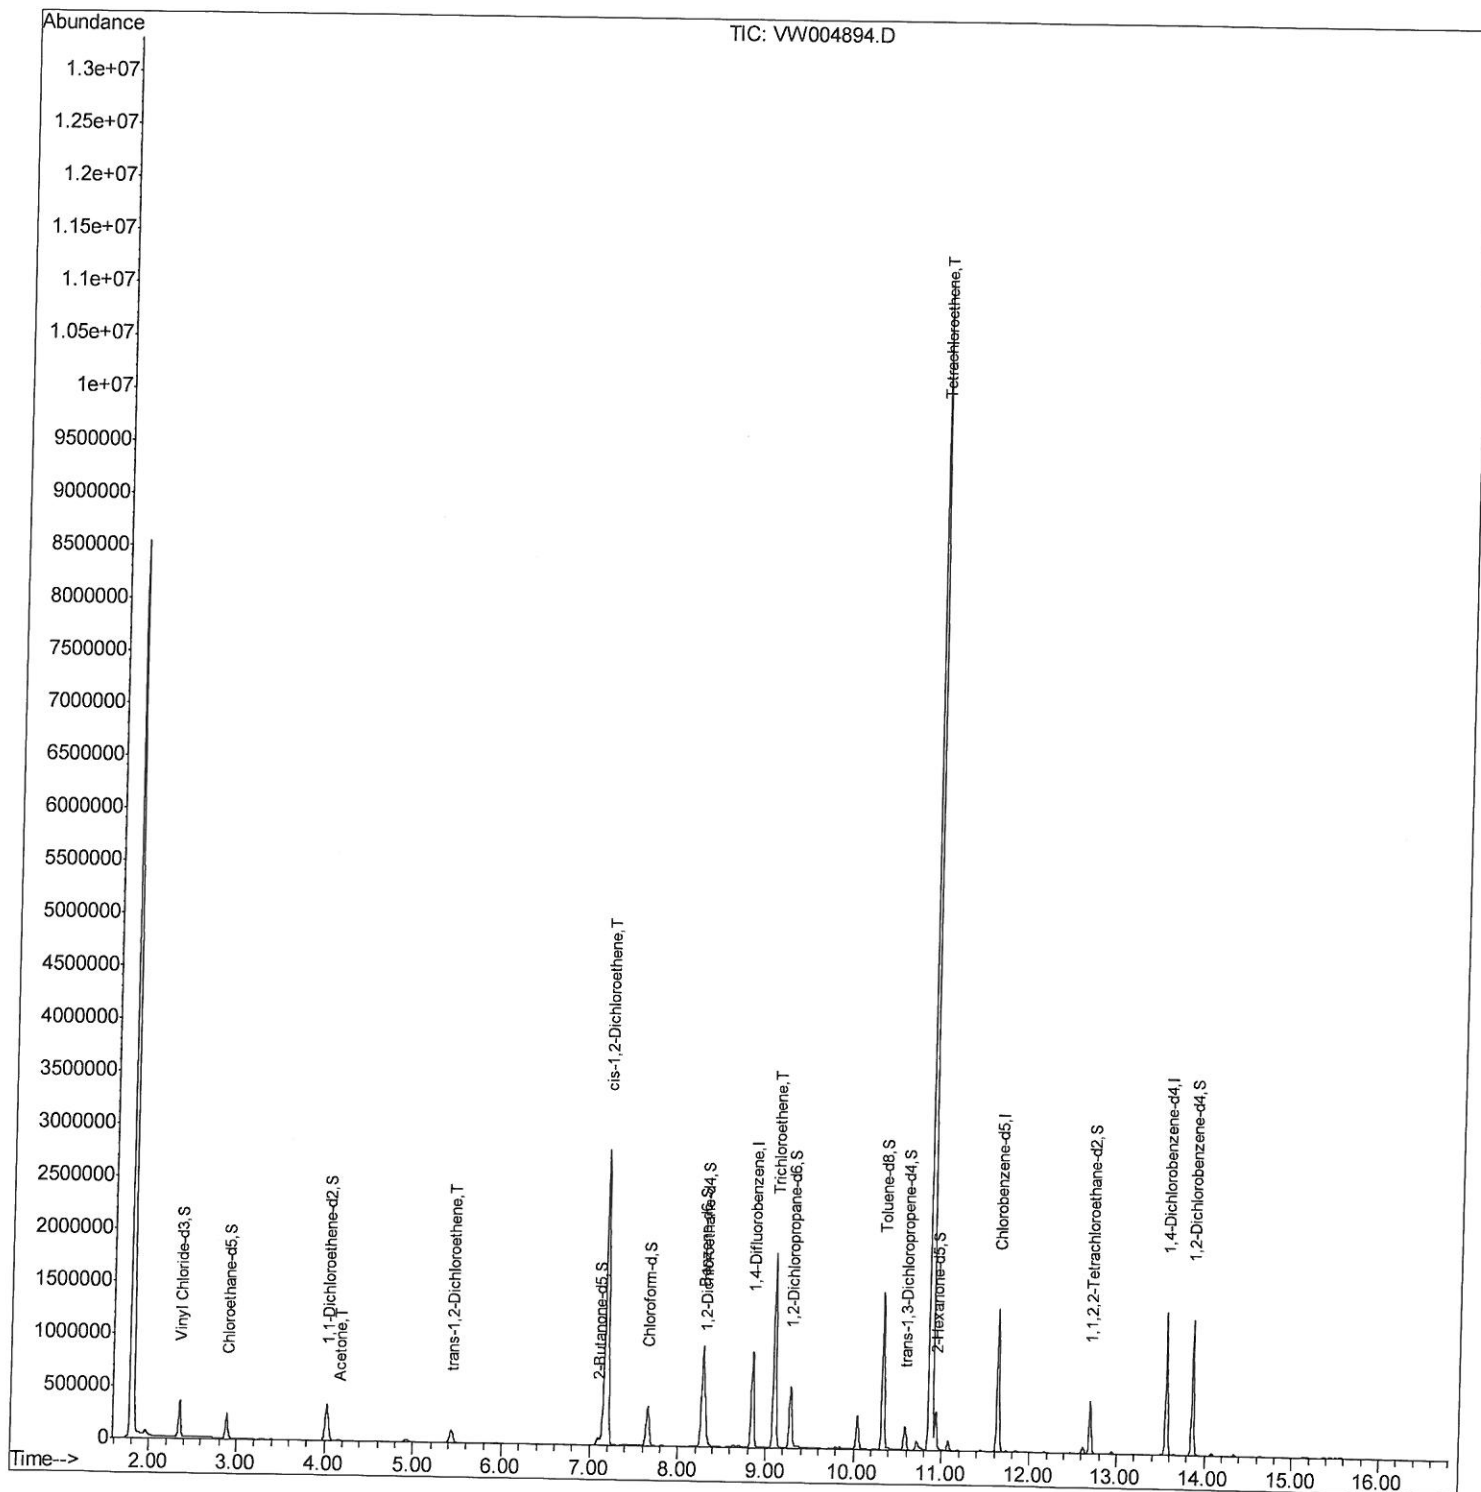

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082318\
 Data File : VW004894.D
 Acq On : 23 Aug 2018 13:40
 Operator : SY/AP
 Sample : J4624-02
 Misc : 6.22G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 E4428

Manual Integrations
APPROVED

MMDadoda
 8/27/2018 1:45:22 PM

Quant Time: Aug 24 05:01:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 05:01:02 2018
 Response via : Initial Calibration

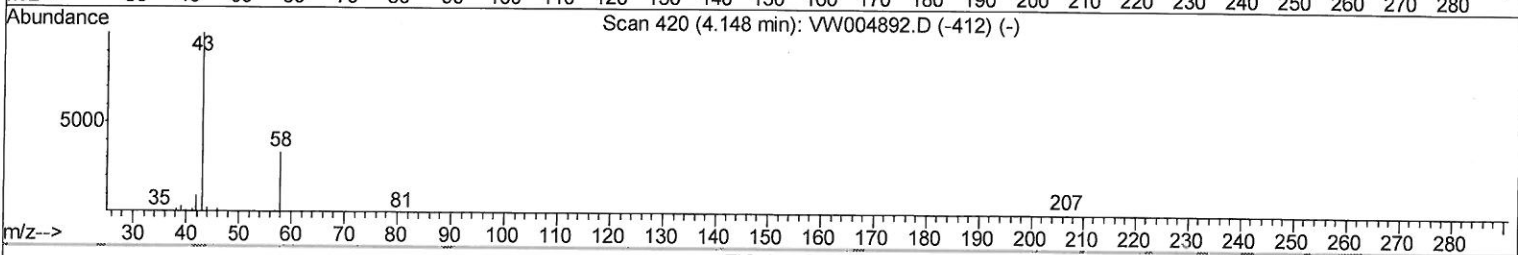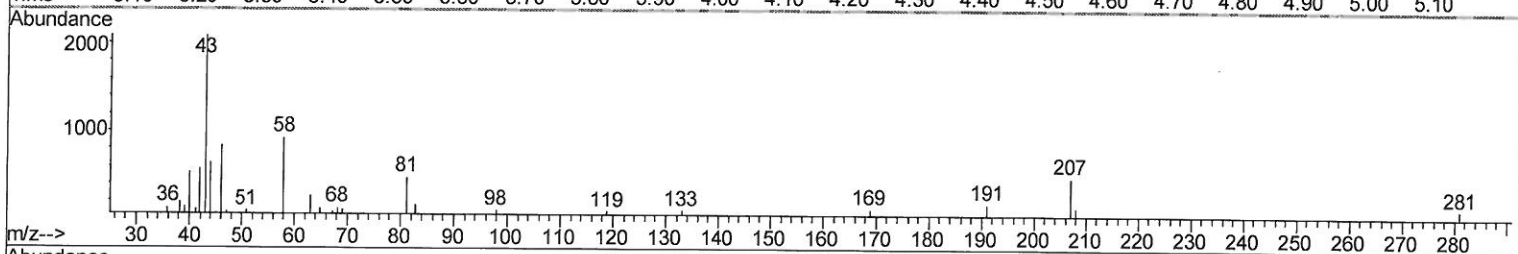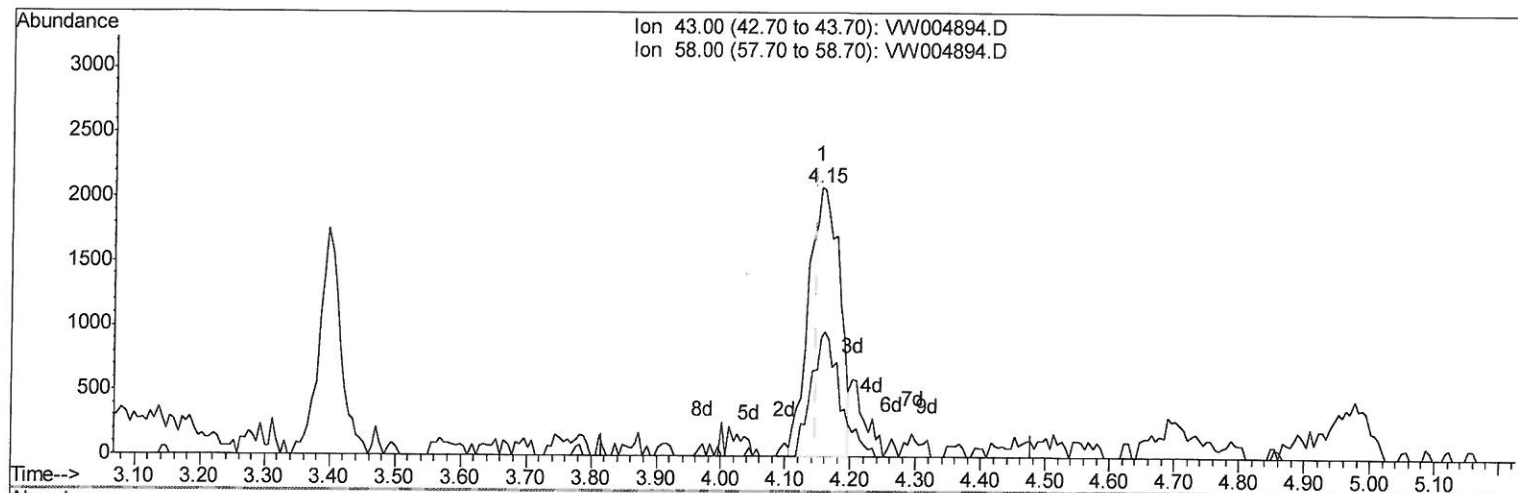

TIC: VW004894.D

(13) Acetone (T)

4.153min (+0.006) 2.80ug/L

response 6904

Ion	Exp%	Act%
43.00	100	100
58.00	34.70	43.53
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082318\
Data File : VW004894.D
Acq On : 23 Aug 2018 13:40
Operator : SY/AP
Sample : J4624-02
Misc : 6.22G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E4428

Manual Integrations
APPROVED

MMDadoda
8/27/2018 1:45:22 PM

Quant Time: Aug 24 05:01:45 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 05:01:02 2018
Response via : Initial Calibration

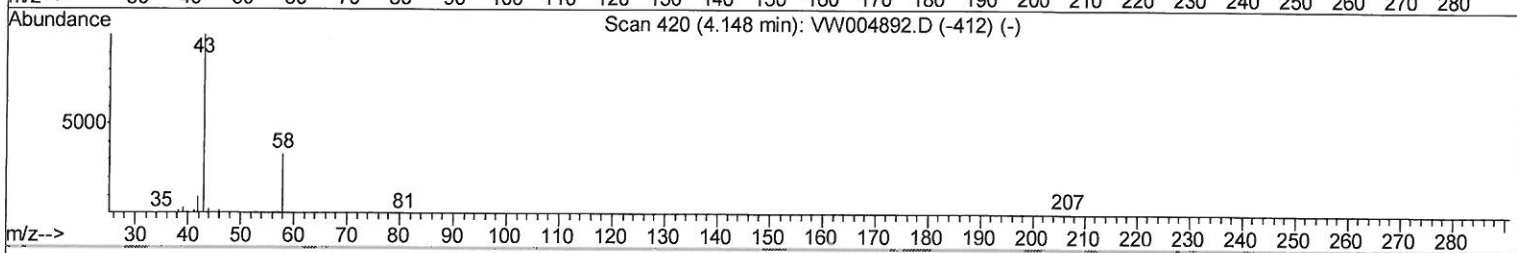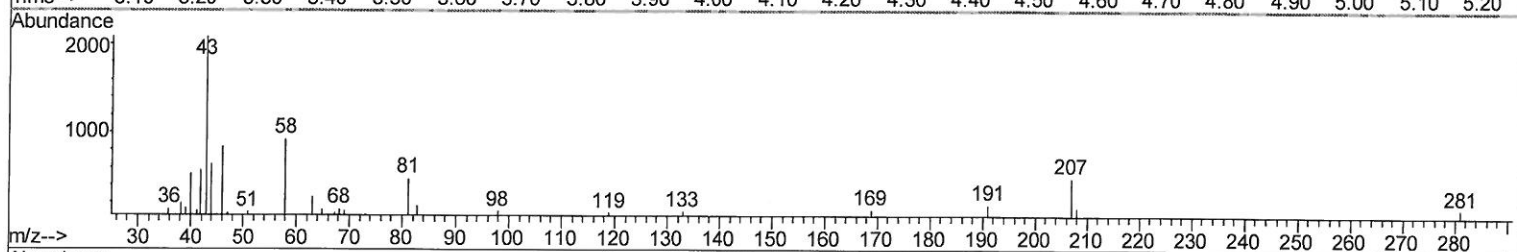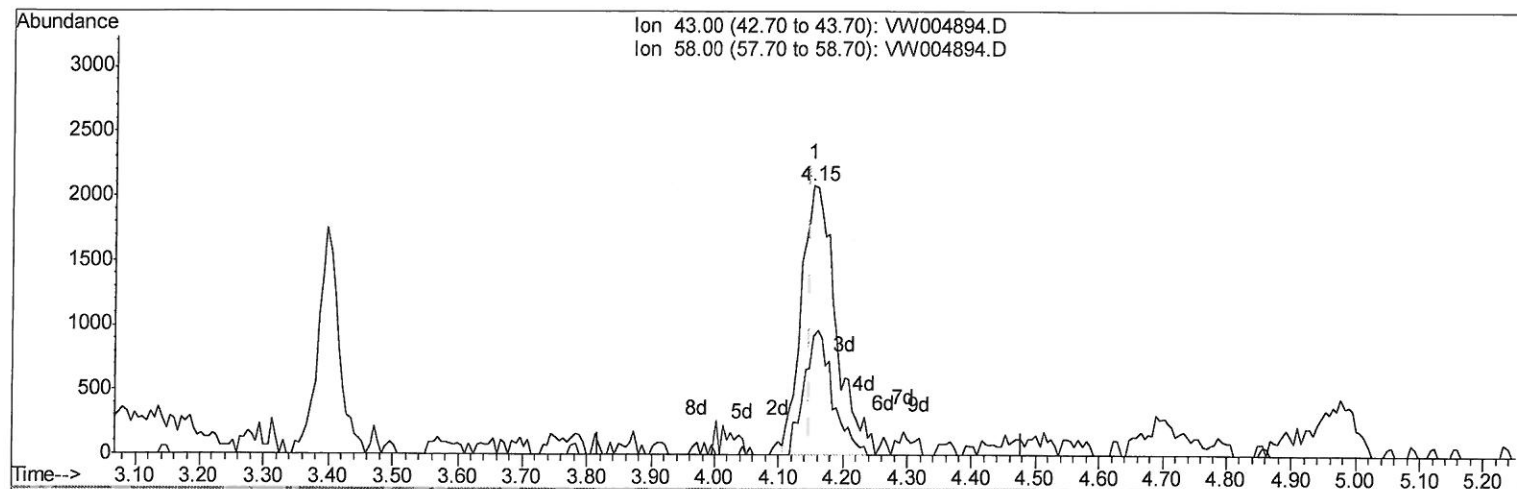

TIC: VW004894.D

(13) Acetone (T)

4.153min (+0.006) 3.18ug/L m

response 7854

Ion	Exp%	Act%
43.00	100	100
58.00	34.70	38.26
0.00	0.00	0.00
0.00	0.00	0.00

08/29/18 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082318\
 Data File : VW004894.D
 Acq On : 23 Aug 2018 13:40
 Operator : SY/AP
 Sample : J4624-02
 Misc : 6.22G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 E4428

Manual Integrations
 APPROVED

MMDadoda
 8/27/2018 1:45:22 PM

Quant Time: Aug 24 05:18:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 05:01:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	828989	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	815621	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	373419	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	328318	20.95	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.80%		
7) Chloroethane-d5	2.89	69	253098	21.79	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.16%		
10) 1,1-Dichloroethene-d2	4.03	63	331232	16.55	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.20%		
20) 2-Butanone-d5	7.09	46	120221	37.70	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	75.40%		
24) Chloroform-d	7.66	84	411747	22.37	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.48%		
26) 1,2-Dichloroethane-d4	8.31	65	225230	22.52	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.08%		
29) Benzene-d6	8.28	84	1018904	24.29	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.16%		
33) 1,2-Dichloropropane-d6	9.28	67	293683	23.82	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.28%		
37) Toluene-d8	10.33	98	1027645	23.12	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	92.48%		
38) trans-1,3-Dichloropropene-	10.59	79	122735	23.14	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	92.56%		
39) 2-Hexanone-d5	10.93	63	124409	40.74	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.48%		
48) 1,1,2,2-Tetrachloroethane-	12.70	84	251303	20.29	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	81.16%		
61) 1,2-Dichlorobenzene-d4	13.87	152	367526	24.50	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.00%		

Target Compounds

13) Acetone	4.15	43	7854m	3.180	ug/L	Ovalue 97
18) trans-1,2-Dichloroethene	5.43	96	78866	7.847	ug/L	97
22) cis-1,2-Dichloroethene	7.18	96	1755077	161.835	ug/L	97
35) Trichloroethene	9.10	95	674649	58.341	ug/L	99
47) Tetrachloroethene	10.87	164	2727032	240.880	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed