

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082321\
 Data File : VW019853.D
 Acq On : 23 Aug 2021 14:52
 Operator : SY/VA
 Sample : M3518-07
 Misc : 6.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AY9

Quant Time: Aug 24 00:56:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 24 00:54:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	19754	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	16999	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	4897	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	11958	39.070	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	156.280%#
7) Chloroethane-d5	2.891	69	8545	31.808	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	127.240%
11) 1,1-Dichloroethene-d2	4.031	63	11705	22.039	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	88.160%
21) 2-Butanone-d5	7.092	46	3026	48.674	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.340%
24) Chloroform-d	7.659	84	17453	32.126	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	128.520%
26) 1,2-Dichloroethane-d4	8.311	65	9631	32.897	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	131.600%#
32) Benzene-d6	8.281	84	29932	30.882	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	123.520%
36) 1,2-Dichloropropane-d6	9.281	67	10212	34.792	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	139.160%#
41) Toluene-d8	10.329	98	20220	22.765	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.040%
43) trans-1,3-Dichloroprop...	10.585	79	2832	23.356	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.440%
47) 2-Hexanone-d5	10.927	63	1603	39.204	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.400%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	7504	31.412	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	125.640%#
66) 1,2-Dichlorobenzene-d4	13.853	152	4442	26.444	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.760%
Target Compounds						Qvalue
16) Methylene chloride	4.934	84	4738	13.975	ug/L	95
42) Toluene	10.390	91	522	0.472	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082321\
Data File : VW019853.D
Acq On : 23 Aug 2021 14:52
Operator : SY/VA
Sample : M3518-07
Misc : 6.89g/10mL/MSVOA_W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AY9

Quant Time: Aug 24 00:56:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 24 00:54:38 2021
Response via : Initial Calibration




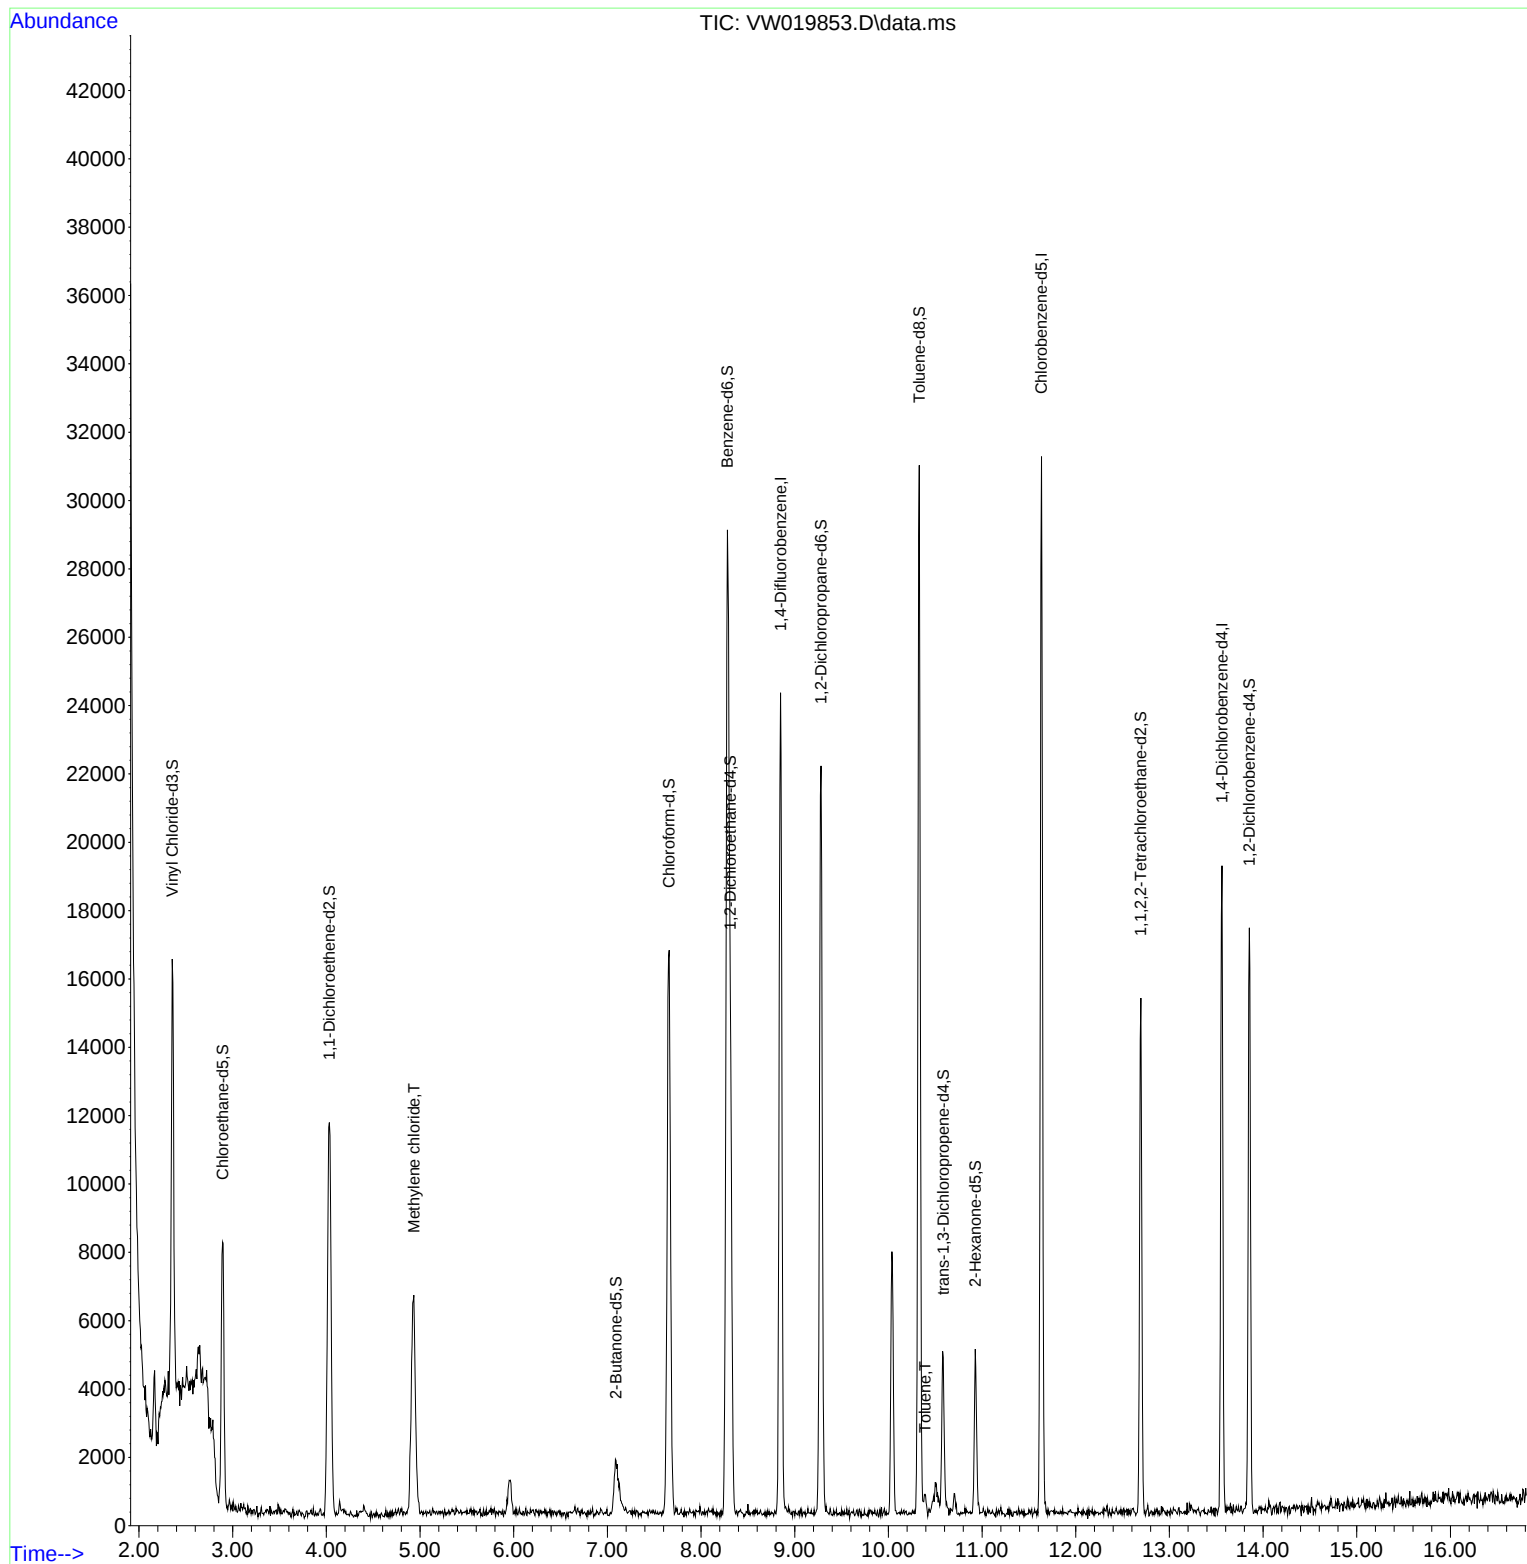


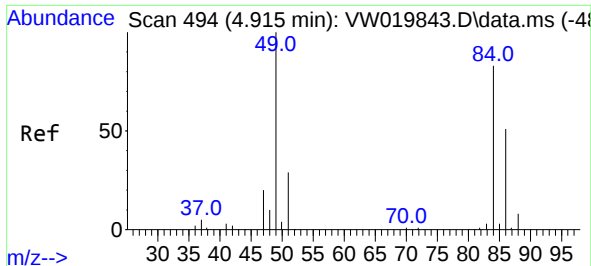

#16
Methylene chloride
Concen: 13.975 ug/L
RT: 4.934 min Scan# 497
Delta R.T. 0.018 min
Lab File: VW019853.D
Acq: 23 Aug 2021 14:52

Instrument :
MSVOA_W
ClientSampled :
C0AY9

Tgt Ion: 84 Resp: 4738
Ion Ratio Lower Upper
84 100
86 71.7 45.3 84.1
49 120.9 86.6 160.8

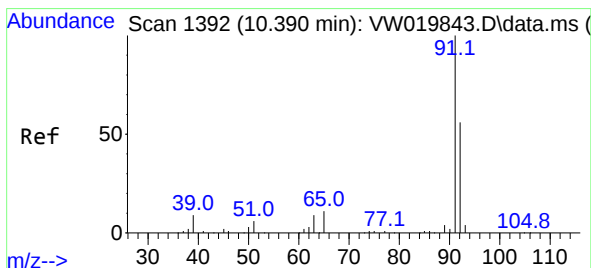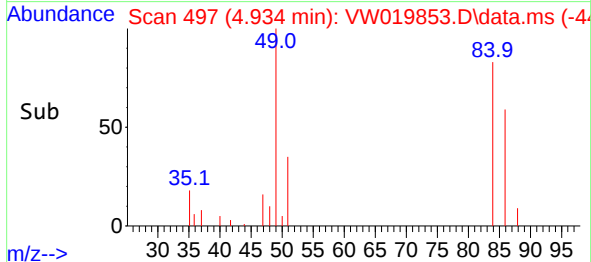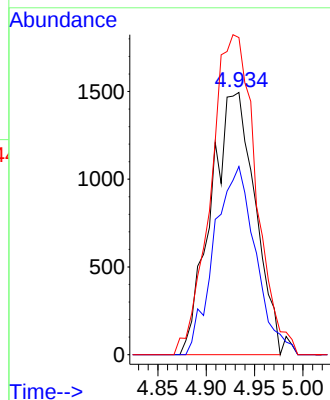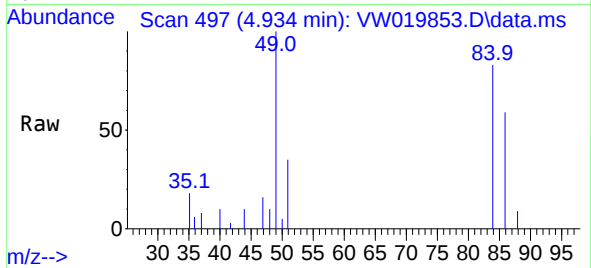

#42
Toluene
Concen: 0.472 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. -0.000 min
Lab File: VW019853.D
Acq: 23 Aug 2021 14:52

Tgt Ion: 91 Resp: 522
Ion Ratio Lower Upper
91 100
92 55.7 39.5 73.3

