

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
 Data File : VW026830.D
 Acq On : 23 Aug 2023 21:21
 Operator : SY/MD
 Sample : 04108-18
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DCHP4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/25/2023
 Supervised By :Semsettin Yesilyurt 08/25/2023

08/25/2023
 Supervised By :Semsettin
 Yesilyurt

Quant Time: Aug 24 04:49:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 23 01:29:10 2023
 Response via : Initial Calibration

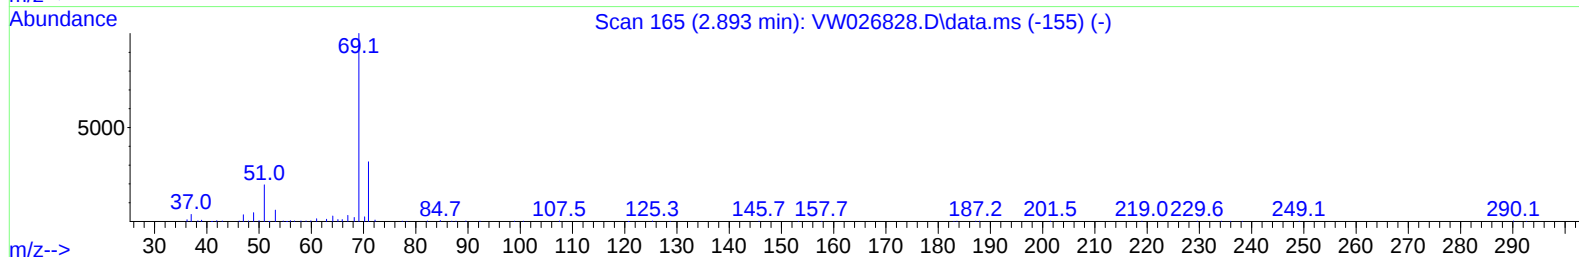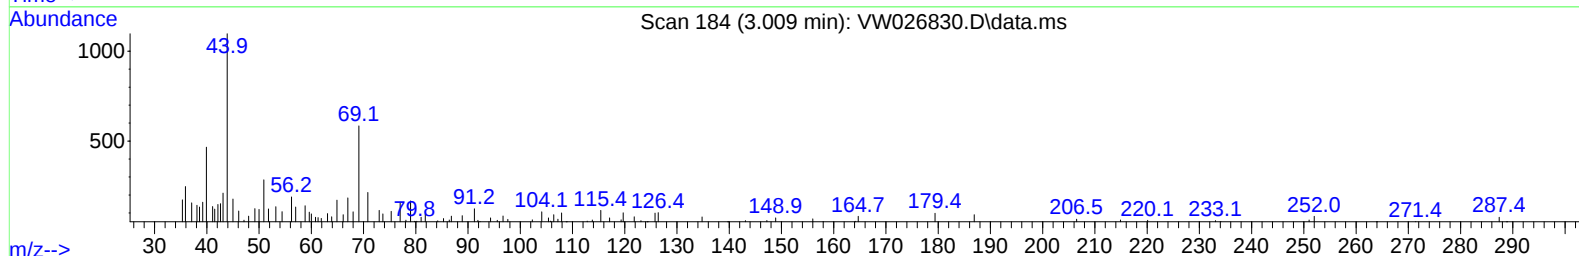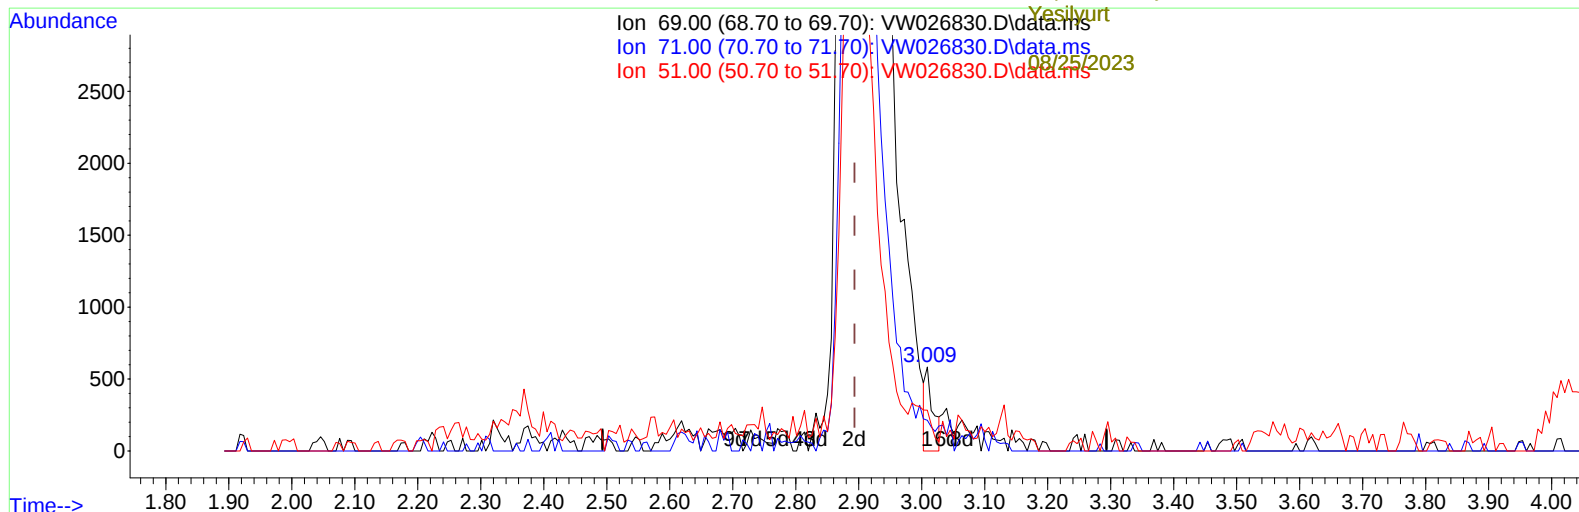

TIC: VW026830.D\data.ms

(7) Chloroethane-d5 (S)

3.009min (+ 0.116) 0.08 ug/L

response 493

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	24.75
51.00	28.30	21.30
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
Data File : VW026830.D
Acq On : 23 Aug 2023 21:21
Operator : SY/MD
Sample : 04108-18
Misc : 5.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
DCHP4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/25/2023
Supervised By :Semsettin Yesilyurt 08/25/2023

08/25/2023
Supervised By :Semsettin
Yesilyurt

Quant Time: Aug 24 04:49:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 23 01:29:10 2023
Response via : Initial Calibration

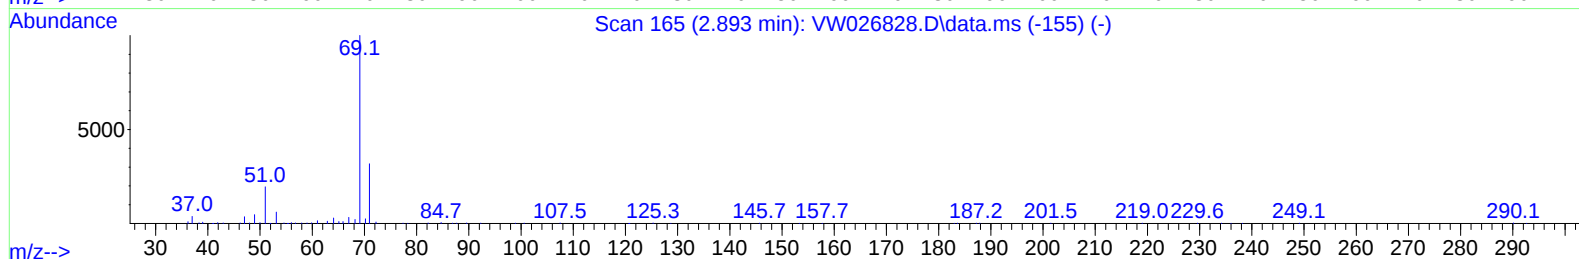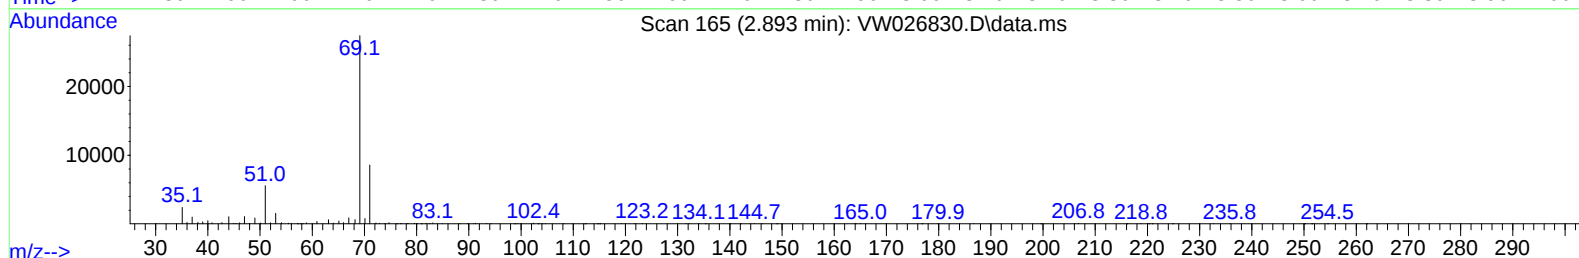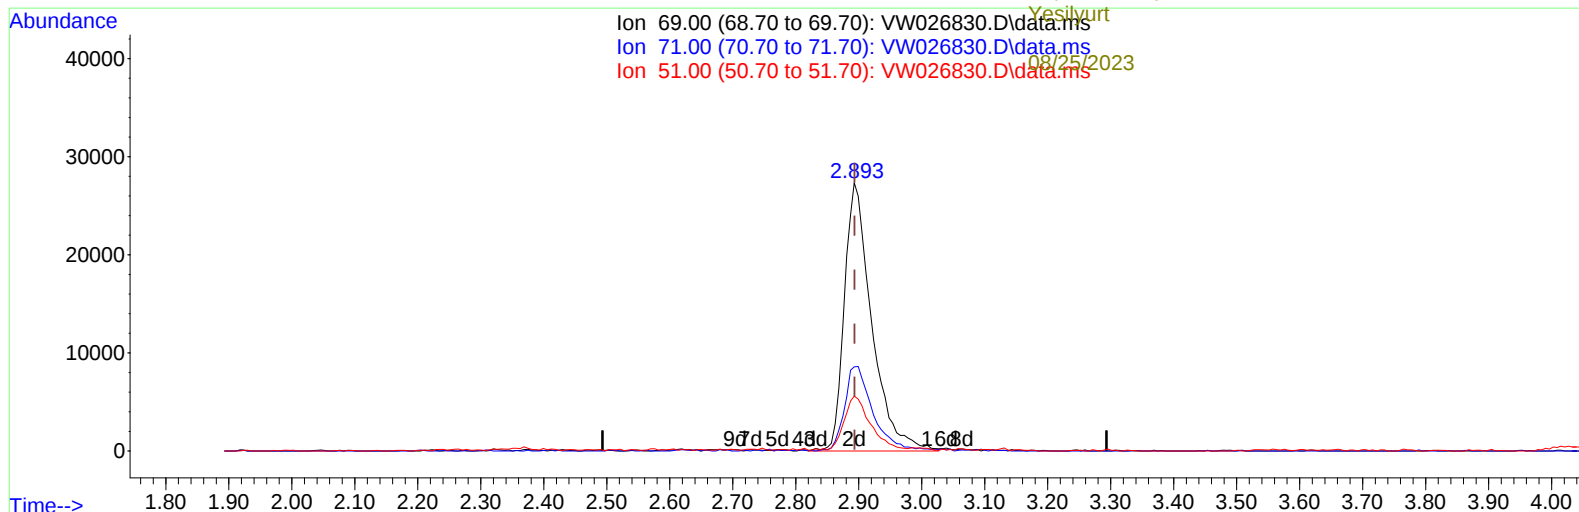

TIC: VW026830.D\data.ms

(7) Chloroethane-d5 (S)

2.893min (-0.000) 13.21 ug/L m

response 82679

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	0.15#
51.00	28.30	0.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
 Data File : VW026830.D
 Acq On : 23 Aug 2023 21:21
 Operator : SY/MD
 Sample : 04108-18
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHP4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/25/2023
 Supervised By :Semsettin Yesilyurt 08/25/2023

08/25/2023
 Supervised By :Semsettin
 Yesilyurt

Quant Time: Aug 24 04:49:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 23 01:29:10 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		512056	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		501139	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		258936	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		88546	10.519	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.080%	
7) Chloroethane-d5	2.893	69		82679m	13.209	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.840%	
11) 1,1-Dichloroethene-d2	4.021	65		56979	13.763	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.040%	
21) 2-Butanone-d5	7.081	46		125330	51.802	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.600%	
24) Chloroform-d	7.648	84		329718	19.185	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.760%	
26) 1,2-Dichloroethane-d4	8.307	65		203447	21.451	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.800%	
32) Benzene-d6	8.276	84		631241	18.277	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.120%	
36) 1,2-Dichloropropane-d6	9.276	67		198650	18.465	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	73.840%	
41) Toluene-d8	10.325	98		534367	18.024	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.080%	
43) trans-1,3-Dichloroprop...	10.575	79		84095	18.932	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.720%	
47) 2-Hexanone-d5	10.922	63		63612	56.271	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.540%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		206186	24.268	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.080%	
66) 1,2-Dichlorobenzene-d4	13.848	152		196144	21.164	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.640%	
Target Compounds							
16) Methylene chloride	4.917	84		66843	6.748	ug/L	94
46) Tetrachloroethene	10.861	164		9969	1.476	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
Data File : VW026830.D
Acq On : 23 Aug 2023 21:21
Operator : SY/MD
Sample : 04108-18
Misc : 5.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHP4

Manual IntegrationsAPPROVED

Quant Time: Aug 24 04:49:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 23 01:29:10 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/25/2023
Supervised By :Semsettin Yesilyurt 08/25/2023

08/25/2023
Supervised By :Semsettin
Yesilyurt

08/25/2023

