




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
Data File : VW026833.D
Acq On : 23 Aug 2023 22:33
Operator : SY/MD
Sample : 04138-03
Misc : 5.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHQ7

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/25/2023
Supervised By :Semsettin Yesilyurt 08/25/2023

Quant Time: Aug 24 04:49:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 23 01:29:10 2023
Response via : Initial Calibration

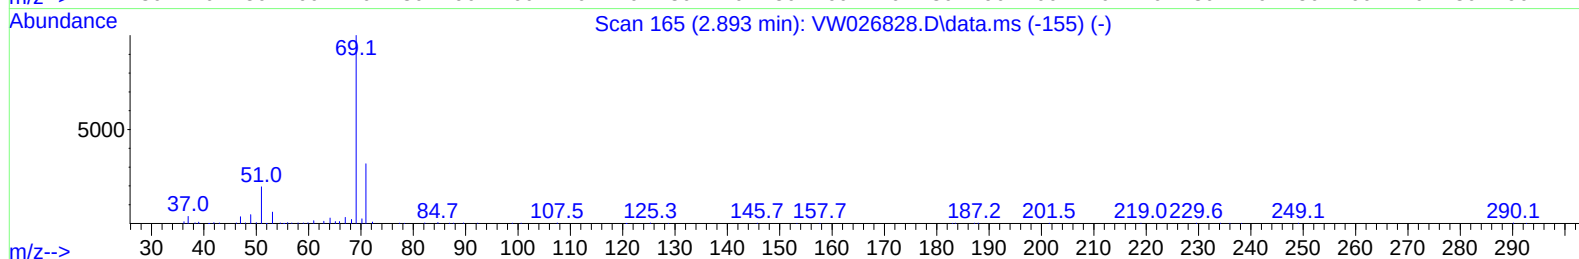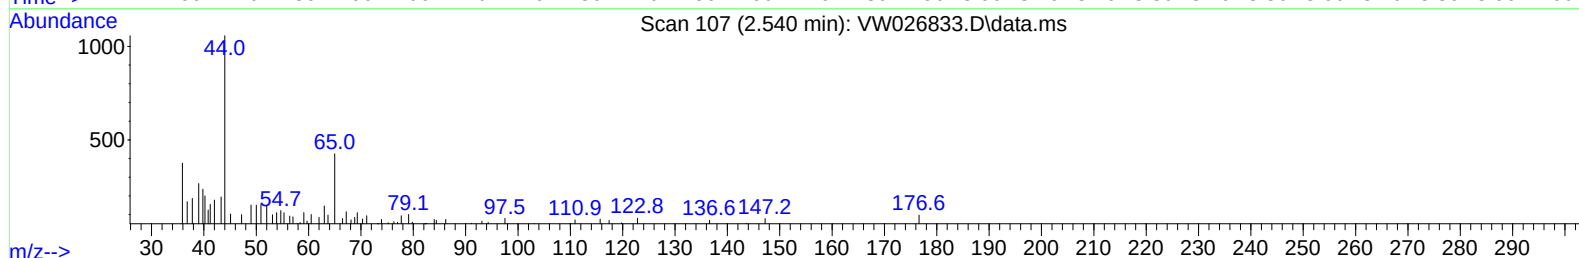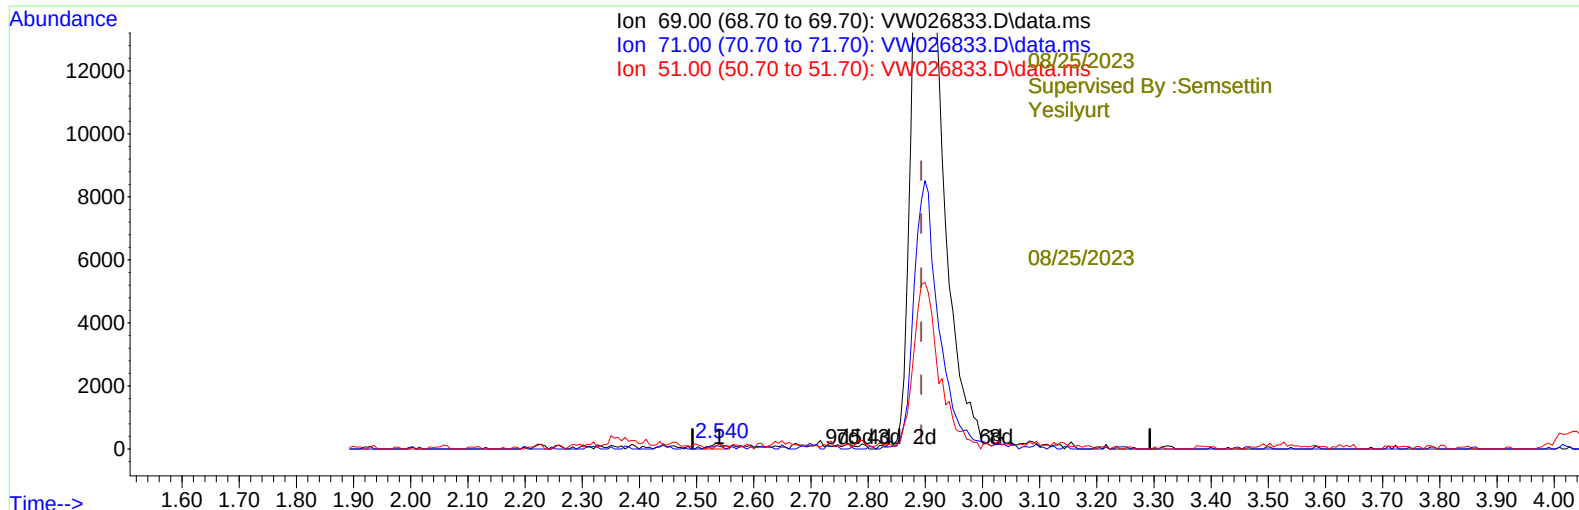

TIC: VW026833.D\data.ms

(7) Chloroethane-d5 (S)

2.540min (-0.354) 0.12 ug/L

response 336

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	27.68
51.00	28.30	33.63
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
Data File : VW026833.D
Acq On : 23 Aug 2023 22:33
Operator : SY/MD
Sample : 04138-03
Misc : 5.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHQ7

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/25/2023
Supervised By :Semsettin Yesilyurt 08/25/2023

Quant Time: Aug 24 04:49:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 23 01:29:10 2023
Response via : Initial Calibration

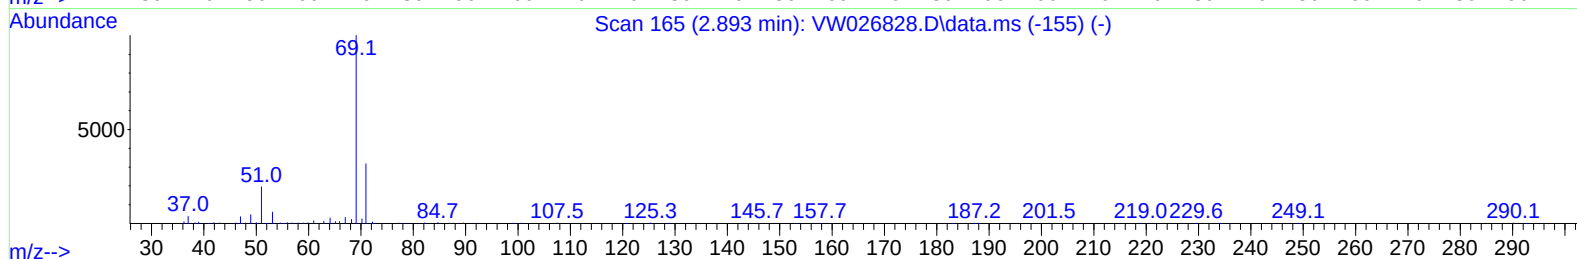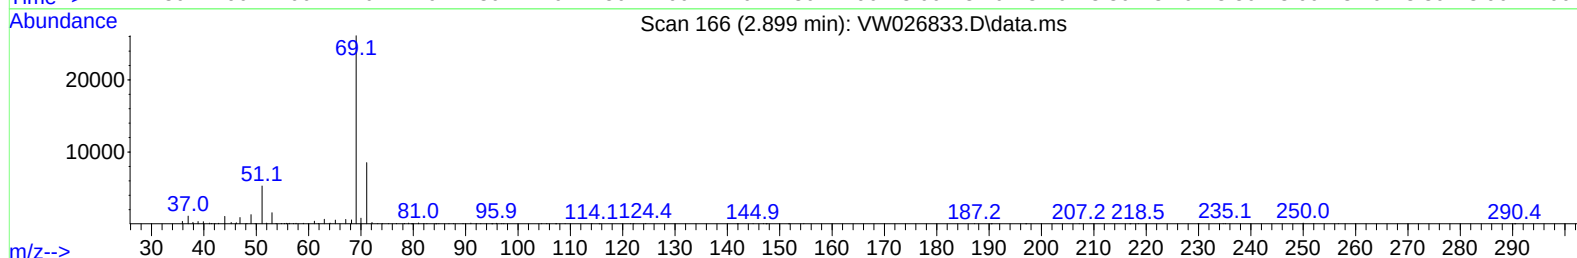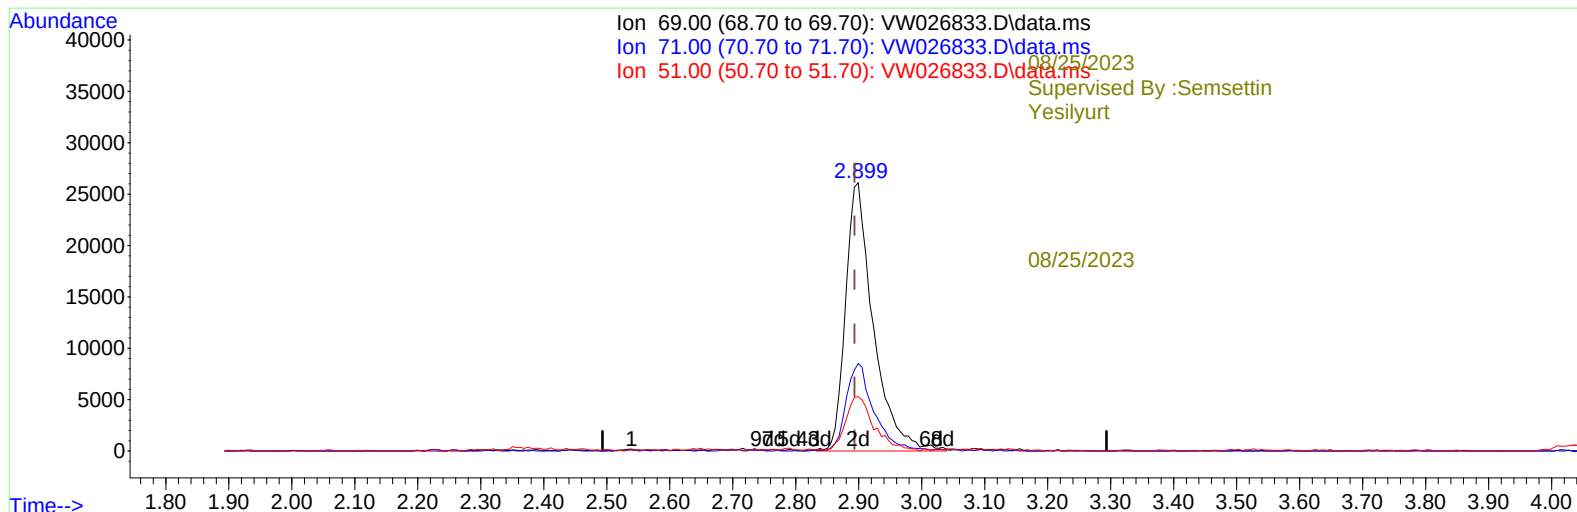

TIC: VW026833.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.006) 29.28 ug/L m

response 79903

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	0.12#
51.00	28.30	0.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
 Data File : VW026833.D
 Acq On : 23 Aug 2023 22:33
 Operator : SY/MD
 Sample : 04138-03
 Misc : 5.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHQ7

Manual IntegrationsAPPROVED

Quant Time: Aug 24 04:49:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 23 01:29:10 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/25/2023
 Supervised By :Semsettin Yesilyurt 08/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	223262	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	234294	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	119697	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	85975	23.425	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	93.720%		
7) Chloroethane-d5	2.899	69	79903m	29.278	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	117.120%		
11) 1,1-Dichloroethene-d2	4.027	65	52685	29.187	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	116.760%#		
21) 2-Butanone-d5	7.081	46	112262	106.422	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	212.840%#		
24) Chloroform-d	7.648	84	321546	42.911	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	171.640%#		
26) 1,2-Dichloroethane-d4	8.307	65	201797	48.800	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	195.200%#		
32) Benzene-d6	8.276	84	593153	36.734	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	146.920%#		
36) 1,2-Dichloropropane-d6	9.276	67	200456	39.854	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	159.400%#		
41) Toluene-d8	10.325	98	510003	36.794	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	147.160%#		
43) trans-1,3-Dichloroprop...	10.581	79	81237	39.118	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	156.480%#		
47) 2-Hexanone-d5	10.922	63	55681	105.354	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	210.700%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	210647	53.031	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	212.120%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	206092	48.105	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	192.400%#		
Target Compounds						
16) Methylene chloride	4.929	84	26097	6.043	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082323\
Data File : VW026833.D
Acq On : 23 Aug 2023 22:33
Operator : SY/MD
Sample : 04138-03
Misc : 5.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHQ7

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/25/2023
Supervised By :Semsettin Yesilyurt 08/25/2023

Quant Time: Aug 24 04:49:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 23 01:29:10 2023
Response via : Initial Calibration

