

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082421\
 Data File : VW019869.D
 Acq On : 24 Aug 2021 11:28
 Operator : SY/VA
 Sample : M3518-07RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AY9RE

Quant Time: Aug 25 00:59:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 25 00:57:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	130	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.646	117	124	25.000	ug/L	# 0.01
58) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/L	-13.56
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.367	65	323	160.361	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	641.440%#	
7) Chloroethane-d5	2.897	69	70	39.594	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	158.360%#	
11) 1,1-Dichloroethene-d2	4.037	63	178	50.928	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	203.720%#	
21) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount	50.000	Range 20 - 135	Recovery	=	0.000%#	
24) Chloroform-d	7.665	84	374	104.610	ug/L	0.01
Spiked Amount	25.000	Range 40 - 150	Recovery	=	418.440%#	
26) 1,2-Dichloroethane-d4	8.323	65	33	17.128	ug/L	0.01
Spiked Amount	25.000	Range 70 - 130	Recovery	=	68.520%#	
32) Benzene-d6	8.275	84	291	41.159	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	164.640%#	
36) 1,2-Dichloropropane-d6	9.262	67	173	80.802	ug/L	-0.01
Spiked Amount	25.000	Range 70 - 120	Recovery	=	323.200%#	
41) Toluene-d8	10.329	98	228	35.190	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	140.760%#	
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount	25.000	Range 30 - 135	Recovery	=	0.000%#	
47) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount	50.000	Range 20 - 135	Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.701	84	66	37.874	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	151.480%#	
66) 1,2-Dichlorobenzene-d4	0.000	152	0	0.000	ug/L	
Spiked Amount	25.000	Range 75 - 120	Recovery	=	0.000%#	
Target Compounds						
16) Methylene chloride	4.922	84	72	32.270	ug/L	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082421\
Data File : VW019869.D
Acq On : 24 Aug 2021 11:28
Operator : SY/VA
Sample : M3518-07RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AY9RE

Quant Time: Aug 25 00:59:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 25 00:57:31 2021
Response via : Initial Calibration

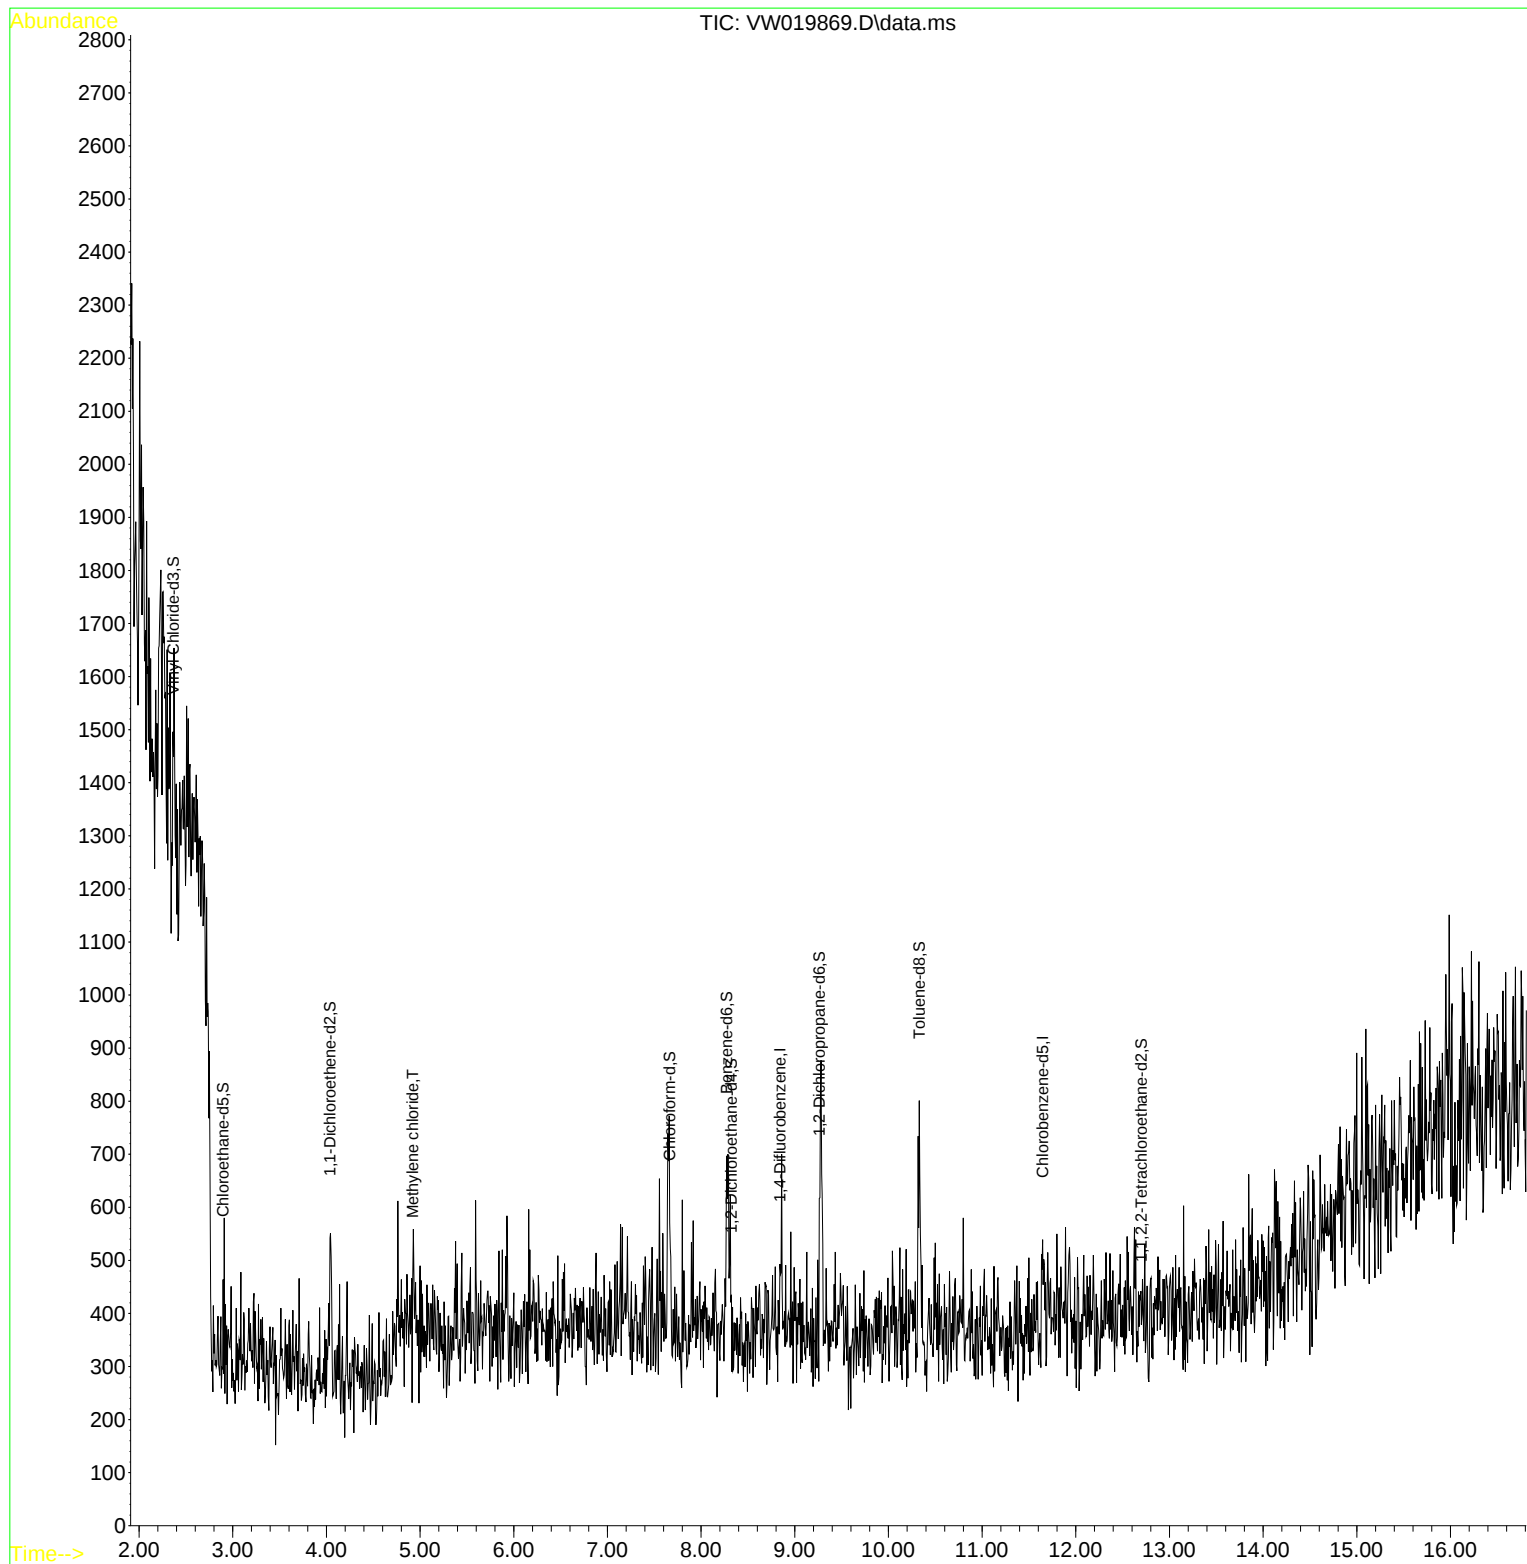

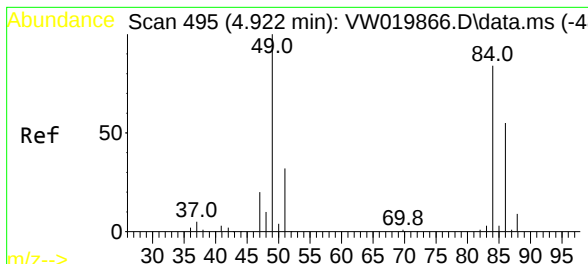

#16
Methylene chloride
Concen: 32.270 ug/L
RT: 4.922 min Scan# 495
Delta R.T. -0.000 min
Lab File: VW019869.D
Acq: 24 Aug 2021 11:28

Instrument :
MSVOA_W
ClientSampleId :
C0AY9RE

Tgt Ion:	84	Resp:	72
Ion	Ratio	Lower	Upper
84	100		
86	0.0	45.3	84.1#
49	0.0	86.6	160.8#

