




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082421\
Data File : VW019871.D
Acq On : 24 Aug 2021 12:16
Operator : SY/VA
Sample : M3518-11RE
Misc : 5.22g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B24RE

Manual Integrations
APPROVED

MMDadoda
8/25/2021 6:53:07 PM

Quant Time: Aug 25 01:00:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 25 00:57:31 2021
Response via : Initial Calibration

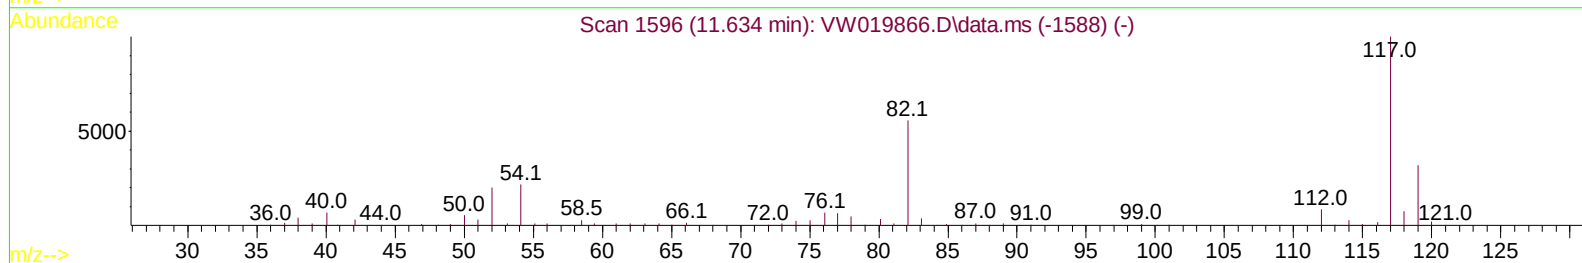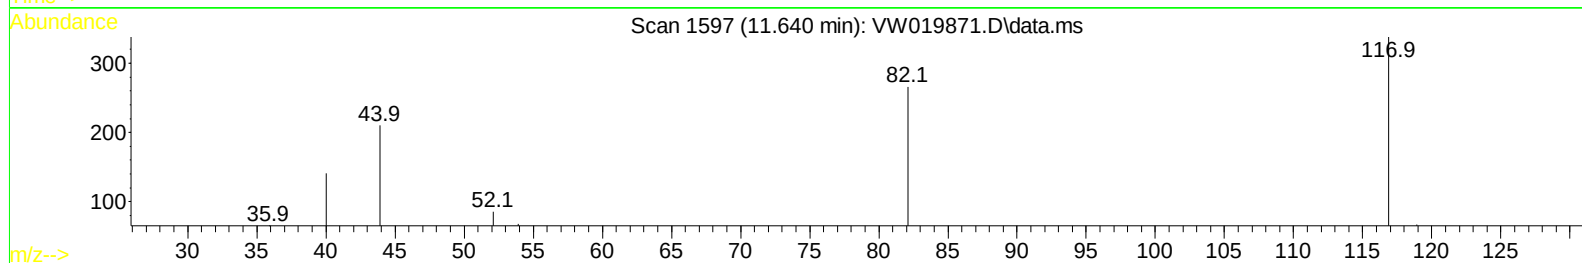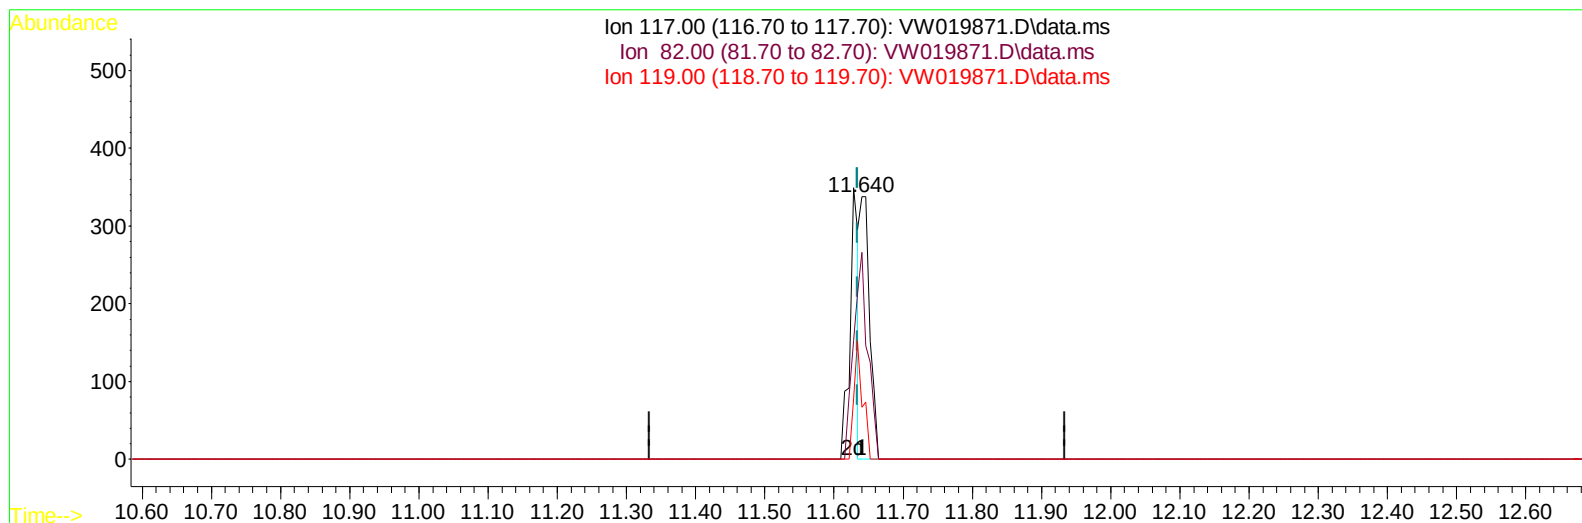

TIC: VW019871.D\data.ms

(28) Chlorobenzene-d5 (I)

11.640min (+ 0.006) 25.00 ug/L

response 336

Ion	Exp%	Act%
117.00	100.00	100.00
82.00	57.20	113.99#
119.00	31.70	40.48#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082421\
 Data File : VW019871.D
 Acq On : 24 Aug 2021 12:16
 Operator : SY/VA
 Sample : M3518-11RE
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B24RE

Manual Integrations
 APPROVED

MMDadoda
 8/25/2021 6:53:07 PM

Quant Time: Aug 25 01:00:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 25 00:57:31 2021
 Response via : Initial Calibration

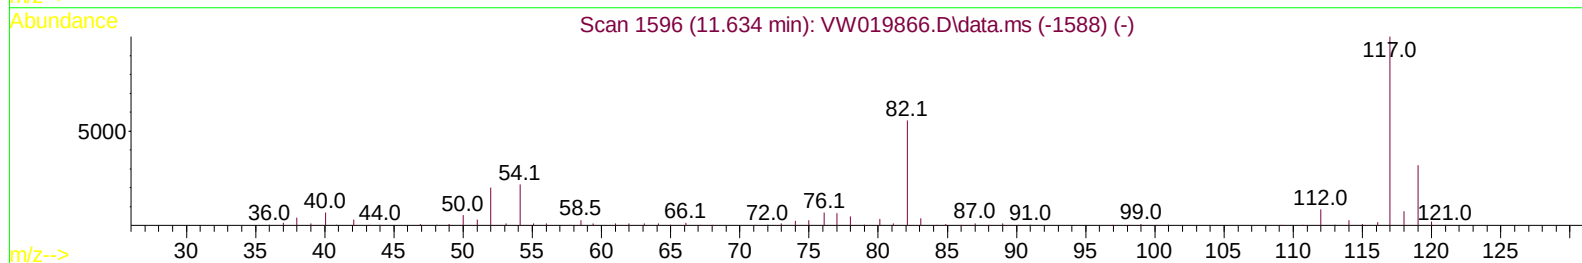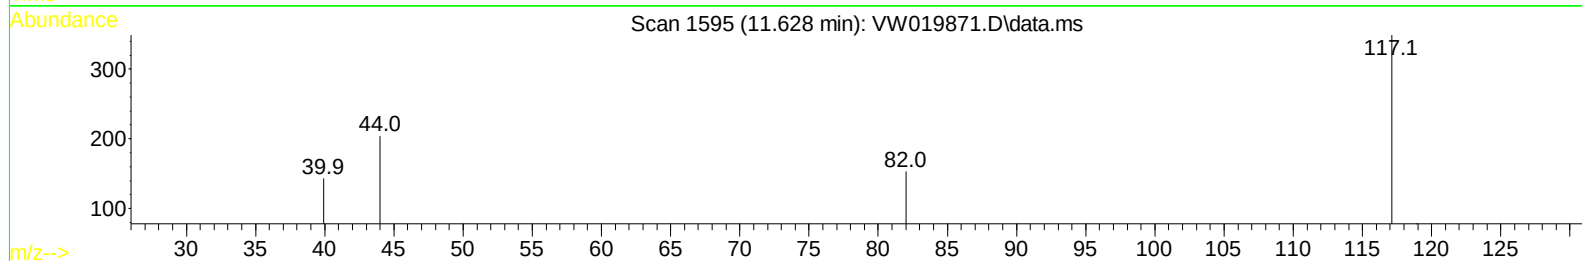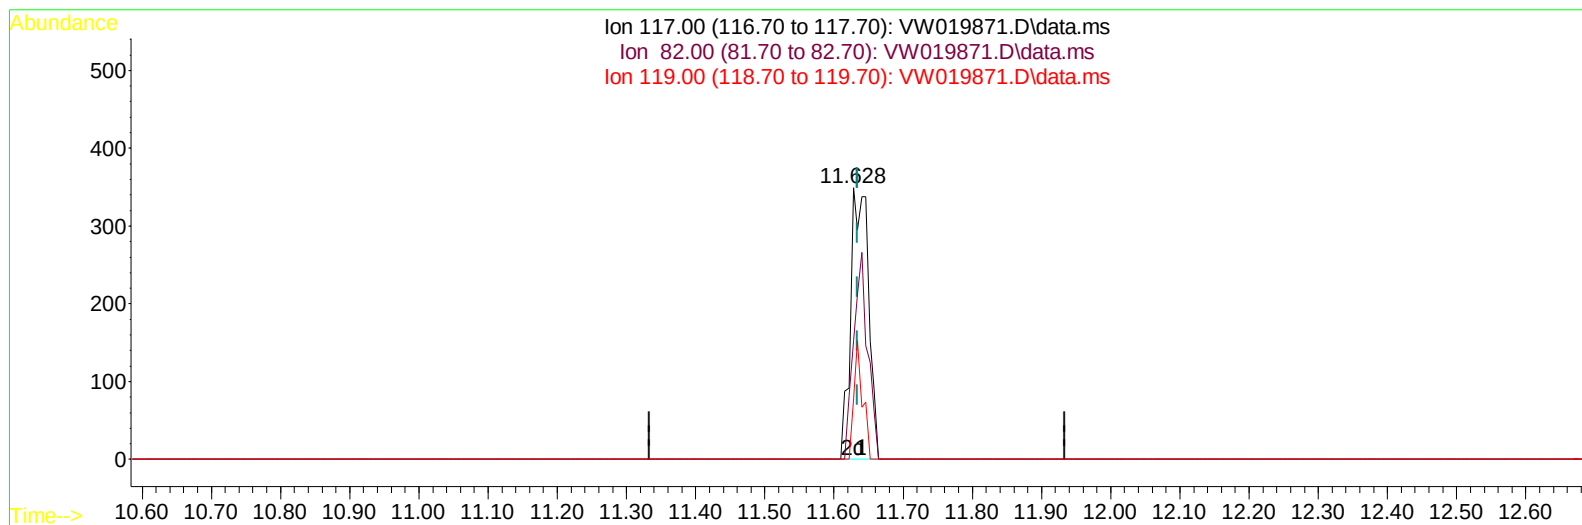

TIC: VW019871.D\data.ms

(28) Chlorobenzene-d5 (I)

11.628min (-0.006) 25.00 ug/L m

response 637

Ion	Exp%	Act%
117.00	100.00	100.00
82.00	57.20	60.13
119.00	31.70	21.35#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082421\
 Data File : VW019871.D
 Acq On : 24 Aug 2021 12:16
 Operator : SY/VA
 Sample : M3518-11RE
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0B24RE

Manual Integrations
 APPROVED

MMDadoda
 8/25/2021 6:53:07 PM

Quant Time: Aug 25 01:00:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 25 00:57:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	1028	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	637m	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/L	-13.56
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	1213	76.157	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	304.640%#	
7) Chloroethane-d5	2.910	69	905	64.734	ug/L	0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	258.920%#	
11) 1,1-Dichloroethene-d2	4.038	63	1189	43.020	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	172.080%#	
21) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount	50.000	Range 20 - 135	Recovery	=	0.000%#	
24) Chloroform-d	7.659	84	1746	61.758	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	247.040%#	
26) 1,2-Dichloroethane-d4	8.311	65	708	46.470	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	185.880%#	
32) Benzene-d6	8.275	84	2116	58.260	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	233.040%#	
36) 1,2-Dichloropropane-d6	9.281	67	910	82.737	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	330.960%#	
41) Toluene-d8	10.329	98	963	28.933	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	115.720%	
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount	25.000	Range 30 - 135	Recovery	=	0.000%#	
47) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount	50.000	Range 20 - 135	Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	526	58.758	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	235.040%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	56	0.000	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	0.000%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082421\
Data File : VW019871.D
Acq On : 24 Aug 2021 12:16
Operator : SY/VA
Sample : M3518-11RE
Misc : 5.22g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B24RE

Manual Integrations
APPROVED

MMDadoda
8/25/2021 6:53:07 PM

Quant Time: Aug 25 01:00:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 25 00:57:31 2021
Response via : Initial Calibration

