
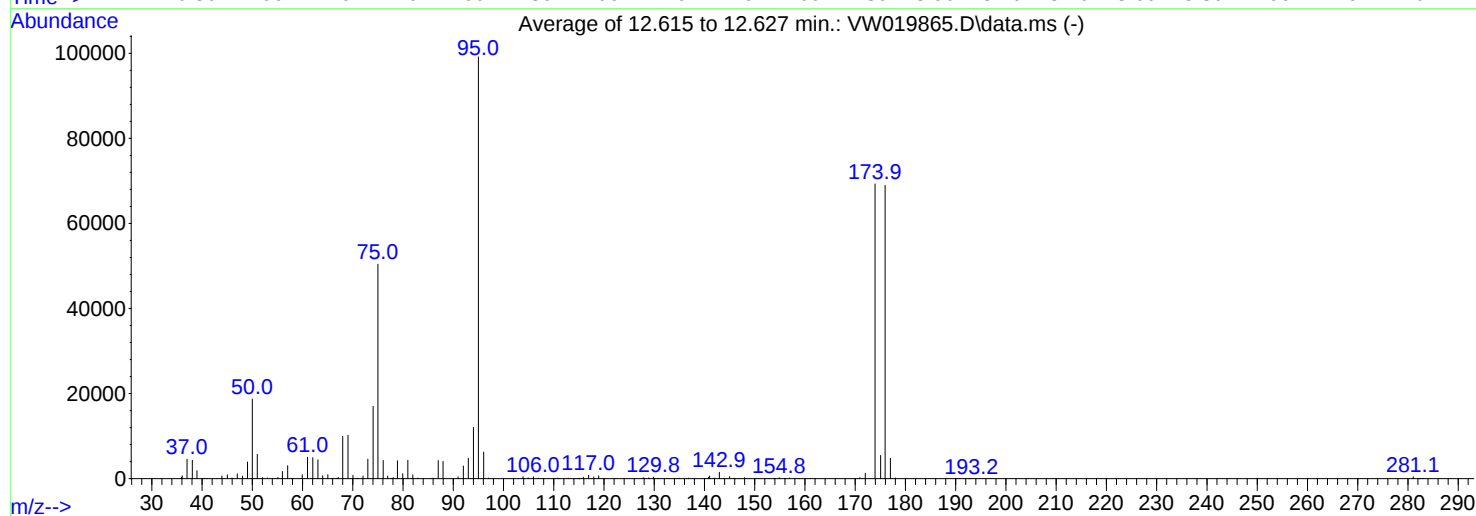


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082421\
 Data File : VW019865.D
 Acq On : 24 Aug 2021 09:11
 Operator : SY/VA
 Sample : BFB423
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB423

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Title : SFAM01.0
 Last Update : Wed Aug 25 00:57:31 2021

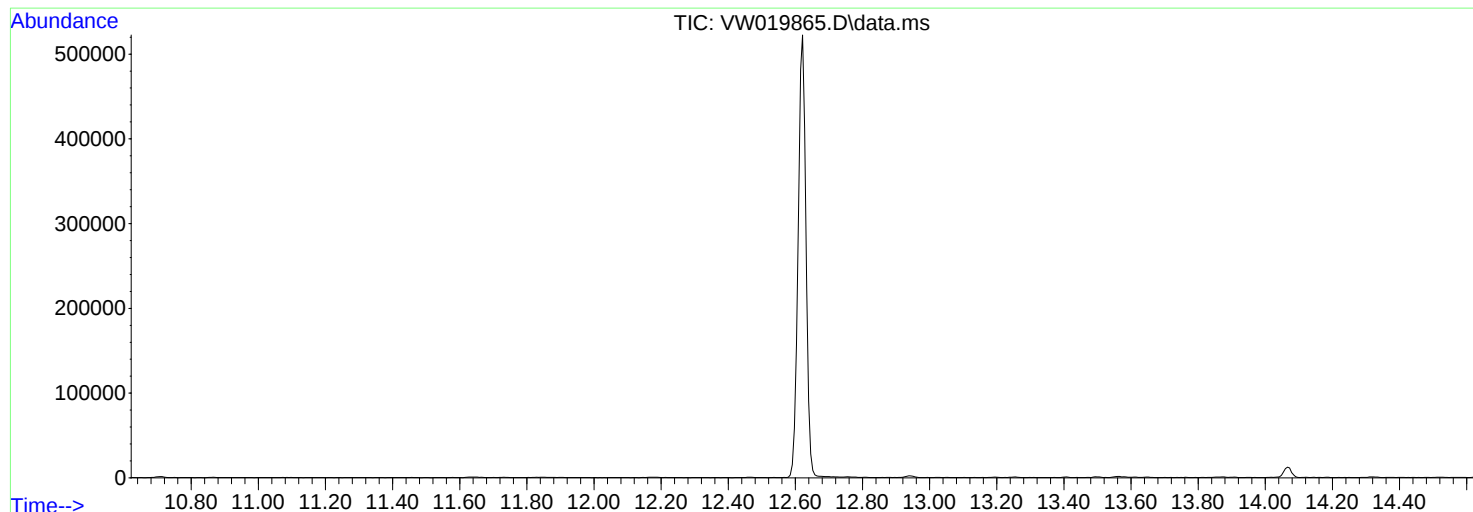

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	18744	PASS
75	95	30	80	50.8	50424	PASS
95	95	100	100	100.0	99165	PASS
96	95	5	9	6.3	6254	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.9	69307	PASS
175	174	5	9	7.9	5445	PASS
176	174	95	105	99.5	68949	PASS
177	176	5	10	6.9	4771	PASS

Scan 1749 (12.567 min): VW019865.D\data.ms
BFB423

m/z	Abundance
40.10	241.0
43.90	305.0

Instrument :
MSVOA_W
ClientSampleId :
BFB423

m/z	Abundance
35.90	1073.0
37.00	5134.0
38.00	4423.0
39.00	2031.0
40.00	179.0
40.50	107.0
41.00	78.0
42.90	55.0
44.00	1141.0
45.00	917.0
46.10	163.0
47.00	1235.0
48.00	735.0
49.10	4072.0
50.00	20728.0
51.00	6184.0
52.10	297.0
53.00	204.0
55.10	383.0
56.00	1747.0
57.00	3129.0
57.90	95.0
60.00	934.0
61.00	5378.0
62.10	5358.0
63.00	5182.0
64.00	796.0
65.00	1090.0
66.10	106.0
66.80	202.0
67.10	191.0
68.00	10217.0
69.00	10826.0
70.10	726.0
70.80	96.0
72.10	663.0
73.00	4949.0
74.00	18256.0
75.00	53464.0
76.00	4439.0
77.00	556.0
77.80	373.0
78.90	4674.0
80.00	1124.0
81.00	4605.0
81.90	909.0
82.90	150.0
85.80	200.0
87.00	4321.0
88.00	3913.0
90.90	399.0
92.00	3089.0
93.00	5263.0
94.00	12018.0
95.00	103528.0
96.10	6389.0
97.00	185.0
103.90	411.0
104.90	121.0
105.90	406.0
106.90	130.0
107.80	63.0
110.00	92.0
110.80	152.0
111.90	97.0
112.90	138.0
114.80	96.0
115.90	276.0
116.90	823.0
118.00	435.0
118.90	759.0
124.10	100.0
127.80	417.0
128.80	213.0
129.10	209.0
129.90	343.0
130.70	86.0
132.80	52.0
135.00	105.0
136.80	160.0
140.10	89.0
140.80	1033.0
141.90	162.0
143.00	1548.0
145.00	727.0
145.90	164.0
147.00	70.0
147.90	209.0
150.10	59.0
152.90	84.0
153.80	96.0
154.90	180.0

Instrument :
MSVOA_W
ClientSampleId :
BFB423

157.10	172.0
158.80	121.0
161.10	68.0
171.00	261.0
172.00	1310.0
174.00	67256.0
175.10	5226.0
175.90	62728.0
177.00	4574.0
178.00	194.0
190.80	78.0
193.20	155.0
281.00	715.0
282.10	149.0
282.90	83.0

Instrument :
MSVOA_W
ClientSampleId :
BFB423

m/z	Abundance
36.10	964.0
37.00	5292.0
38.10	4900.0
39.00	2117.0
39.90	163.0
40.30	161.0
40.90	50.0
43.00	109.0
44.00	943.0
45.00	936.0
45.90	133.0
47.00	1359.0
48.00	645.0
49.00	4499.0
50.00	20936.0
51.00	6425.0
52.00	278.0
53.00	240.0
55.10	347.0
56.00	1852.0
57.00	3465.0
57.90	187.0
59.90	1075.0
61.00	5670.0
62.00	5250.0
63.10	4611.0
64.00	910.0
65.10	979.0
65.90	60.0
67.20	279.0
68.00	11132.0
69.10	11523.0
70.00	1005.0
71.00	92.0
72.00	716.0
73.00	5060.0
74.10	18640.0
75.00	56288.0
76.10	5105.0
77.00	668.0
78.10	327.0
78.90	4453.0
79.90	1409.0
80.90	4910.0
82.00	1010.0
83.00	154.0
85.80	140.0
87.00	5026.0
88.00	4437.0
90.90	531.0
92.00	3262.0
93.00	5013.0
94.00	13020.0
95.00	109544.0
96.10	7134.0
97.00	139.0
102.90	81.0
103.90	560.0
104.90	269.0
106.00	483.0
106.90	134.0
107.70	76.0
110.00	69.0
110.80	99.0
111.90	157.0
112.70	131.0
114.80	82.0
115.90	539.0
117.00	868.0
118.00	442.0
118.90	627.0
124.00	74.0
128.00	330.0
128.90	242.0
129.80	433.0
130.80	150.0
132.80	79.0
134.60	133.0
135.10	172.0
136.80	143.0
141.00	1109.0
142.00	184.0
142.90	1487.0
145.10	432.0
146.10	205.0
146.90	91.0
147.90	239.0
148.90	73.0
150.00	127.0
153.80	94.0
154.90	242.0
156.00	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB423

156.90	208.0
159.00	91.0
161.10	100.0
170.90	290.0
172.00	1443.0
173.90	75840.0
175.00	5960.0
176.00	75840.0
177.00	5536.0
178.00	158.0
192.60	58.0
281.10	516.0
282.00	110.0
283.10	96.0

Instrument :
MSVOA_W
ClientSampleId :
BFB423

m/z	Abundance
36.00	921.0
37.00	3256.0
38.10	3647.0
39.00	1481.0
39.90	201.0
41.10	53.0
43.00	62.0
44.00	809.0
45.10	811.0
45.90	164.0
47.00	847.0
48.10	467.0
49.00	3162.0
50.00	14569.0
51.00	4605.0
52.10	237.0
52.90	122.0
55.10	240.0
56.00	1482.0
57.10	2532.0
58.20	71.0
60.00	814.0
61.00	4133.0
62.00	4183.0
63.00	3505.0
63.90	482.0
65.10	732.0
65.90	90.0
67.00	387.0
68.00	8418.0
69.00	8209.0
70.10	703.0
71.00	68.0
72.10	429.0
73.00	3800.0
74.00	14170.0
75.00	41520.0
76.00	3307.0
76.90	542.0
78.00	373.0
78.90	3494.0
79.90	1015.0
80.90	3478.0
82.00	799.0
83.00	144.0
86.10	182.0
87.00	3405.0
87.90	3795.0
91.00	313.0
92.00	2523.0
93.00	4087.0
94.00	11062.0
95.00	84424.0
96.00	5238.0
97.00	181.0
102.90	60.0
103.90	418.0
104.90	180.0
105.90	422.0
106.80	76.0
110.00	91.0
110.70	66.0
111.10	112.0
112.10	101.0
112.90	140.0
115.00	54.0
115.90	235.0
116.90	665.0
117.90	356.0
119.00	707.0
127.80	299.0
128.70	77.0
128.90	77.0
129.90	400.0
130.90	88.0
135.10	120.0
136.90	192.0
141.00	713.0
141.90	138.0
143.00	1445.0
143.80	61.0
144.90	357.0
145.90	93.0
148.00	247.0
149.90	95.0
152.00	73.0
154.80	250.0
156.10	96.0
156.90	144.0
158.90	74.0
161.00	65.0
170.80	175.0

Instrument :
MSVOA_W
ClientSampleId :
BFB423

172.00	1082.0
174.00	64824.0
175.10	5148.0
176.00	68280.0
177.00	4204.0
178.00	159.0
280.90	148.0
282.30	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB423