




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082422\
 Data File : VW024327.D
 Acq On : 24 Aug 2022 17:25
 Operator : SY/VA
 Sample : N4322-01RE
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY163RE

Manual IntegrationsAPPROVED

Quant Time: Aug 25 01:33:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 25 01:31:24 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/25/2022
 Supervised By :Mahesh Dadoda 08/25/2022

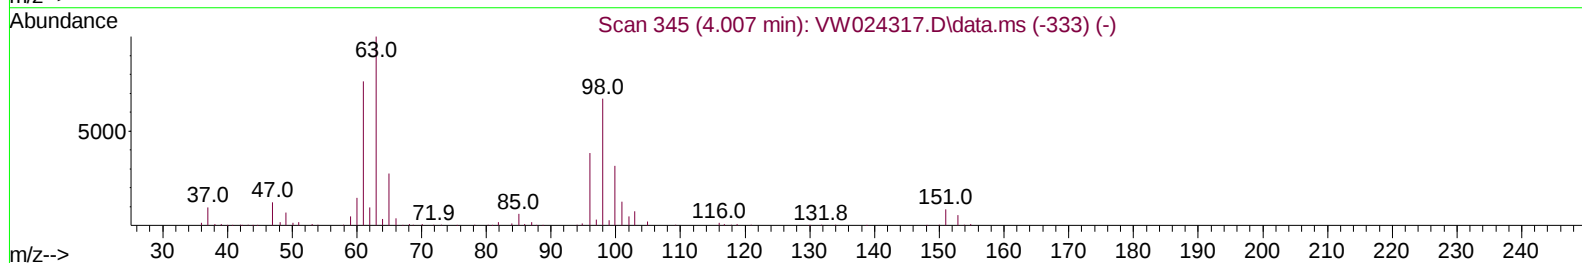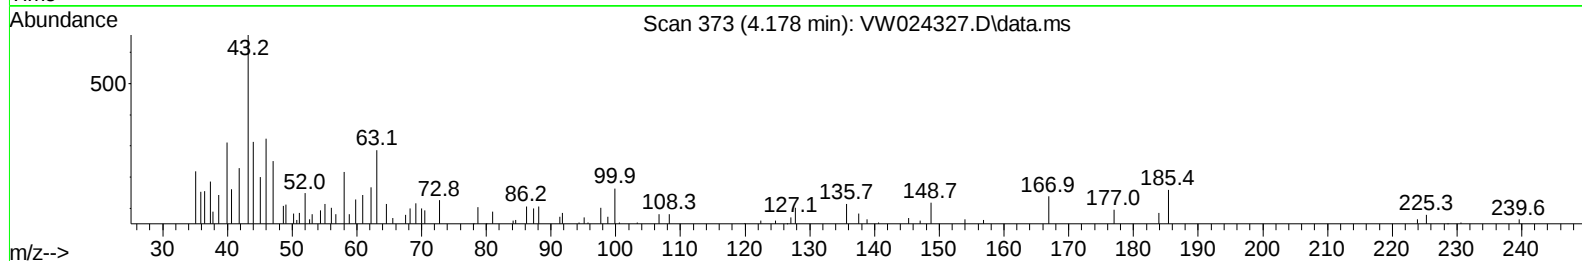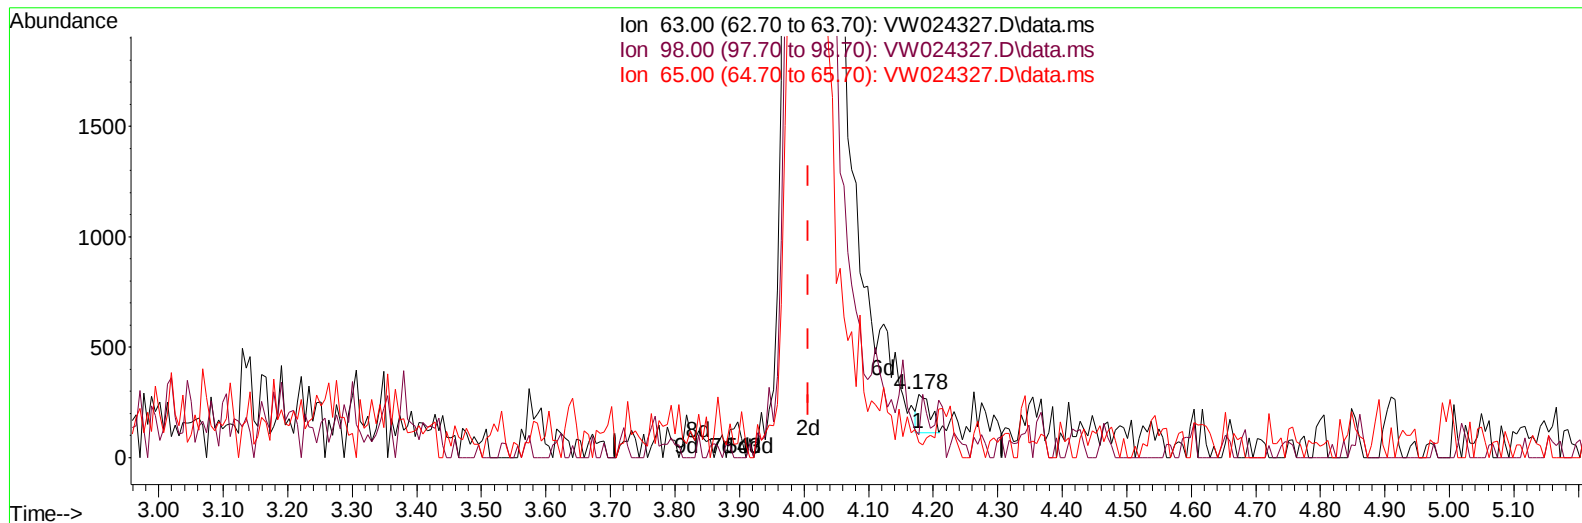

TIC: VW024327.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.178min (+ 0.171) 0.04 ug/L

response 238

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.50	71.43
65.00	23.50	17.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082422\
 Data File : VW024327.D
 Acq On : 24 Aug 2022 17:25
 Operator : SY/VA
 Sample : N4322-01RE
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY163RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/25/2022
 Supervised By :Mahesh Dadoda 08/25/2022

Quant Time: Aug 25 01:33:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 25 01:31:24 2022
 Response via : Initial Calibration

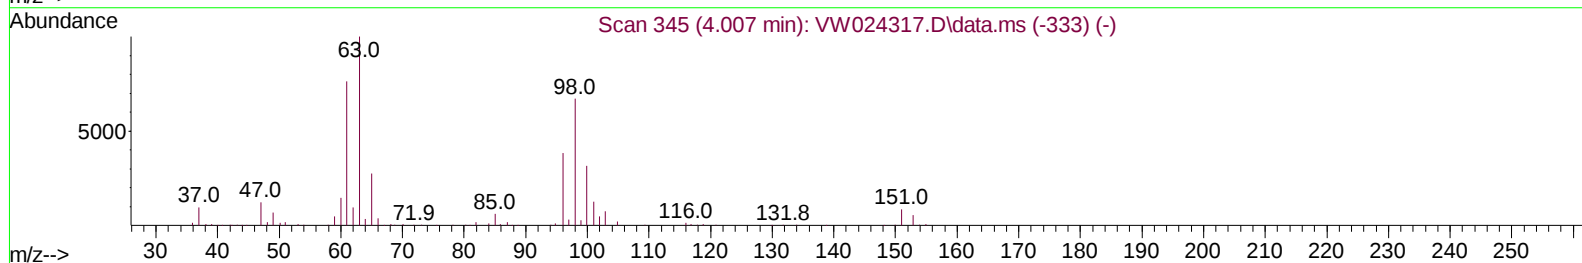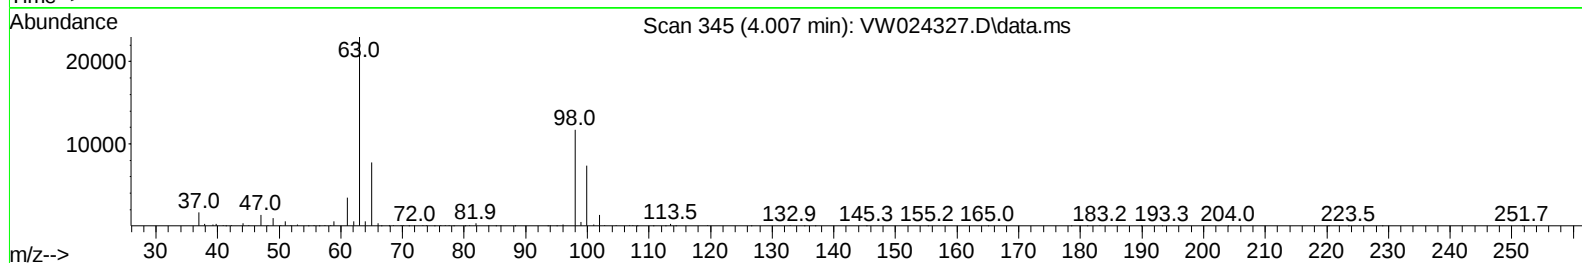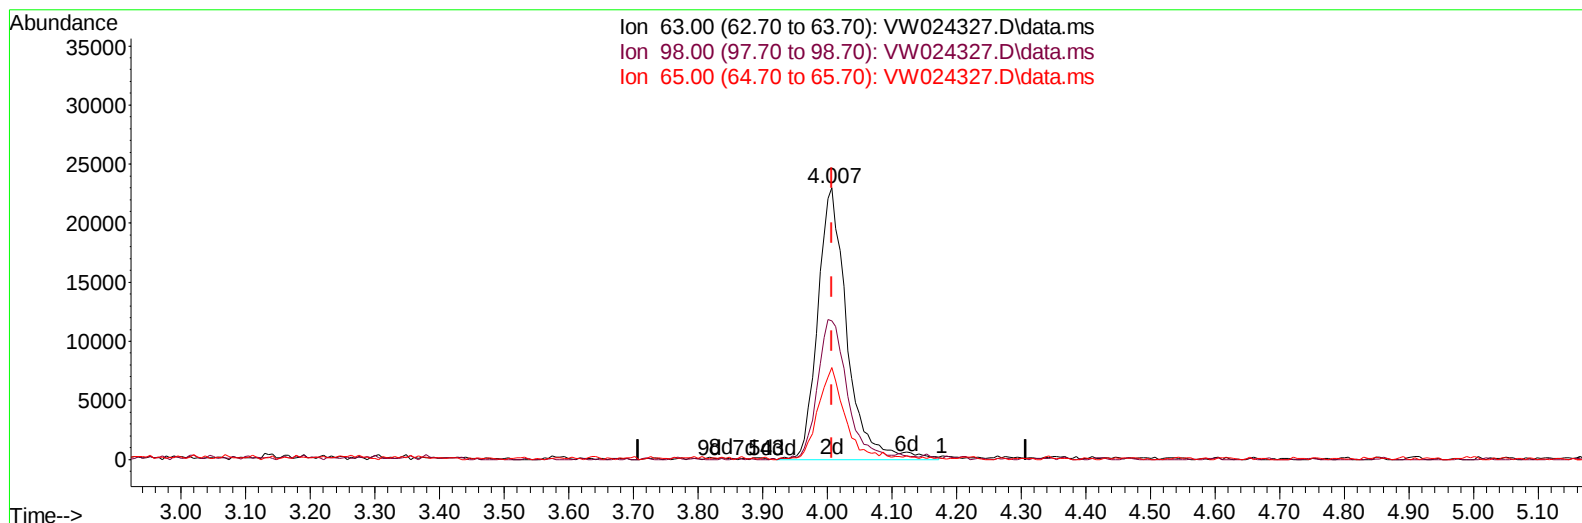

TIC: VW024327.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.007min (+ 0.000) 12.37 ug/L m

response 72291

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.50	0.24#
65.00	23.50	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082422\
 Data File : VW024327.D
 Acq On : 24 Aug 2022 17:25
 Operator : SY/VA
 Sample : N4322-01RE
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY163RE

Manual IntegrationsAPPROVED

Quant Time: Aug 25 01:33:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 25 01:31:24 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/25/2022
 Supervised By :Mahesh Dadoda 08/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		245373	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		199378	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		44833	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		112583	21.951	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	87.800%		
7) Chloroethane-d5	2.873	69		94455	29.563	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	118.240%		
11) 1,1-Dichloroethene-d2	4.007	63		72291m	12.368	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	49.480%		
21) 2-Butanone-d5	7.080	46		48573	50.904	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	101.800%		
24) Chloroform-d	7.647	84		159469	21.479	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	85.920%		
26) 1,2-Dichloroethane-d4	8.299	65		97558	23.668	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	94.680%		
32) Benzene-d6	8.269	84		271638	23.101	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	92.400%		
36) 1,2-Dichloropropane-d6	9.274	67		94922	27.341	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	109.360%		
41) Toluene-d8	10.323	98		205255	18.675	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	74.720%		
43) trans-1,3-Dichloroprop...	10.579	79		29336	19.292	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	77.160%		
47) 2-Hexanone-d5	10.921	63		35112	54.755	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	109.520%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		89693	26.628	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	106.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152		35265	21.495	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	85.960%		
Target Compounds							
						Qvalue	
13) Acetone	4.123	43		17248	24.551	ug/L	88
14) Carbon disulfide	4.367	76		11740	1.244	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082422\
Data File : VW024327.D
Acq On : 24 Aug 2022 17:25
Operator : SY/VA
Sample : N4322-01RE
Misc : 5.64g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY163RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/25/2022
Supervised By :Mahesh Dadoda 08/25/2022

Quant Time: Aug 25 01:33:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 25 01:31:24 2022
Response via : Initial Calibration

