




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026857.D
 Acq On : 24 Aug 2023 15:38
 Operator : SY/MD
 Sample : 04113-05
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYL2

Manual IntegrationsAPPROVED

Quant Time: Aug 25 02:26:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 02:23:07 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/25/2023
 Supervised By :Mahesh Dadoda 08/26/2023

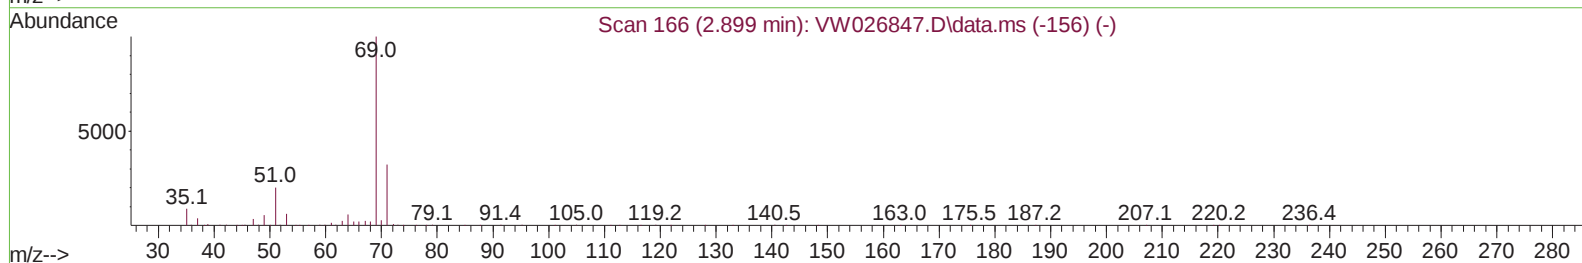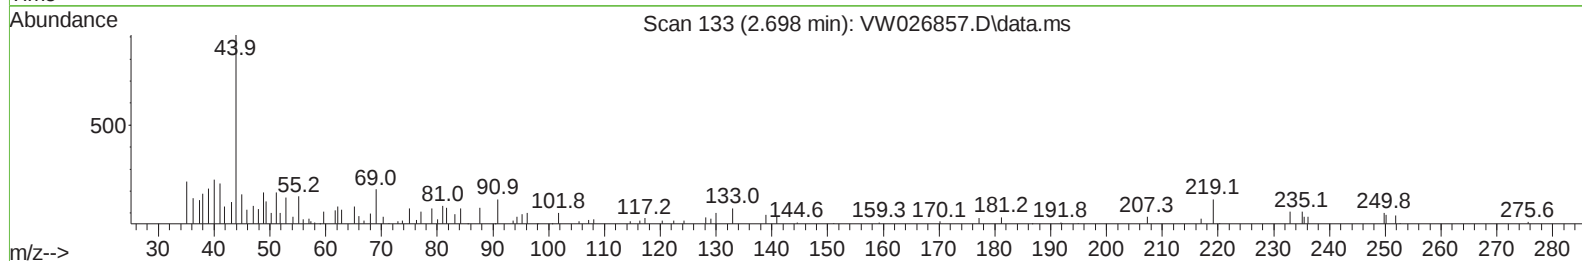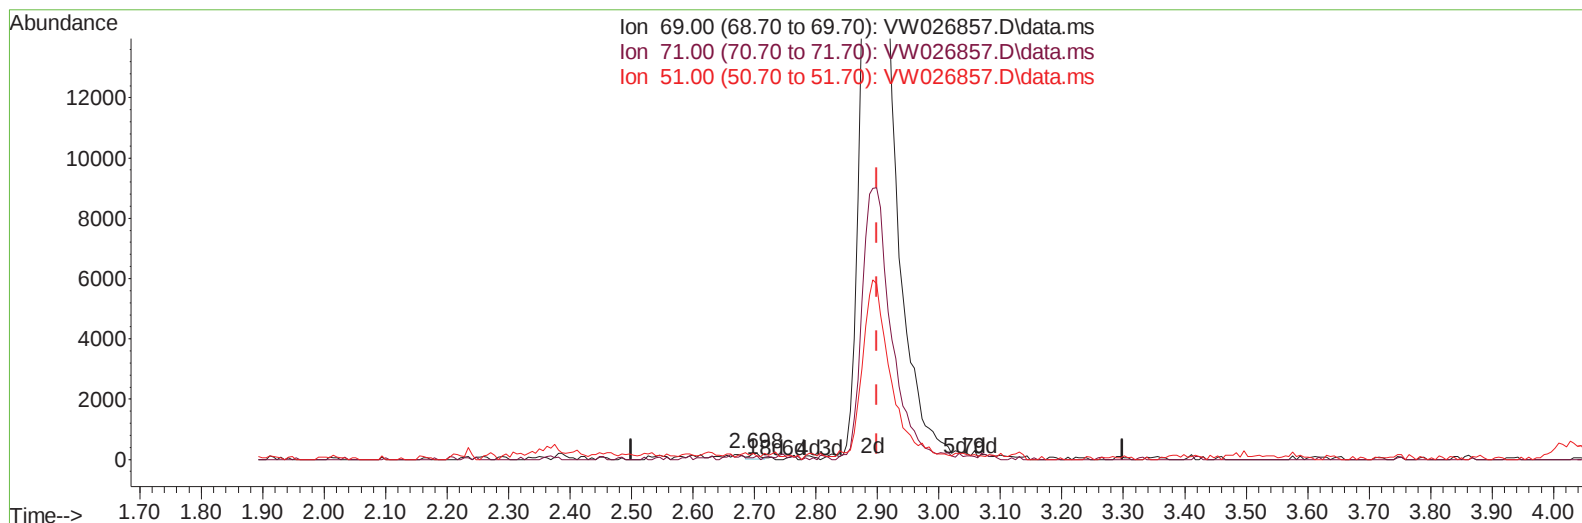

TIC: VW026857.D\data.ms

(7) Chloroethane-d5 (S)

2.698min (-0.201) 0.02 ug/L

response	198	
Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	30.30
51.00	28.30	25.76
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026857.D
 Acq On : 24 Aug 2023 15:38
 Operator : SY/MD
 Sample : 04113-05
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYL2

Manual IntegrationsAPPROVED

Quant Time: Aug 25 02:26:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 02:23:07 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/25/2023
 Supervised By :Mahesh Dadoda 08/26/2023

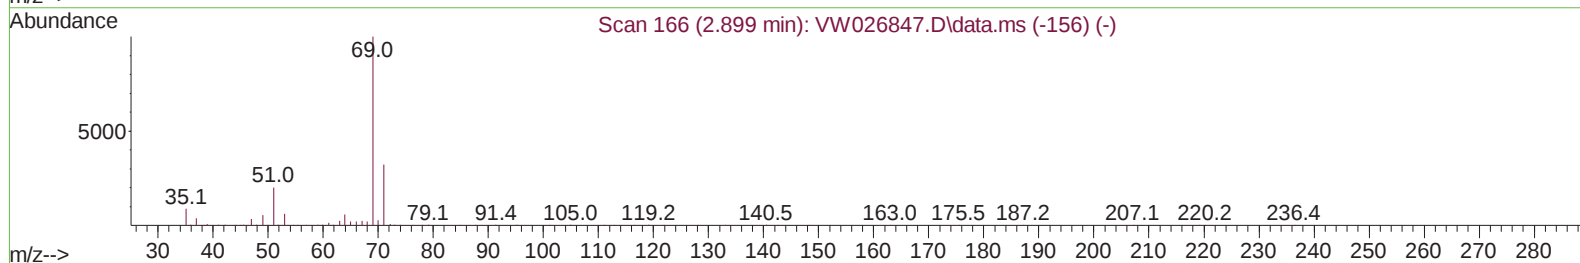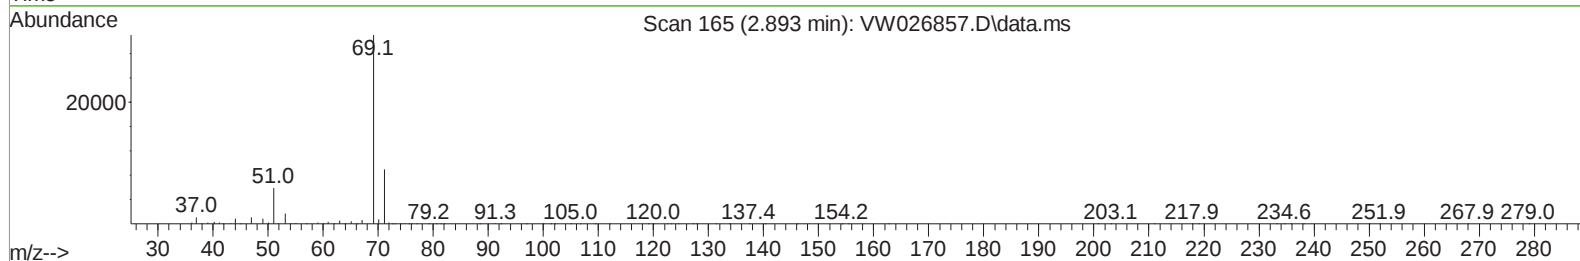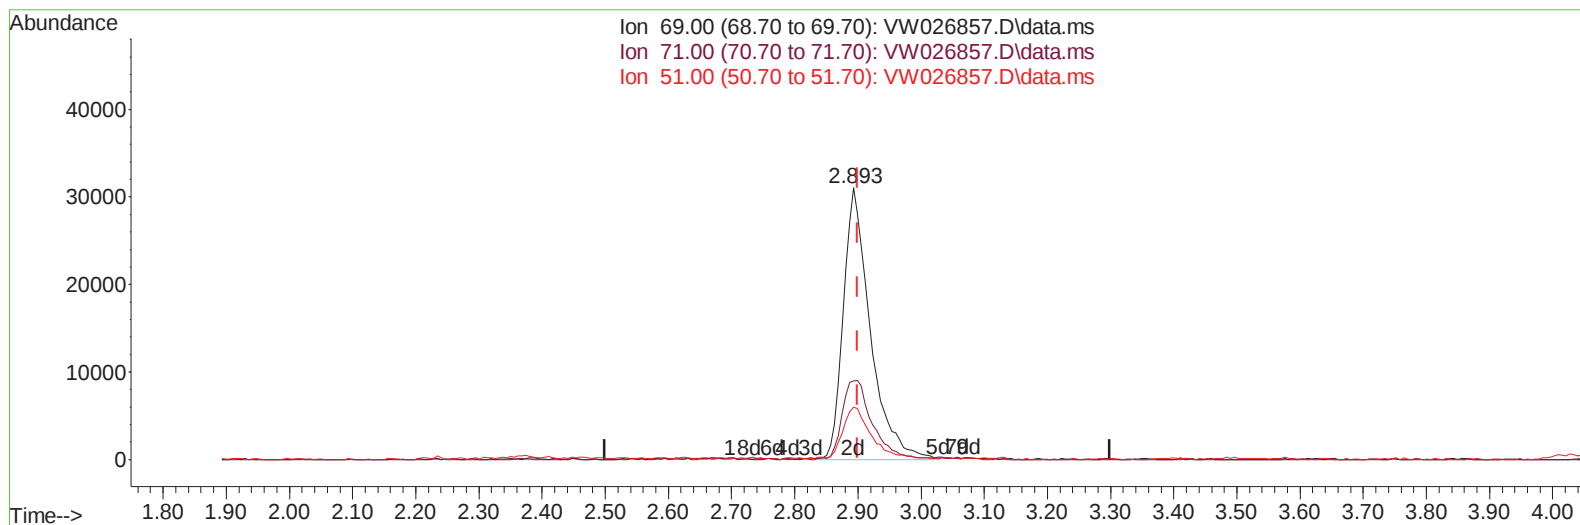

TIC: VW026857.D\data.ms

(7) Chloroethane-d5 (S)

2.893min (-0.006) 9.97 ug/L m

response 92143

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	0.07#
51.00	28.30	0.06#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
Data File : VW026857.D
Acq On : 24 Aug 2023 15:38
Operator : SY/MD
Sample : 04113-05
Misc : 5.49g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYL2

Manual IntegrationsAPPROVED

Quant Time: Aug 25 02:26:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 25 02:23:07 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/25/2023
Supervised By :Mahesh Dadoda 08/26/2023

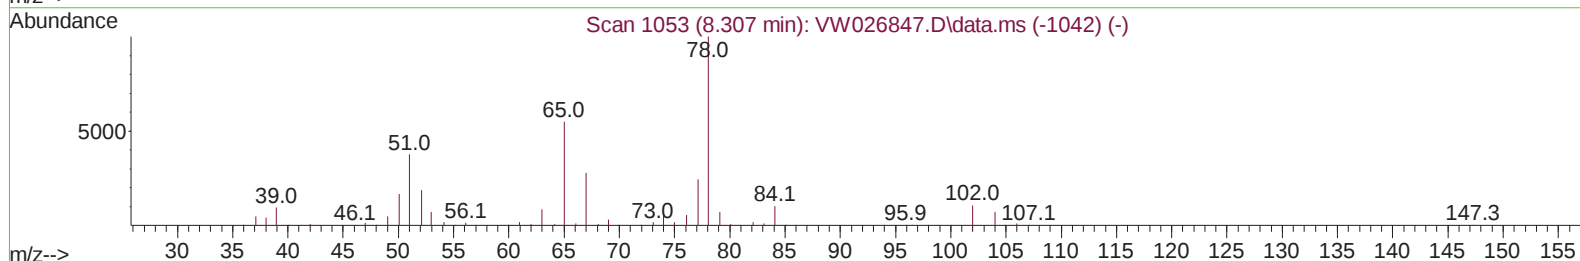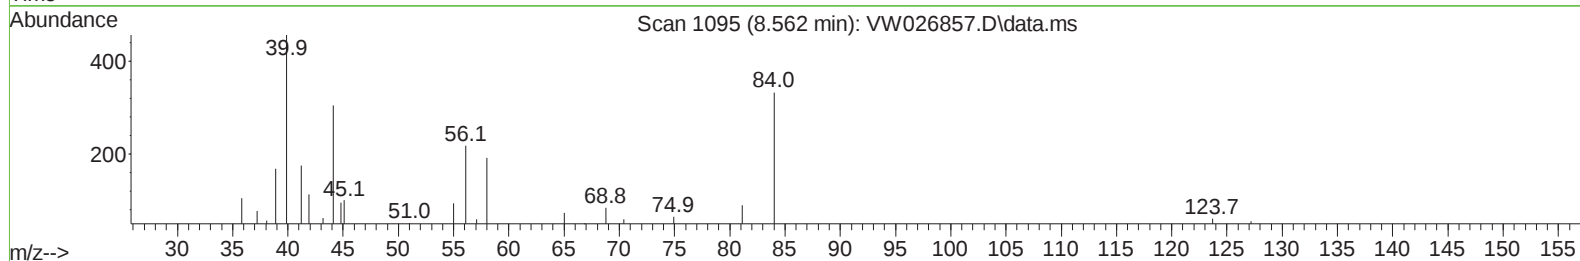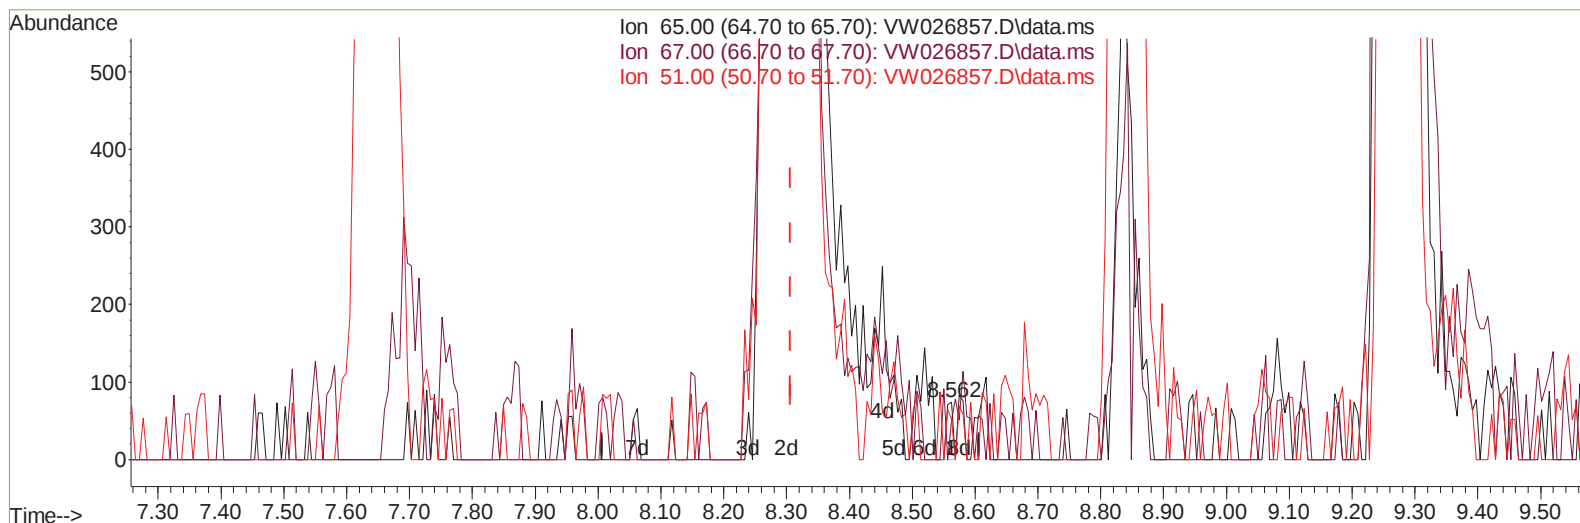

TIC: VW026857.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.562min (+ 0.256) 0.00 ug/L

response 53

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	62.26
51.00	112.90	81.13
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026857.D
 Acq On : 24 Aug 2023 15:38
 Operator : SY/MD
 Sample : 04113-05
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYL2

Manual IntegrationsAPPROVED

Quant Time: Aug 25 02:26:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 02:23:07 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/25/2023
 Supervised By :Mahesh Dadoda 08/26/2023

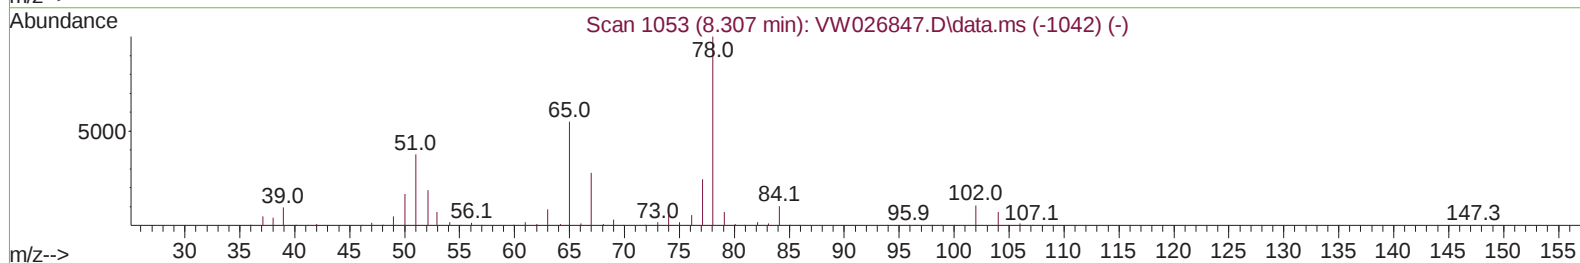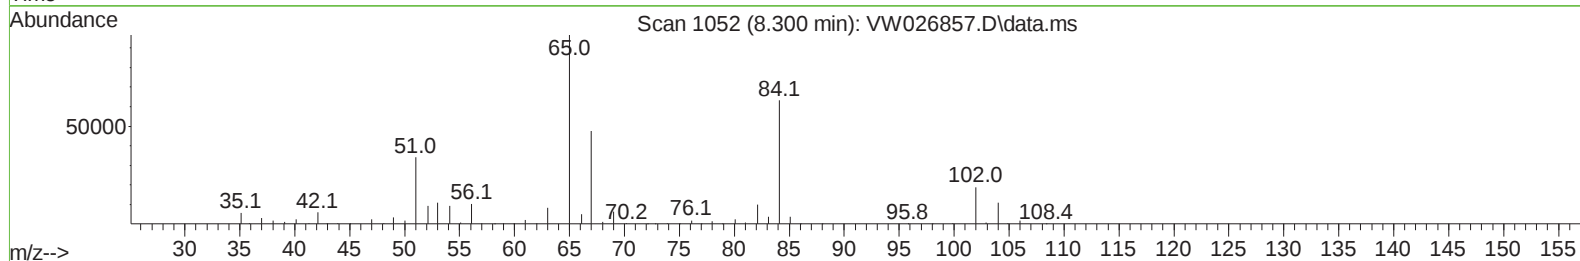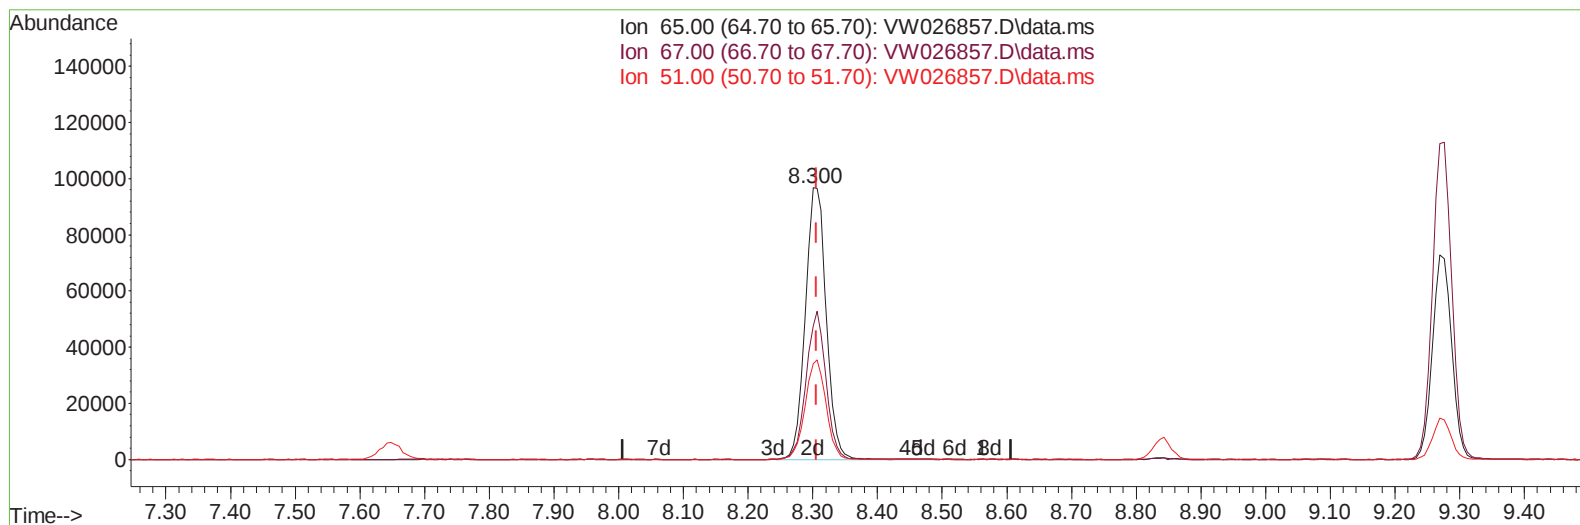

TIC: VW026857.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.300min (-0.006) 15.48 ug/L m

response 216820

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	0.02#
51.00	112.90	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026857.D
 Acq On : 24 Aug 2023 15:38
 Operator : SY/MD
 Sample : 04113-05
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYL2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/25/2023
 Supervised By :Mahesh Dadoda 08/26/2023

Quant Time: Aug 25 02:26:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 02:23:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	756024	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	570086	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	144447	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	94850	7.632	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	30.520%	
7) Chloroethane-d5	2.893	69	92143m	9.970	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	39.880%	
11) 1,1-Dichloroethene-d2	4.021	65	64330	10.524	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	42.080%#	
21) 2-Butanone-d5	7.075	46	108786	30.454	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	60.900%	
24) Chloroform-d	7.648	84	378752	14.927	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	59.720%	
26) 1,2-Dichloroethane-d4	8.300	65	216820m	15.484	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	61.920%#	
32) Benzene-d6	8.276	84	708732	18.039	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	72.160%	
36) 1,2-Dichloropropane-d6	9.276	67	233545	19.083	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	76.320%	
41) Toluene-d8	10.324	98	540567	16.028	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	64.120%	
43) trans-1,3-Dichloroprop...	10.580	79	70424	13.937	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	55.760%	
47) 2-Hexanone-d5	10.922	63	50905	39.585	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	79.160%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	185555	19.199	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	76.800%	
66) 1,2-Dichlorobenzene-d4	13.848	152	101016	19.538	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	78.160%	
Target Compounds						
13) Acetone	4.118	43	13178	3.710	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
Data File : VW026857.D
Acq On : 24 Aug 2023 15:38
Operator : SY/MD
Sample : 04113-05
Misc : 5.49g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYL2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/25/2023
Supervised By :Mahesh Dadoda 08/26/2023

Quant Time: Aug 25 02:26:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 25 02:23:07 2023
Response via : Initial Calibration

