




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026879.D
 Acq On : 25 Aug 2023 02:29
 Operator : SY/MD
 Sample : 04157-06
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHU2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/25/2023
 Supervised By :Mahesh Dadoda 08/26/2023

Quant Time: Aug 25 05:25:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 05:00:16 2023
 Response via : Initial Calibration

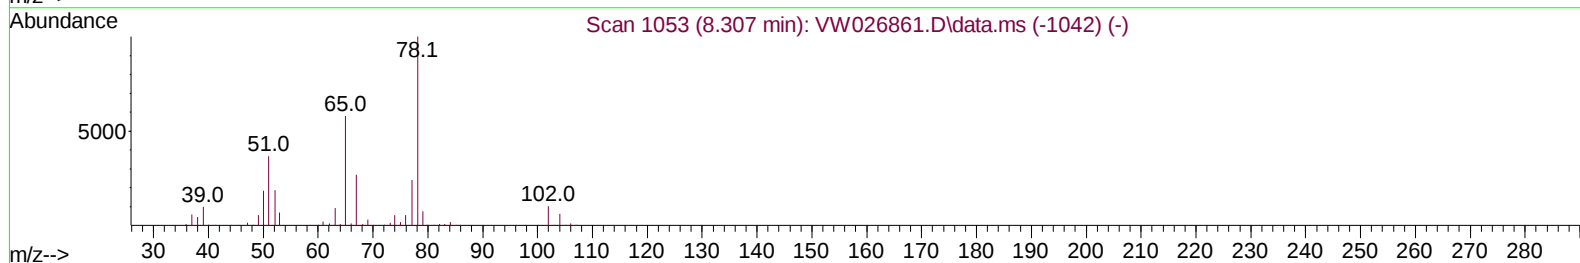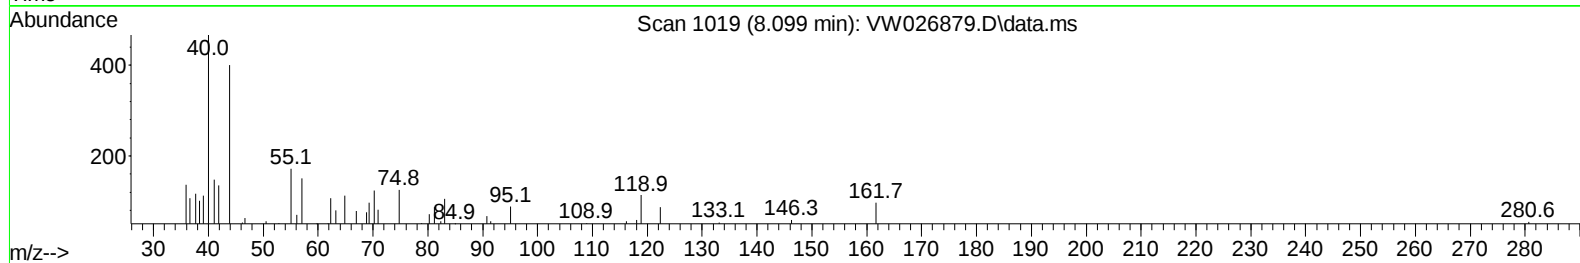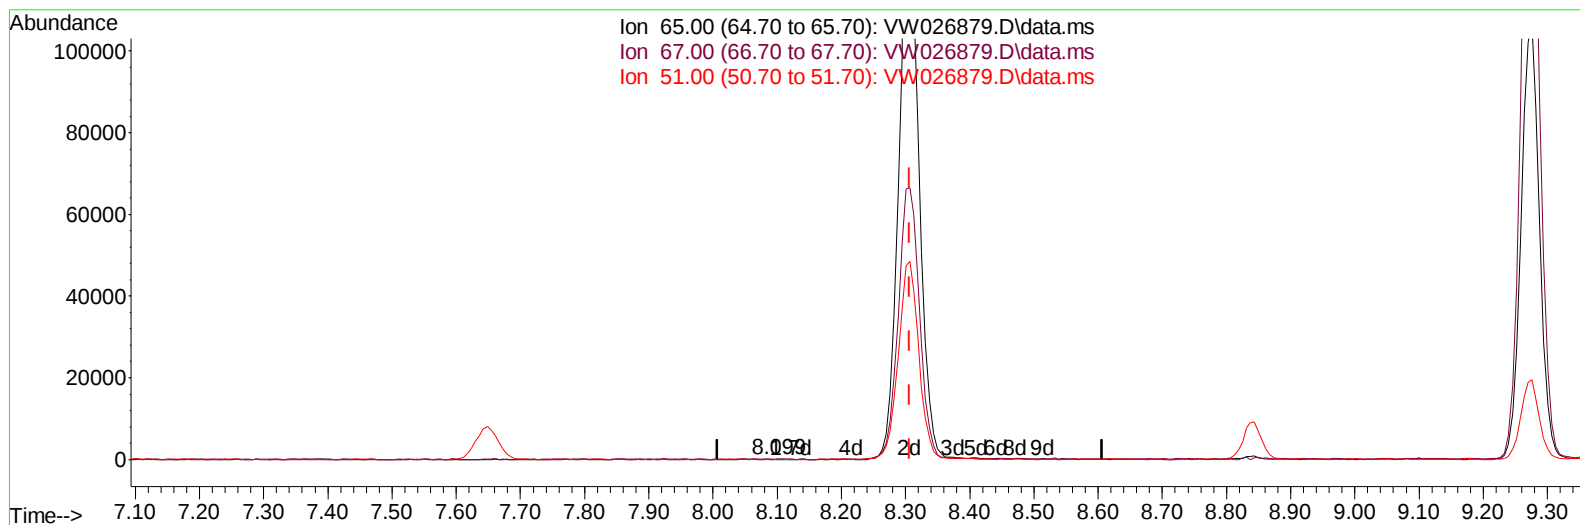

TIC: VW026879.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.099min (-0.207) 0.00 ug/L

response 83

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	61.45
51.00	112.90	80.72
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026879.D
 Acq On : 25 Aug 2023 02:29
 Operator : SY/MD
 Sample : 04157-06
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHU2

Manual IntegrationsAPPROVED

Quant Time: Aug 25 05:25:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 05:00:16 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/25/2023
 Supervised By :Mahesh Dadoda 08/26/2023

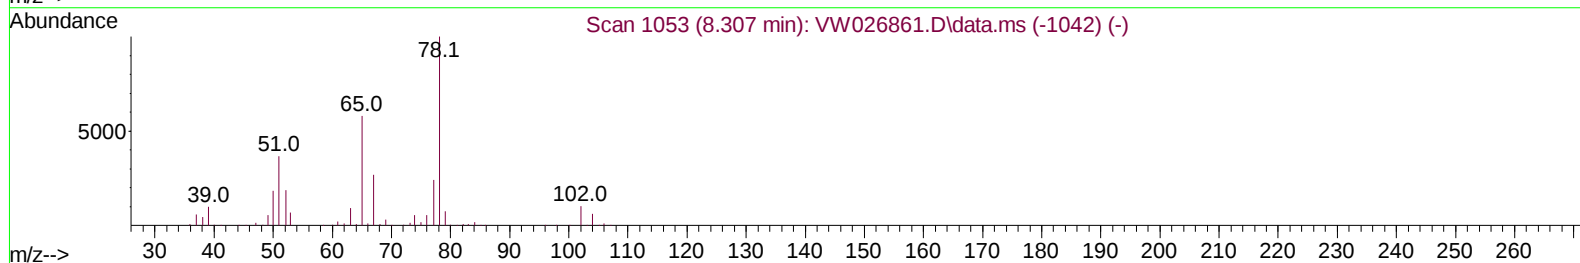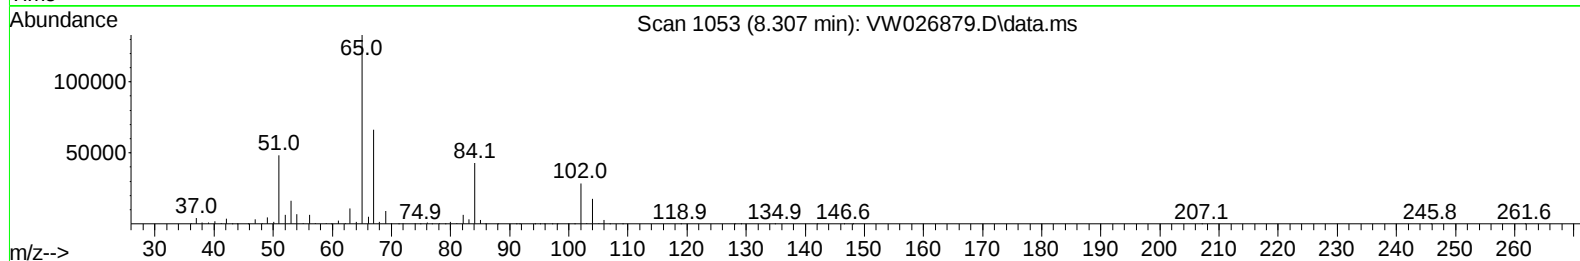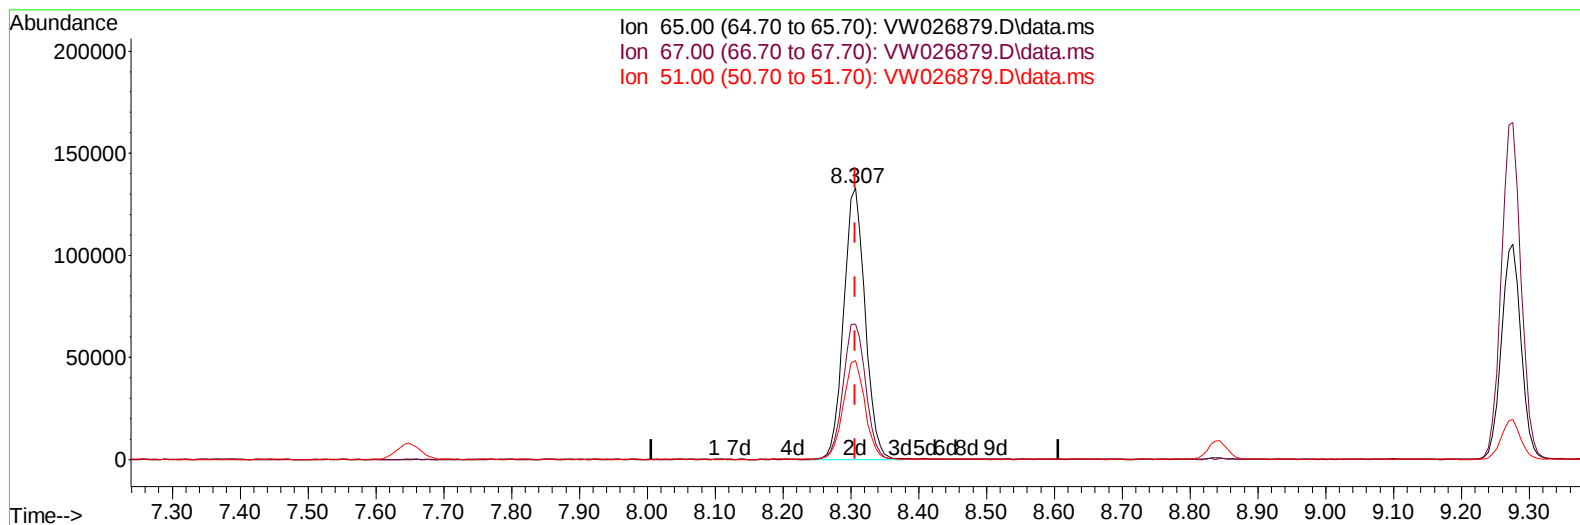

TIC: VW026879.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 16.53 ug/L m

response 289573

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	0.02#
51.00	112.90	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026879.D
 Acq On : 25 Aug 2023 02:29
 Operator : SY/MD
 Sample : 04157-06
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHU2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/25/2023
 Supervised By :Mahesh Dadoda 08/26/2023

Quant Time: Aug 25 05:25:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 05:00:16 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		945851	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		888494	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		477910	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		162624	10.459	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	41.840%		
7) Chloroethane-d5	2.893	69		156442	13.531	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.120%		
11) 1,1-Dichloroethene-d2	4.021	65		90811	11.875	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	47.480%		
21) 2-Butanone-d5	7.081	46		163752	36.642	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	73.280%		
24) Chloroform-d	7.648	84		531221	16.734	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	66.920%		
26) 1,2-Dichloroethane-d4	8.307	65		289573m	16.529	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	66.120%#		
32) Benzene-d6	8.276	84		1035306	16.907	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	67.640%		
36) 1,2-Dichloropropane-d6	9.276	67		335529	17.591	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	70.360%		
41) Toluene-d8	10.325	98		924018	17.579	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	70.320%		
43) trans-1,3-Dichloroprop...	10.581	79		128430	16.308	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	65.240%		
47) 2-Hexanone-d5	10.922	63		88543	44.178	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	88.360%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		294687	19.563	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	78.240%		
66) 1,2-Dichlorobenzene-d4	13.854	152		352115	20.585	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	82.320%		
Target Compounds							
16) Methylene chloride	4.923	84		46811	2.558	ug/L	88
19) 1,1-Dichloroethane	6.216	63		280241	8.728	ug/L	97
20) cis-1,2-Dichloroethene	7.173	96		33474	1.996	ug/L	90
46) Tetrachloroethene	10.861	164		38441	3.211	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
Data File : VW026879.D
Acq On : 25 Aug 2023 02:29
Operator : SY/MD
Sample : 04157-06
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHU2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/25/2023
Supervised By :Mahesh Dadoda 08/26/2023

Quant Time: Aug 25 05:25:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 25 05:00:16 2023
Response via : Initial Calibration

