

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
 Data File : VW026878.D
 Acq On : 25 Aug 2023 02:05
 Operator : SY/MD
 Sample : VIBLK491
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK491

Quant Time: Aug 25 05:25:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 05:00:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	545434	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	533444	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	293885	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	154034	17.179	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.720%
7) Chloroethane-d5	2.893	69	126174	18.924	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.680%
11) 1,1-Dichloroethene-d2	4.027	65	74952	16.996	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.000%
21) 2-Butanone-d5	7.081	46	112198	43.537	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.080%
24) Chloroform-d	7.648	84	368042	20.105	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.400%
26) 1,2-Dichloroethane-d4	8.307	65	216561	21.437	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.760%
32) Benzene-d6	8.276	84	770296	20.952	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.800%
36) 1,2-Dichloropropane-d6	9.276	67	236422	20.645	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.560%
41) Toluene-d8	10.325	98	697611	22.105	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.440%
43) trans-1,3-Dichloroprop...	10.581	79	96656	20.442	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.760%
47) 2-Hexanone-d5	10.922	63	64935	53.963	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.920%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	204508	22.613	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	252232	23.979	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.920%
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	29161	2.764	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082423\
Data File : VW026878.D
Acq On : 25 Aug 2023 02:05
Operator : SY/MD
Sample : VIBLK491
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK491


Quant Time: Aug 25 05:25:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 25 05:00:16 2023
Response via : Initial Calibration

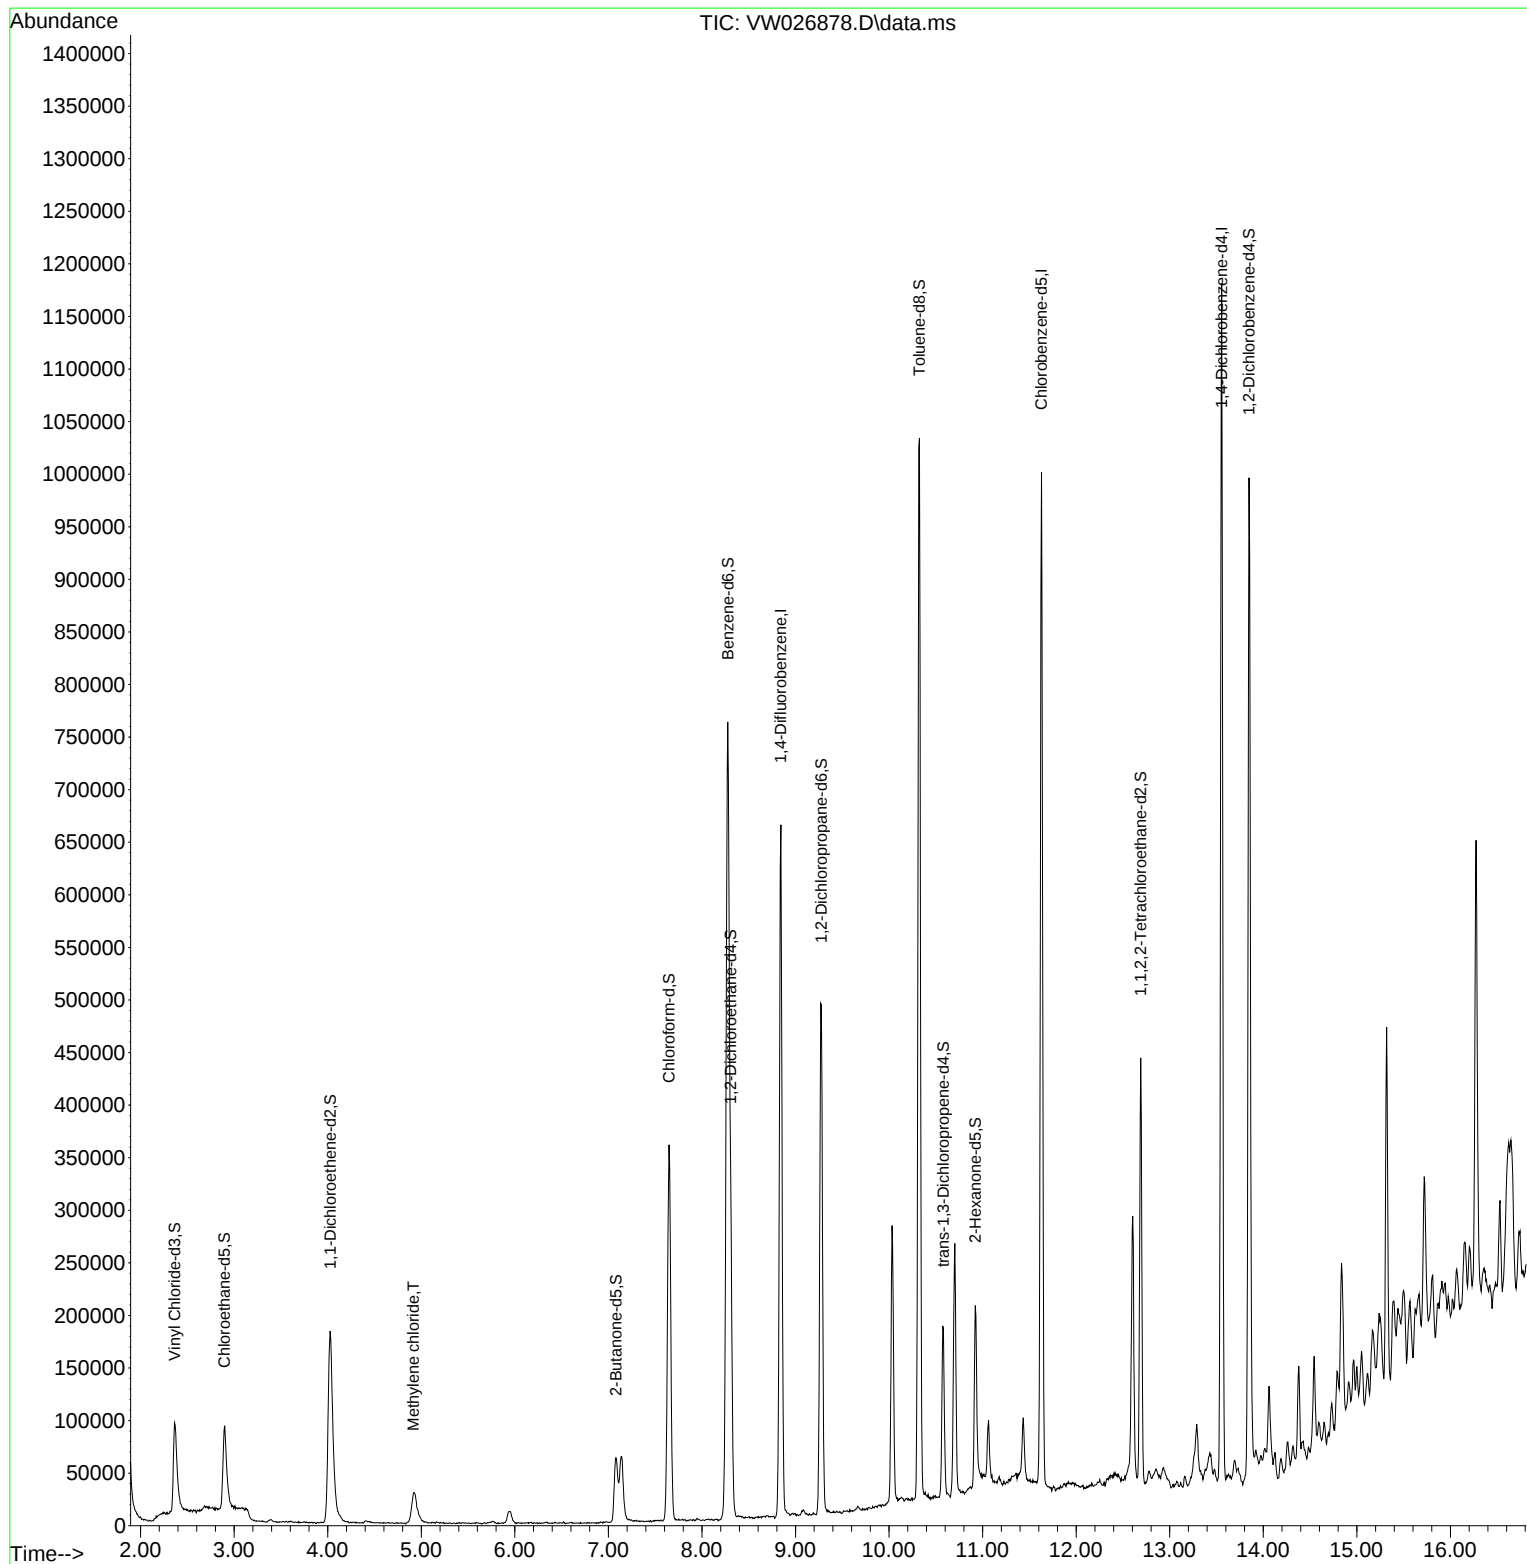

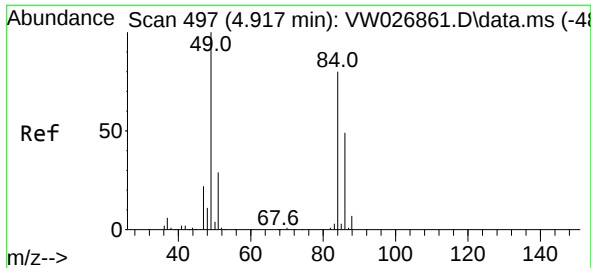

#16
Methylene chloride
Concen: 2.764 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW026878.D
Acq: 25 Aug 2023 02:05

Instrument :
MSVOA_W
ClientSampleId :
VIBLK491

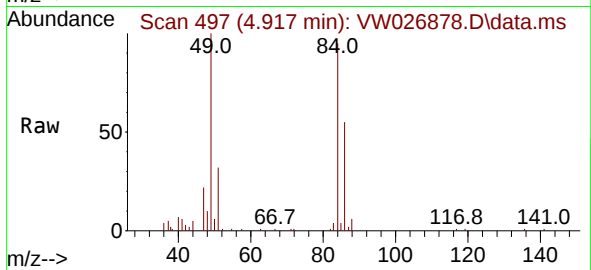

Tgt Ion:	84	Resp:	29161
Ion	Ratio	Lower	Upper
84	100		
86	58.1	43.5	80.9
49	105.5	96.0	178.2

