

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082521\
 Data File : VW019903.D
 Acq On : 25 Aug 2021 18:48
 Operator : SY/VA
 Sample : M3526-16
 Misc : 5.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7C6

Quant Time: Aug 26 01:12:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 26 01:07:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	569266	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	512172	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	241060	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	162886	18.468	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.880%
7) Chloroethane-d5	2.898	69	132769	17.150	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.600%
11) 1,1-Dichloroethene-d2	4.026	63	219817	14.362	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.440%
21) 2-Butanone-d5	7.080	46	57926	32.332	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.660%
24) Chloroform-d	7.653	84	294209	18.793	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.160%
26) 1,2-Dichloroethane-d4	8.311	65	150445	17.832	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.320%
32) Benzene-d6	8.281	84	596595	20.429	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.720%
36) 1,2-Dichloropropane-d6	9.275	67	175076	19.797	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.200%
41) Toluene-d8	10.323	98	543205	20.298	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.200%
43) trans-1,3-Dichloroprop...	10.579	79	66319	18.153	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.600%
47) 2-Hexanone-d5	10.927	63	40900	33.199	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.400%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	116577	16.196	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	64.800%
66) 1,2-Dichlorobenzene-d4	13.853	152	164010	19.835	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.320%
Target Compounds						Qvalue
16) Methylene chloride	4.916	84	47324	4.844	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082521\
Data File : VW019903.D
Acq On : 25 Aug 2021 18:48
Operator : SY/VA
Sample : M3526-16
Misc : 5.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW7C6

Quant Time: Aug 26 01:12:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 26 01:07:03 2021
Response via : Initial Calibration

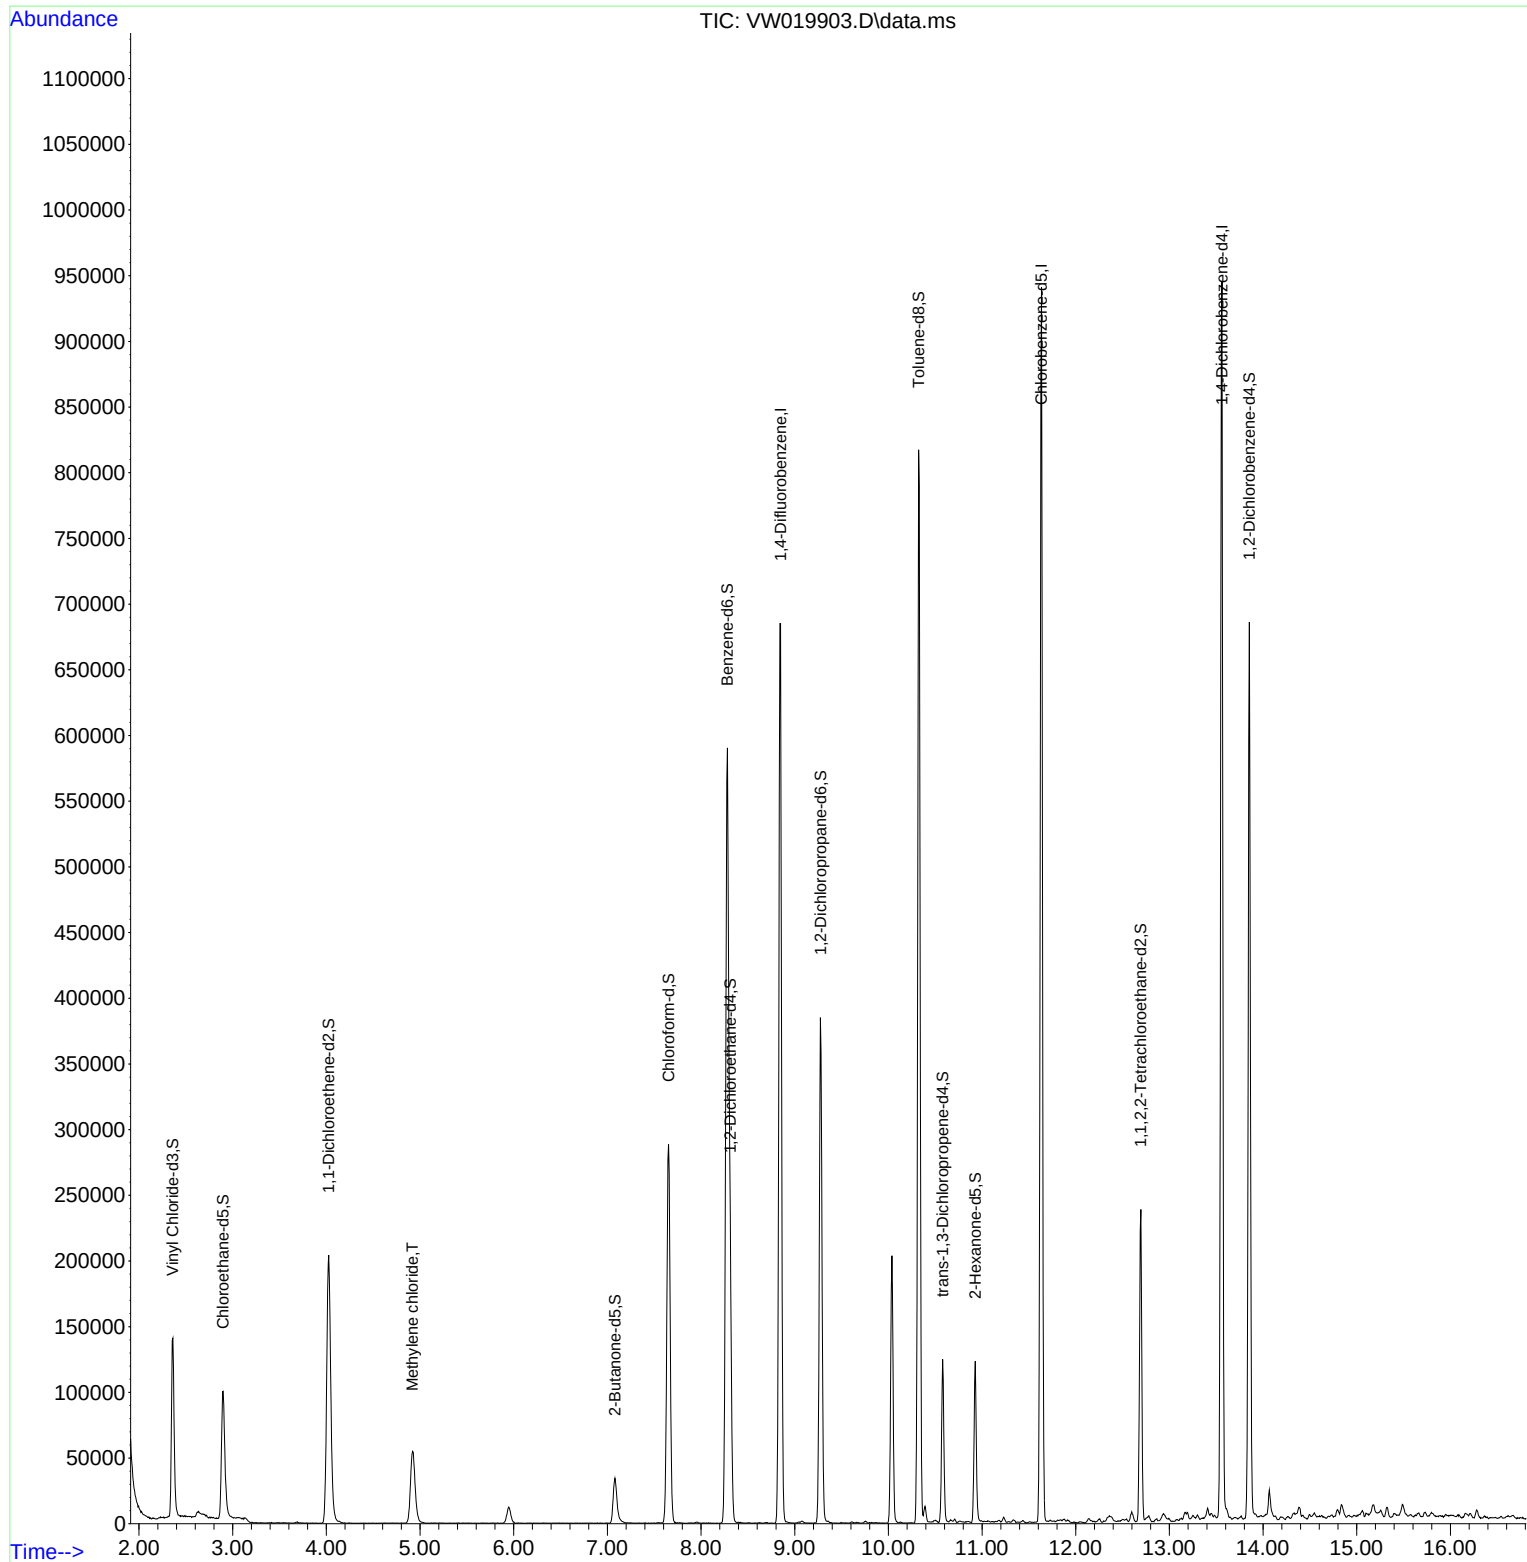

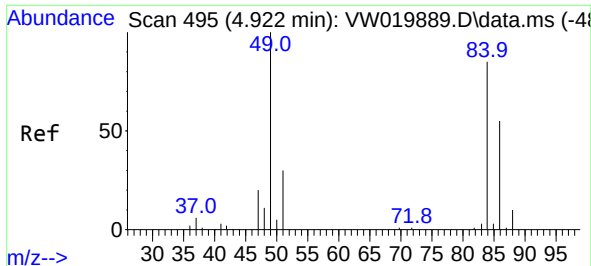

#16
Methylene chloride
Concen: 4.844 ug/L
RT: 4.916 min Scan# 494
Delta R.T. -0.006 min
Lab File: VW019903.D
Acq: 25 Aug 2021 18:48

Instrument :
MSVOA_W
ClientSampleId :
EW7C6

Tgt Ion: 84 Resp: 47324

Ion	Ratio	Lower	Upper
84	100		
86	61.0	45.3	84.1
49	117.6	86.6	160.8

