


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW082620\
 Data File : VW016353.D
 Acq On : 26 Aug 2020 08:16
 Operator : SY/VA
 Sample : BFB16
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB16

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082420S.M
 Title : VOC Analysis
 Last Update : Thu Aug 27 02:40:32 2020

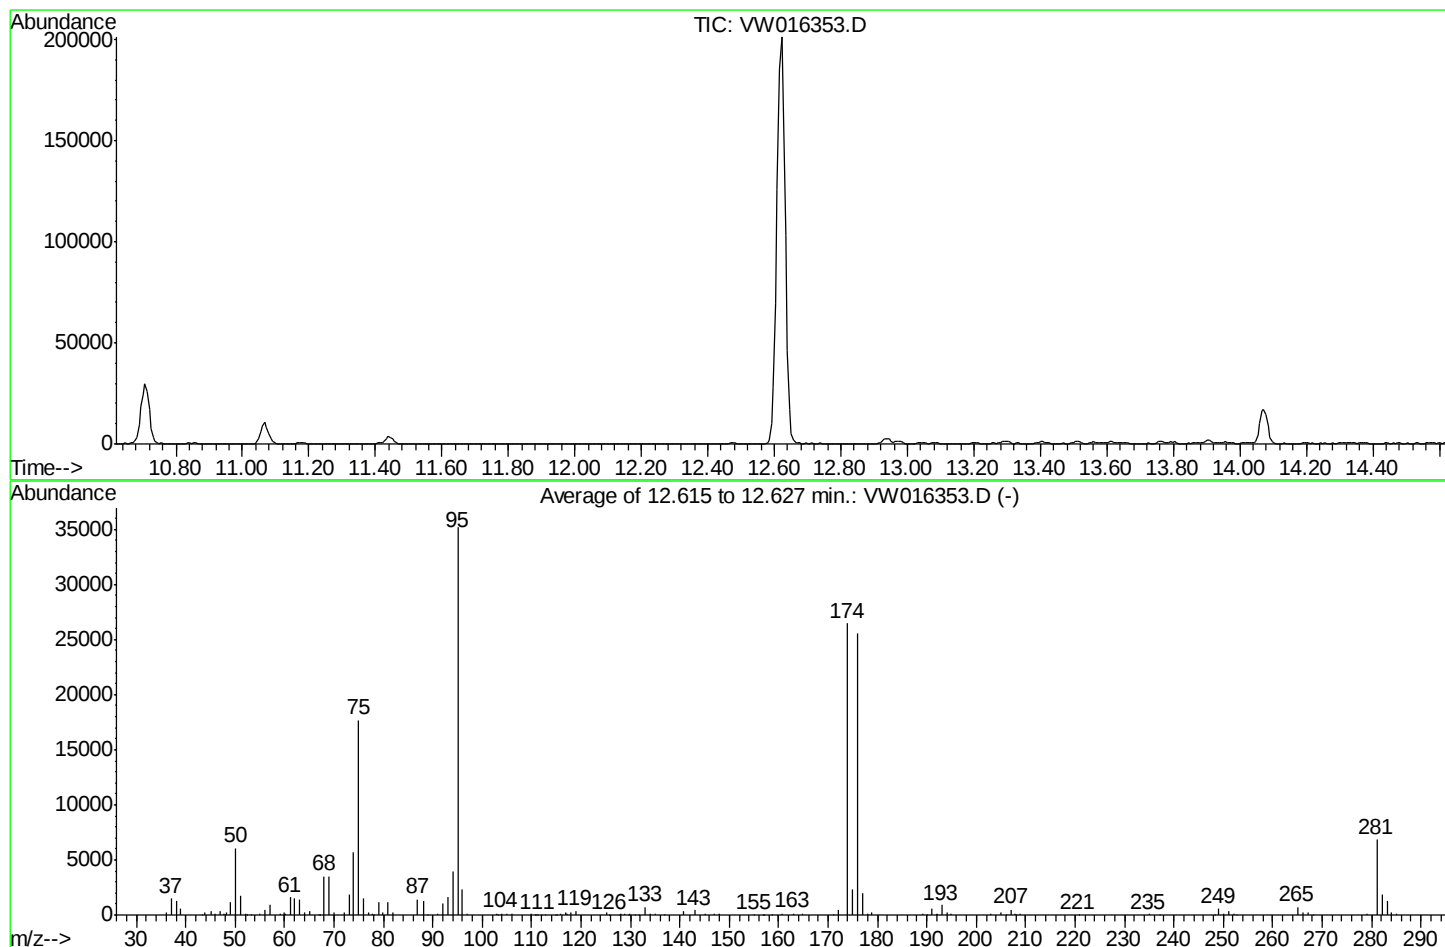

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	6080	PASS
75	95	30	80	50.2	17677	PASS
95	95	100	100	100.0	35181	PASS
96	95	5	9	6.7	2355	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.3	26477	PASS
175	174	5	9	8.6	2270	PASS
176	174	95	101	96.7	25592	PASS
177	176	5	9	7.7	1973	PASS

m/z	Abundance
35.90	201.0
37.00	1424.0
38.10	1201.0
39.00	572.0
39.90	158.0
43.30	69.0
43.90	263.0
45.10	335.0
46.00	73.0
47.00	325.0
47.70	210.0
48.20	238.0
49.00	1290.0
50.10	6334.0
51.10	1688.0
52.00	98.0
55.10	81.0
56.10	437.0
57.00	1060.0
59.10	249.0
60.00	300.0
61.10	1669.0
62.00	1387.0
63.00	1360.0
64.10	341.0
65.10	417.0
68.00	3551.0
69.00	3617.0
70.00	256.0
71.90	181.0
73.00	1989.0
74.00	5532.0
75.00	17616.0
76.10	1231.0
77.00	115.0
77.70	83.0
78.90	1024.0
79.90	260.0
81.00	1126.0
82.00	228.0
86.90	1392.0
88.00	1171.0
89.00	108.0
91.00	169.0
92.10	1188.0
93.00	1660.0
94.00	4148.0
95.00	34664.0
96.00	2469.0
97.00	116.0
102.90	247.0
104.00	119.0
104.80	120.0
106.00	90.0
110.00	184.0
111.00	122.0
111.90	53.0
112.90	79.0
115.10	68.0
116.00	93.0
117.10	349.0
118.00	288.0
118.90	508.0
125.10	558.0
127.70	70.0
128.10	105.0
128.80	57.0
129.70	146.0
130.90	89.0
131.70	60.0
133.00	1004.0
133.90	314.0
135.00	183.0
140.90	481.0
143.00	477.0
145.00	217.0
146.90	131.0
148.10	108.0
158.70	59.0
160.80	147.0
162.90	278.0
164.90	193.0
172.00	484.0
174.00	21496.0
175.00	2127.0
176.00	22344.0
177.00	2122.0
178.00	205.0
178.90	279.0
189.20	121.0
190.00	63.0
191.10	1012.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

191.90	281.0
193.00	1496.0
194.00	292.0
195.00	152.0
203.00	256.0
205.10	302.0
206.10	68.0
207.20	470.0
208.00	162.0
208.90	62.0
220.70	68.0
235.00	169.0
237.00	52.0
248.30	107.0
249.00	774.0
250.10	268.0
251.00	441.0
252.00	136.0
252.60	57.0
265.10	1039.0
266.10	323.0
267.20	250.0
268.20	58.0
279.00	141.0
281.10	9954.0
282.10	2771.0
283.10	1597.0
284.00	437.0
285.10	182.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

m/z	Abundance
36.00	315.0
37.00	1722.0
38.00	1479.0
39.00	608.0
40.00	97.0
44.20	275.0
45.00	334.0
45.90	124.0
47.00	437.0
48.10	406.0
49.10	1219.0
50.00	6569.0
51.10	2084.0
52.00	94.0
55.00	146.0
56.00	609.0
57.00	866.0
59.00	64.0
60.00	338.0
61.10	1659.0
62.00	1686.0
63.00	1298.0
64.10	256.0
65.10	429.0
67.10	105.0
68.00	4074.0
69.00	3717.0
70.10	190.0
71.90	257.0
73.10	1872.0
74.00	6563.0
75.00	19320.0
76.10	1499.0
77.00	295.0
78.00	174.0
79.00	1331.0
80.00	352.0
81.00	1275.0
82.00	249.0
87.00	1686.0
87.90	1606.0
88.90	52.0
90.90	160.0
92.10	1046.0
93.00	1699.0
94.00	4161.0
95.00	38648.0
96.00	2467.0
97.00	147.0
102.80	191.0
103.80	241.0
104.90	101.0
105.90	125.0
110.00	140.0
110.60	51.0
111.20	148.0
112.80	52.0
114.80	82.0
115.10	70.0
116.00	237.0
116.80	289.0
118.10	284.0
118.90	302.0
124.90	104.0
125.80	116.0
128.00	154.0
128.80	118.0
129.90	214.0
133.10	762.0
133.80	83.0
135.00	164.0
136.90	76.0
140.90	450.0
142.90	466.0
145.00	155.0
146.90	181.0
147.90	91.0
156.70	57.0
158.70	57.0
160.80	162.0
163.00	144.0
165.00	62.0
171.00	70.0
172.10	571.0
174.00	31000.0
175.00	2485.0
176.00	26928.0
177.00	1930.0
178.00	137.0
178.90	253.0
189.00	84.0
191.00	629.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

192.90	781.0
194.10	170.0
194.90	124.0
202.90	120.0
205.10	185.0
207.10	675.0
207.80	55.0
208.20	51.0
235.00	107.0
249.10	683.0
250.10	145.0
251.10	292.0
252.10	101.0
265.10	761.0
266.00	314.0
267.10	252.0
278.90	99.0
281.10	6698.0
282.10	1942.0
283.00	1250.0
284.00	231.0
285.20	123.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

m/z	Abundance
36.00	216.0
37.00	1294.0
38.00	1143.0
39.00	414.0
40.10	64.0
43.90	315.0
45.00	321.0
46.90	347.0
47.90	109.0
49.00	1125.0
50.00	5339.0
51.00	1438.0
52.30	159.0
53.10	77.0
54.90	97.0
55.90	483.0
57.00	875.0
58.90	65.0
60.20	195.0
61.00	1513.0
62.00	1343.0
63.10	1391.0
64.00	222.0
64.90	303.0
66.80	70.0
67.10	76.0
68.00	3004.0
69.00	3243.0
70.00	134.0
72.00	253.0
73.00	1702.0
74.00	5119.0
75.00	16095.0
76.00	1644.0
77.10	157.0
77.70	119.0
79.00	971.0
79.90	240.0
80.90	1012.0
82.00	276.0
87.00	1271.0
88.10	1101.0
90.90	76.0
92.00	922.0
93.10	1445.0
94.10	3634.0
95.00	32232.0
96.00	2129.0
96.90	82.0
103.10	78.0
104.00	126.0
104.90	56.0
105.90	96.0
114.90	73.0
115.90	137.0
116.90	255.0
118.10	300.0
119.00	290.0
125.00	169.0
128.00	167.0
128.80	131.0
129.90	191.0
133.00	381.0
137.00	92.0
140.70	248.0
143.10	419.0
145.00	131.0
146.90	103.0
148.00	122.0
155.10	62.0
157.10	71.0
171.00	72.0
172.00	471.0
174.00	26936.0
175.00	2198.0
176.00	27504.0
177.00	1869.0
178.00	110.0
178.80	86.0
191.10	272.0
192.10	59.0
192.90	414.0
194.10	88.0
205.00	64.0
207.10	331.0
209.00	167.0
235.00	66.0
249.00	279.0
250.00	57.0
251.10	177.0
264.90	378.0
266.10	154.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

267.00	95.0
281.10	3846.0
282.10	810.0
283.20	859.0
284.10	99.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

Scan 1750 (12.573 min): VW016353.D
BFB16

m/z	Abundance
39.90	126.0
44.10	98.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16