

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082621\
 Data File : VW019914.D
 Acq On : 26 Aug 2021 13:59
 Operator : SY/VA
 Sample : VIBLK416
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK416

Manual Integrations
 APPROVED

MMDadoda
 8/27/2021 4:44:05 PM

Quant Time: Aug 27 01:03:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 27 00:59:57 2021
 Response via : Initial Calibration

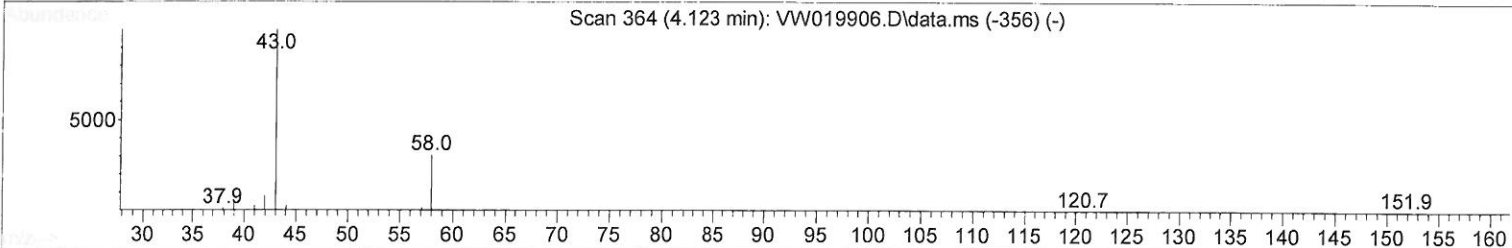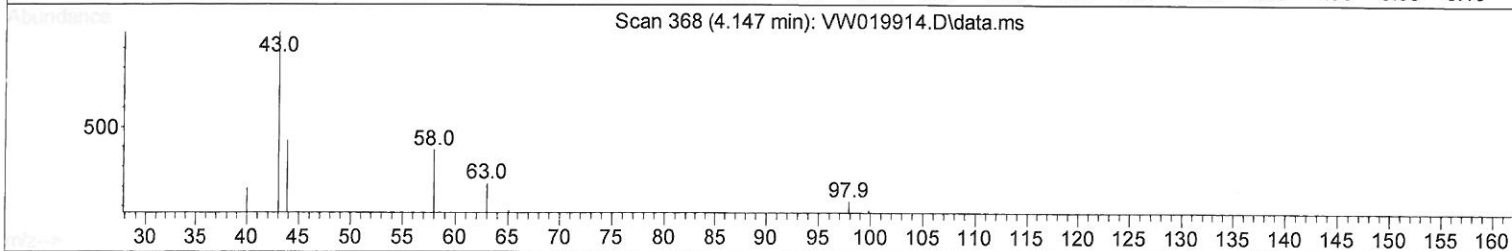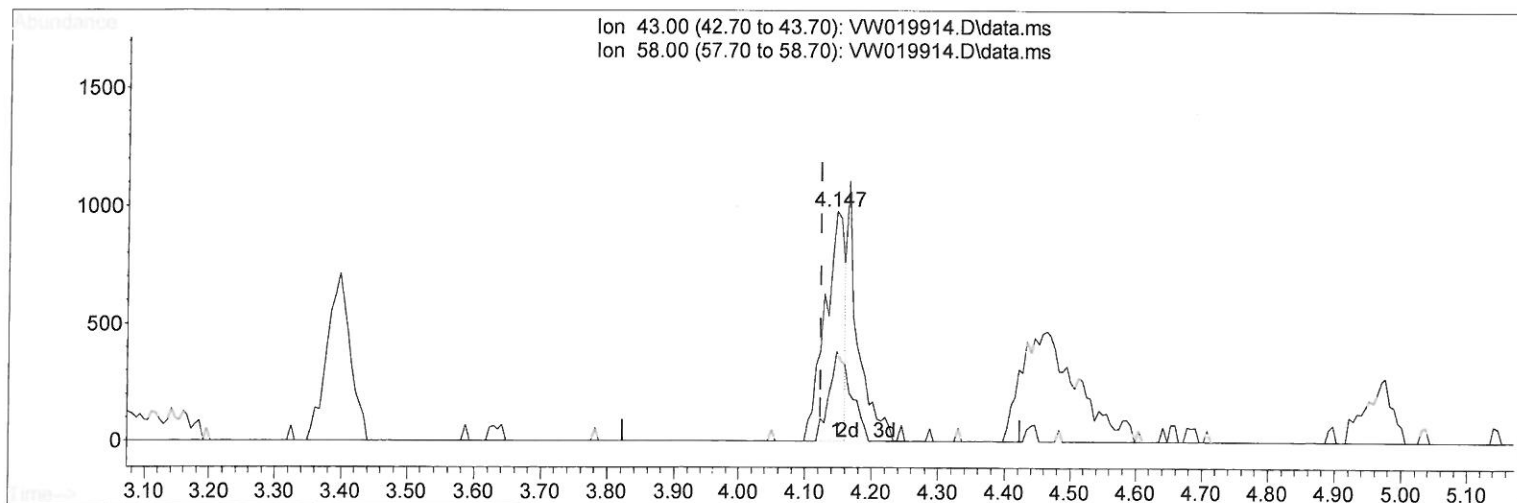

TIC: VW019914.D\data.ms

(13) Acetone (T)

4.147min (+ 0.024) 2.06 ug/L

response 2045

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	43.57
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082621\
 Data File : VW019914.D
 Acq On : 26 Aug 2021 13:59
 Operator : SY/VA
 Sample : VIBLK416
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1


Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK416

Manual Integrations
 APPROVED


MMDadoda
 8/27/2021 4:44:05 PM

Quant Time: Aug 27 01:03:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 27 00:59:57 2021
 Response via : Initial Calibration


Ion 43.00 (42.70 to 43.70): VW019914.D\data.ms
 Ion 58.00 (57.70 to 58.70): VW019914.D\data.ms

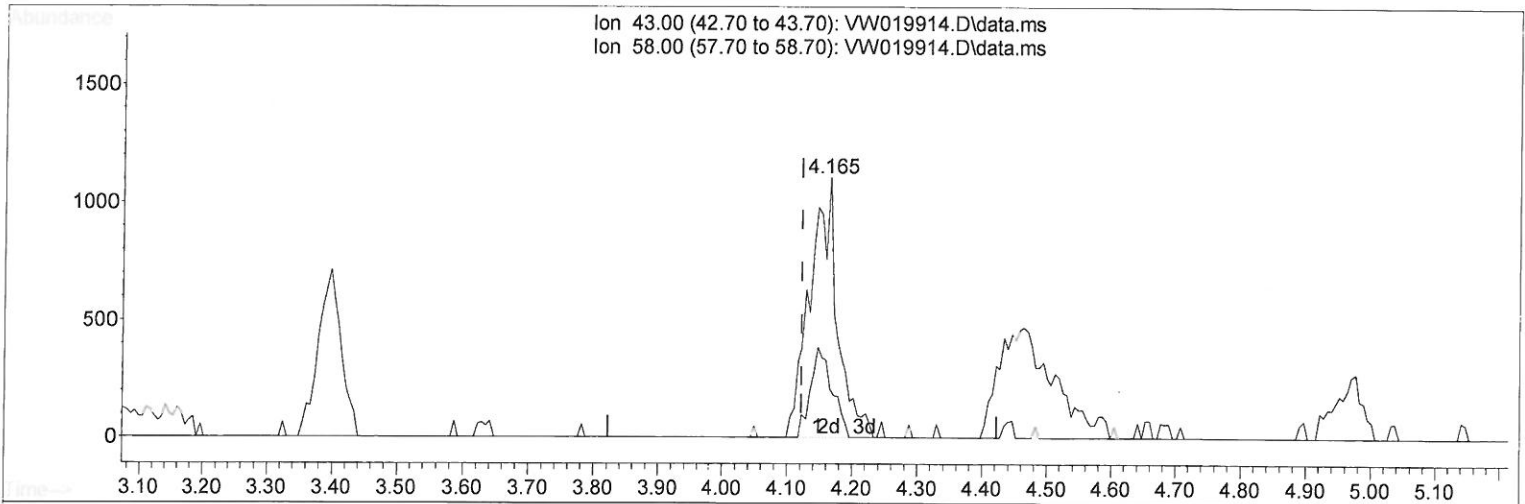

Scan 371 (4.165 min): VW019914.D\data.ms

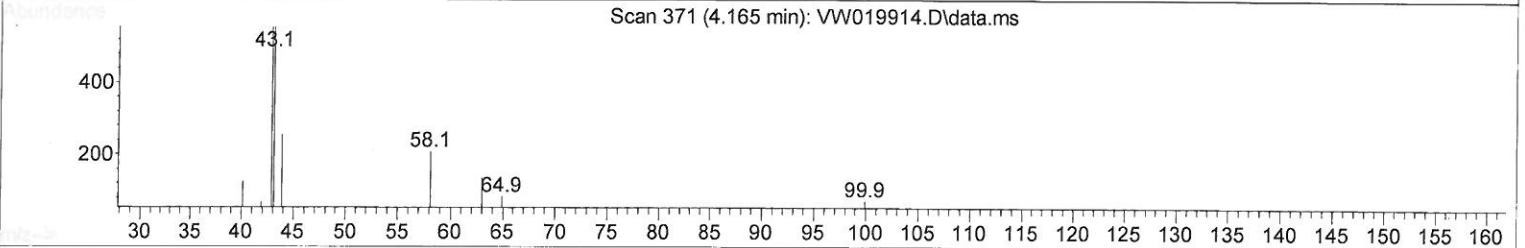

Scan 364 (4.123 min): VW019906.D\data.ms (-356) (-)

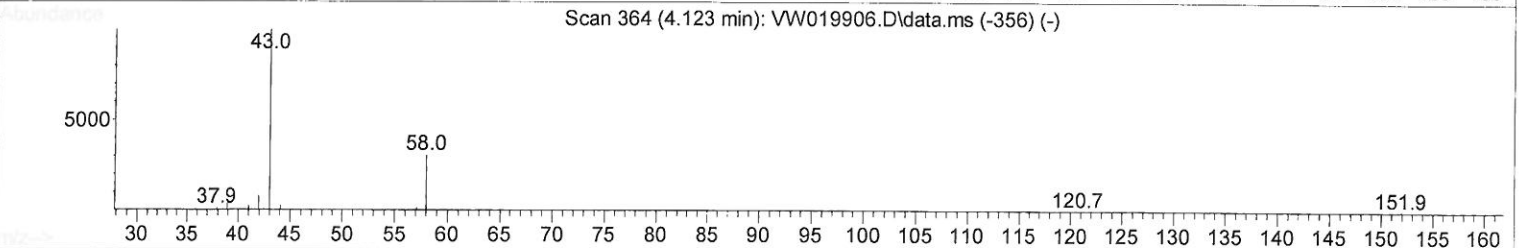

TIC: VW019914.D\data.ms

(13) Acetone (T)

4.165min (+ 0.043) 3.23 ug/L m

response 3203

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	27.82
0.00	0.00	0.00
0.00	0.00	0.00

08/27/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082621\
 Data File : VW019914.D
 Acq On : 26 Aug 2021 13:59
 Operator : SY/VA
 Sample : VIBLK416
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK416

Manual Integrations
 APPROVED

MMDadoda
 8/27/2021 4:44:05 PM

Quant Time: Aug 27 01:03:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 27 00:59:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	368976	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	341682	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	163153	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	105685	18.487	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.960%		
7) Chloroethane-d5	2.897	69	93547	18.643	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.560%		
11) 1,1-Dichloroethene-d2	4.025	63	132455	13.352	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	53.400%		
21) 2-Butanone-d5	7.086	46	47025	40.496	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.000%		
24) Chloroform-d	7.653	84	200252	19.734	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	78.920%		
26) 1,2-Dichloroethane-d4	8.311	65	109010	19.934	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	79.720%		
32) Benzene-d6	8.281	84	391855	20.114	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	80.440%		
36) 1,2-Dichloropropane-d6	9.280	67	119648	20.281	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	81.120%		
41) Toluene-d8	10.329	98	352002	19.716	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.880%		
43) trans-1,3-Dichloroprop...	10.579	79	47264	19.392	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.560%		
47) 2-Hexanone-d5	10.926	63	32718	39.809	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.620%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	98530	20.520	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	82.080%		
66) 1,2-Dichlorobenzene-d4	13.853	152	120137	21.466	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	85.880%		
Target Compounds						
13) Acetone	4.165	43	3203m	3.231	ug/L	Qvalue
16) Methylene chloride	4.921	84	12951	2.045	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082621\
Data File : VW019914.D
Acq On : 26 Aug 2021 13:59
Operator : SY/VA
Sample : VIBLK416
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK416

Manual Integrations
APPROVED

MMDadoda
8/27/2021 4:44:05 PM

Quant Time: Aug 27 01:03:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 27 00:59:57 2021
Response via : Initial Calibration

