

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024354.D
 Acq On : 26 Aug 2022 17:01
 Operator : SY/VA
 Sample : N4319-09
 Misc : 6.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 27 00:41:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	382753	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	397718	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	154244	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.336	65	177425	16.816	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.280%
7) Chloroethane-d5	2.873	69	115948	14.667	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.680%
11) 1,1-Dichloroethene-d2	3.994	63	112325	12.275	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.120%
21) 2-Butanone-d5	7.079	46	50550	26.012	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	52.020%
24) Chloroform-d	7.640	84	212618	17.279	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	69.120%
26) 1,2-Dichloroethane-d4	8.299	65	122198	16.375	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	65.520%#
32) Benzene-d6	8.268	84	425256	18.662	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.640%
36) 1,2-Dichloropropane-d6	9.268	67	124834	17.615	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	70.480%
41) Toluene-d8	10.323	98	364163	16.808	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.240%
43) trans-1,3-Dichloroprop...	10.573	79	47685	14.379	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	57.520%
47) 2-Hexanone-d5	10.926	63	39926	25.176	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	50.360%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	109016	13.587	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	54.360%
66) 1,2-Dichlorobenzene-d4	13.852	152	119900	20.642	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.560%
Target Compounds						
13) Acetone	4.129	43	11159	9.622	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024354.D
Acq On : 26 Aug 2022 17:01
Operator : SY/VA
Sample : N4319-09
Misc : 6.33g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 27 00:41:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 27 00:35:21 2022
Response via : Initial Calibration

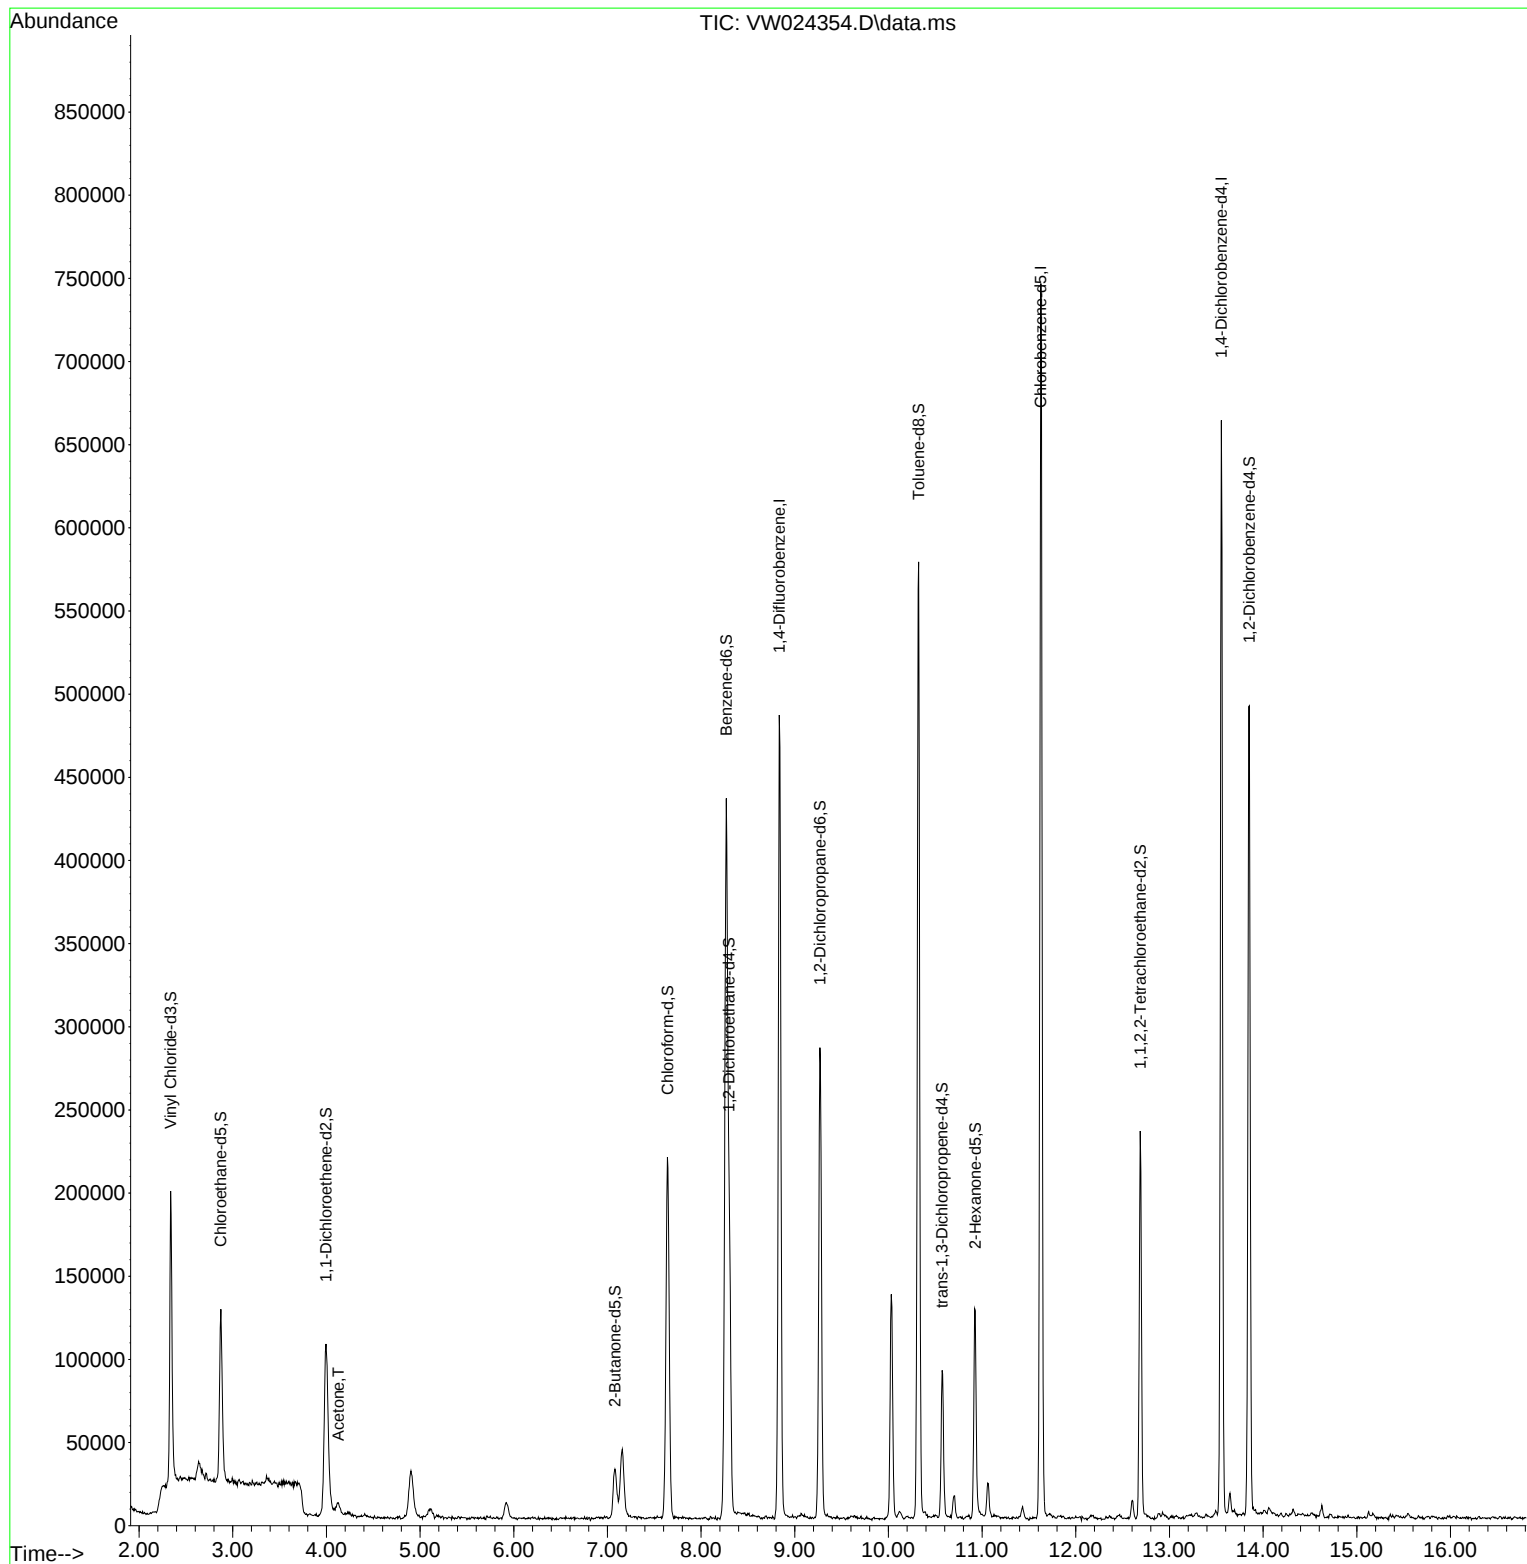

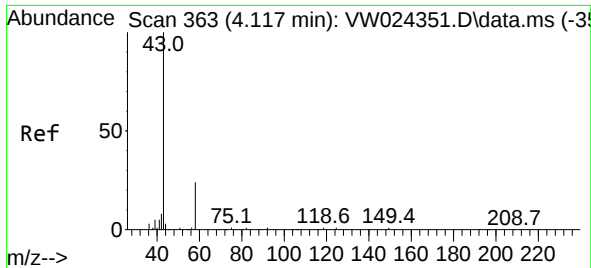

#13
 Acetone
 Concen: 9.622 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW024354.D
 Acq: 26 Aug 2022 17:01

Instrument :
 MSVOA_W
 ClientSampleId :

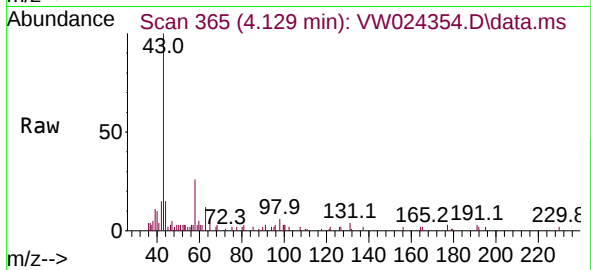

Tgt Ion: 43 Resp: 11159
 Ion Ratio Lower Upper
 43 100
 58 25.3 0.0 58.4

