

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024388.D
 Acq On : 27 Aug 2022 08:36
 Operator : SY/VA
 Sample : N4345-15
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 29 00:58:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 00:57:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	182046	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	174218	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	74495	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	99345	19.797	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.200%
7) Chloroethane-d5	2.873	69	79873	21.243	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.960%
11) 1,1-Dichloroethene-d2	3.909	63	92	0.021	ug/L	-0.10
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.080%#
21) 2-Butanone-d5	7.086	46	27398	29.642	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.280%
24) Chloroform-d	7.647	84	91882	15.699	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	62.800%
26) 1,2-Dichloroethane-d4	8.305	65	56178	15.828	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	63.320%#
32) Benzene-d6	8.275	84	182560	18.289	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.160%
36) 1,2-Dichloropropane-d6	9.268	67	53206	17.139	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	68.560%#
41) Toluene-d8	10.323	98	167042	17.601	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.400%
43) trans-1,3-Dichloroprop...	10.573	79	17285	11.898	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	47.600%
47) 2-Hexanone-d5	10.926	63	20805	29.949	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.900%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	50201	14.283	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	57.120%
66) 1,2-Dichlorobenzene-d4	13.847	152	46500	16.576	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	66.320%#
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	7.159	96	4337	1.532	ug/L	99
34) Trichloroethene	9.091	95	1851	0.647	ug/L #	78
46) Tetrachloroethene	10.866	164	688462	310.079	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024388.D
Acq On : 27 Aug 2022 08:36
Operator : SY/VA
Sample : N4345-15
Misc : 5.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 29 00:58:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 00:57:06 2022
Response via : Initial Calibration

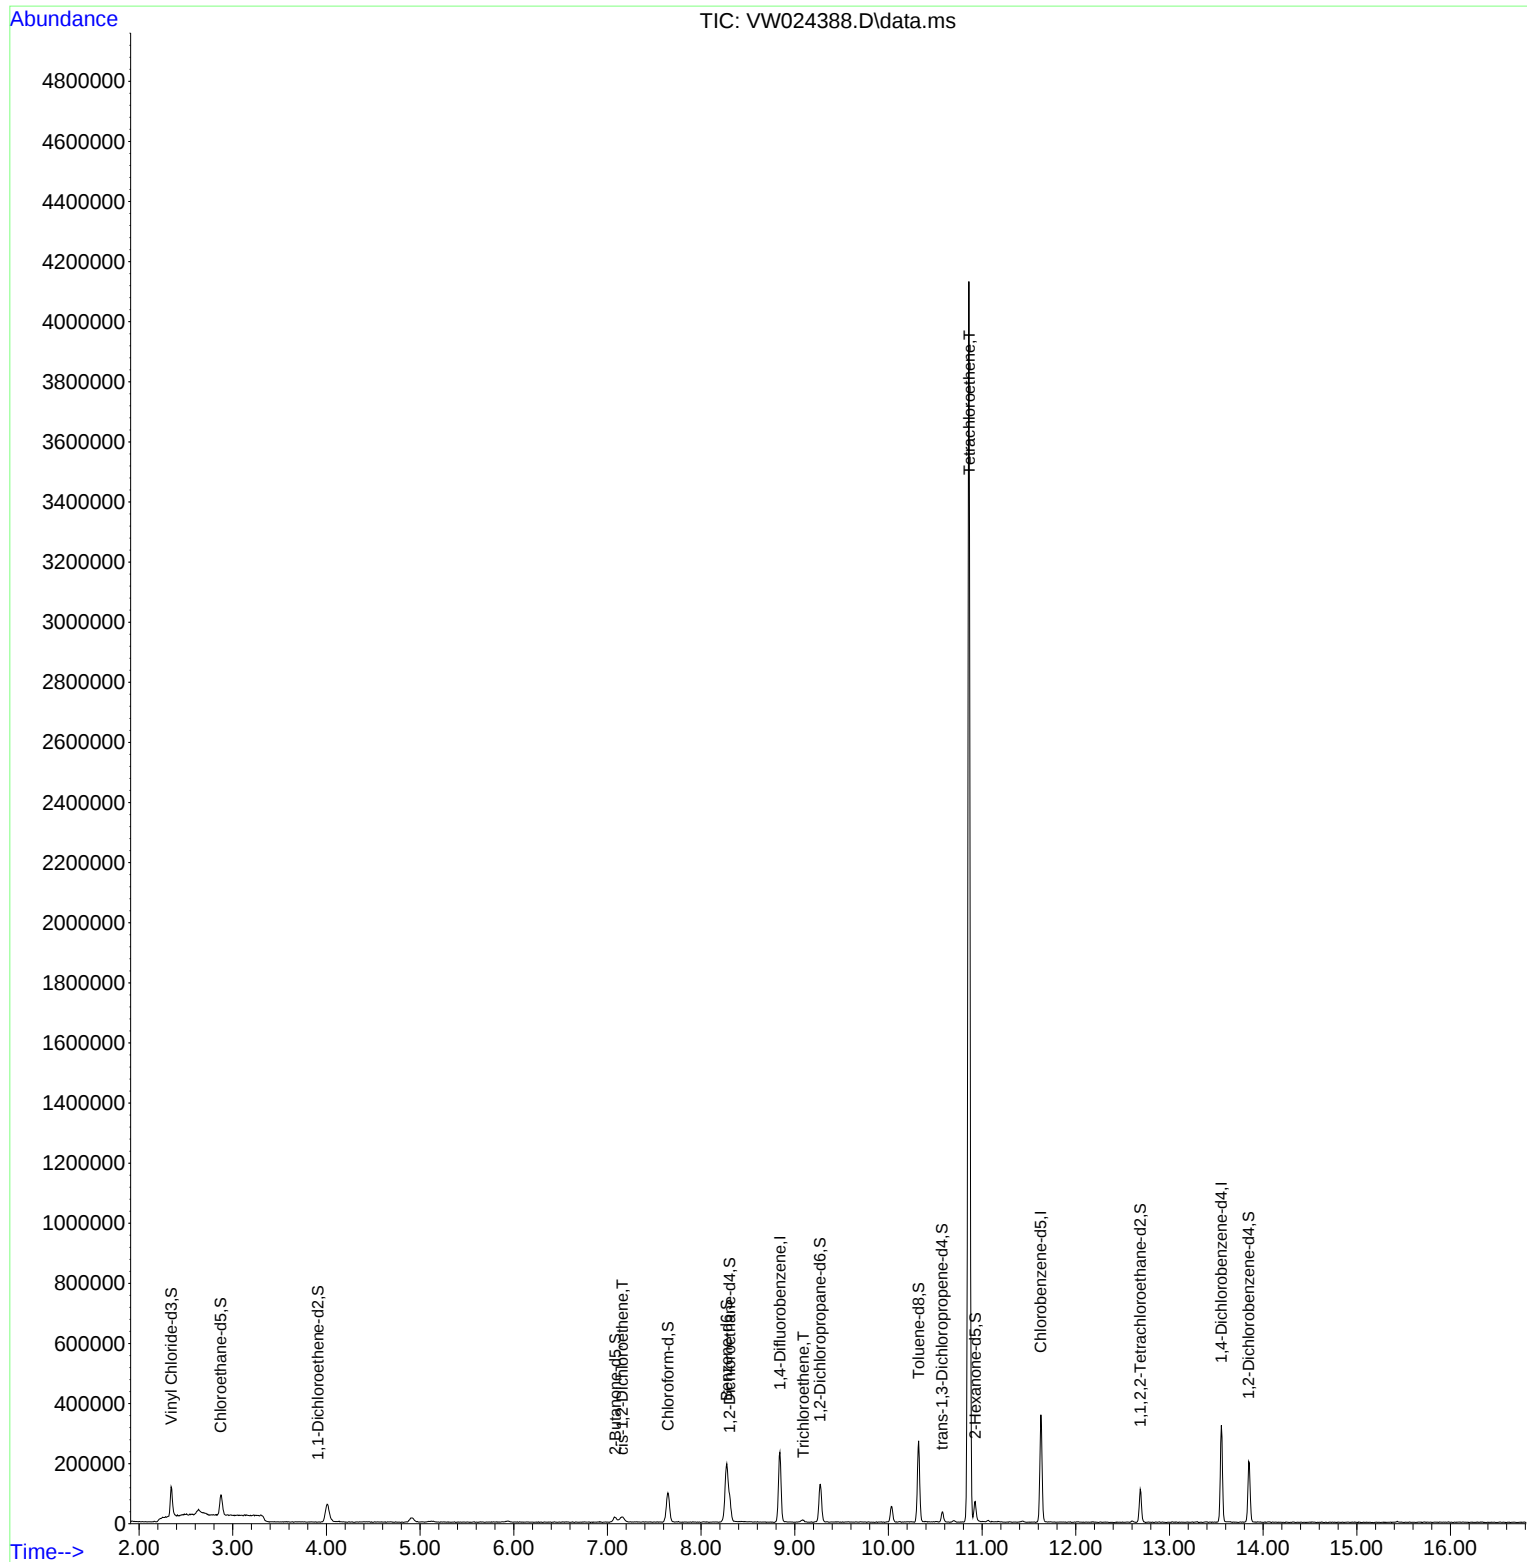

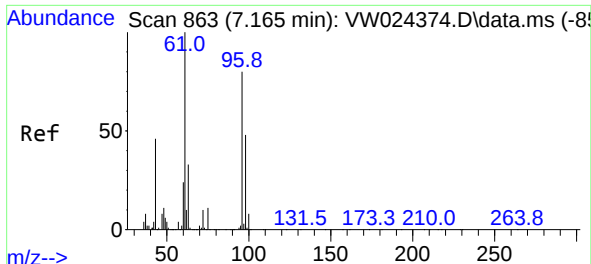




#20
cis-1,2-Dichloroethene
Concen: 1.532 ug/L
RT: 7.159 min Scan# 862
Delta R.T. -0.006 min
Lab File: VW024388.D
Acq: 27 Aug 2022 08:36

Instrument :
MSVOA_W
ClientSampleId :

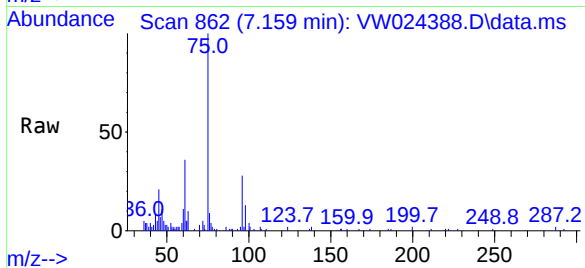

Tgt Ion: 96 Resp: 4337




Ion	Ratio	Lower	Upper
96	100		
61	128.2	90.2	167.6
68	0.0	0.0	0.0

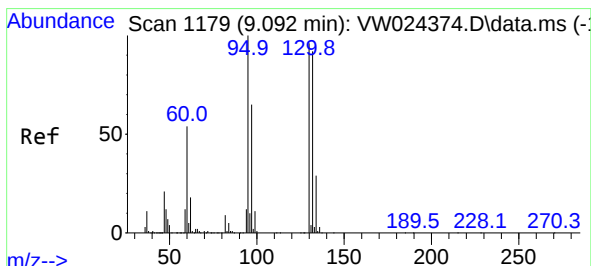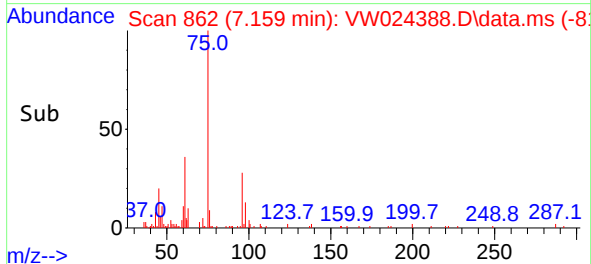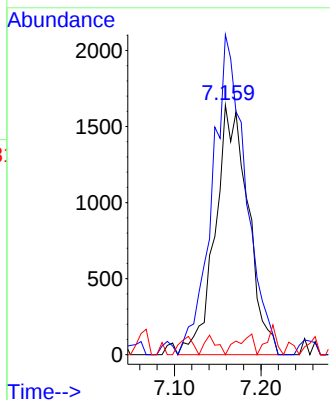


#34
Trichloroethene
Concen: 0.647 ug/L
RT: 9.091 min Scan# 1179
Delta R.T. -0.000 min
Lab File: VW024388.D
Acq: 27 Aug 2022 08:36

Tgt Ion: 95 Resp: 1851


Ion	Ratio	Lower	Upper
95	100		
97	62.8	48.4	89.8
132	62.8	68.6	127.4
130	85.4	72.6	134.8

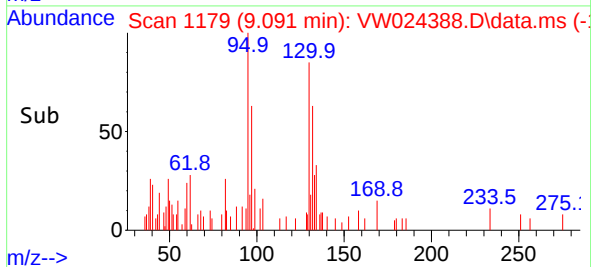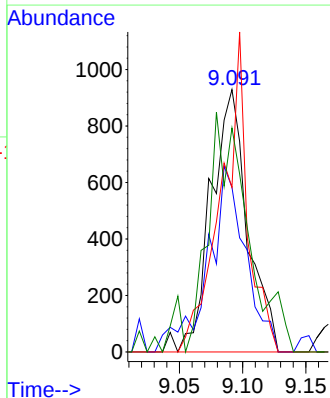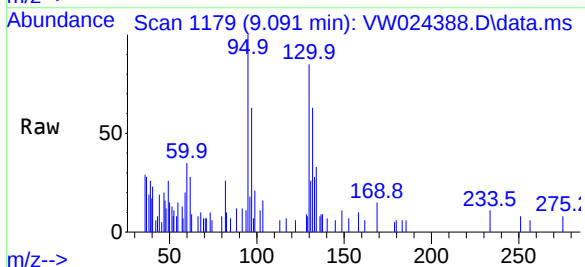

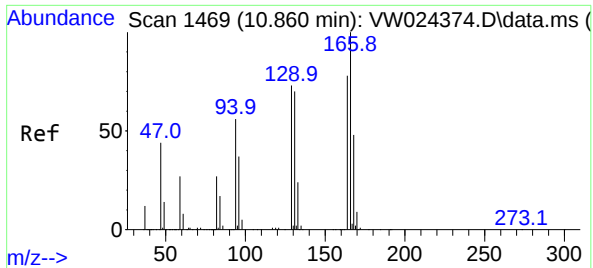

#46
 Tetrachloroethene
 Concen: 310.079 ug/L
 RT: 10.866 min Scan# 14
 Delta R.T. 0.006 min
 Lab File: VW024388.D
 Acq: 27 Aug 2022 08:36

Instrument :
 MSVOA_W
 ClientSampleId :

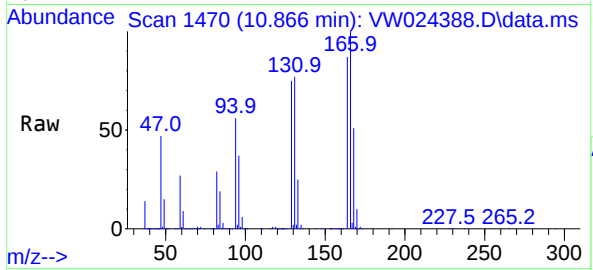

Tgt Ion:164 Resp: 688462

Ion	Ratio	Lower	Upper
164	100		
129	86.7	72.9	135.3
131	88.2	63.7	118.3
166	114.8	86.2	160.0

