

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024360.D
 Acq On : 26 Aug 2022 19:30
 Operator : SY/VA
 Sample : N4345-10
 Misc : 4.90g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

08/30/2022
 Supervised By :Mahesh
 Dadoda
 08/30/2022

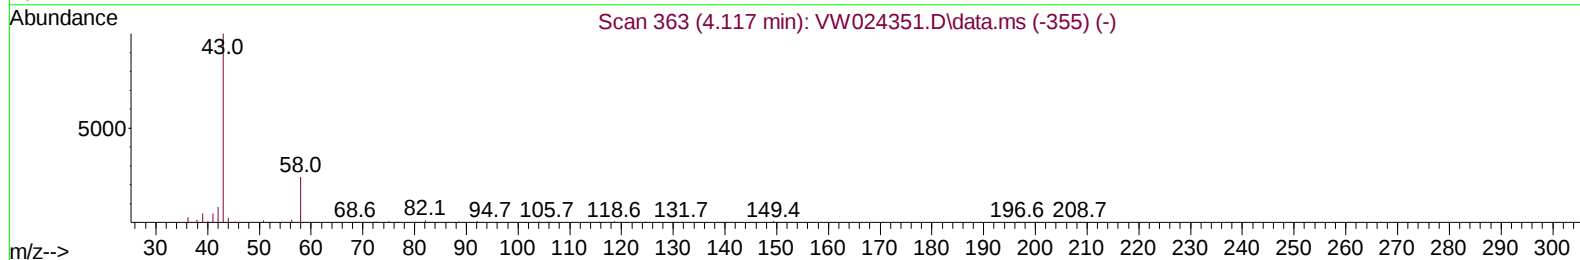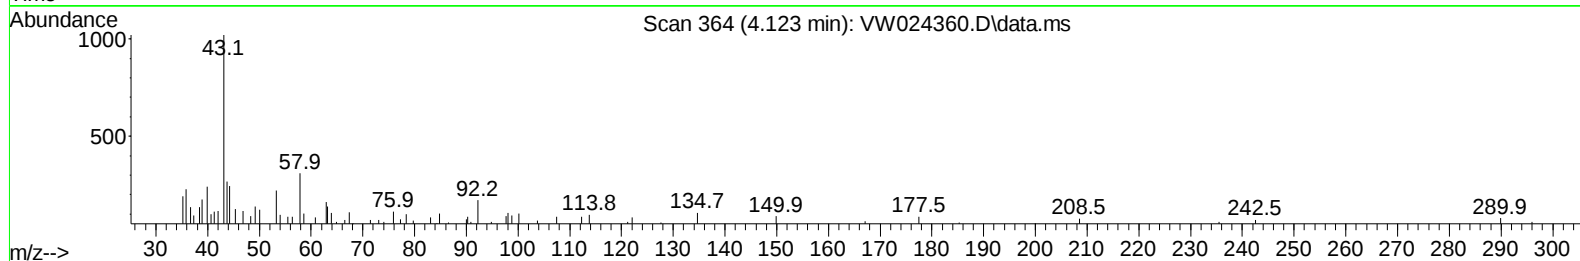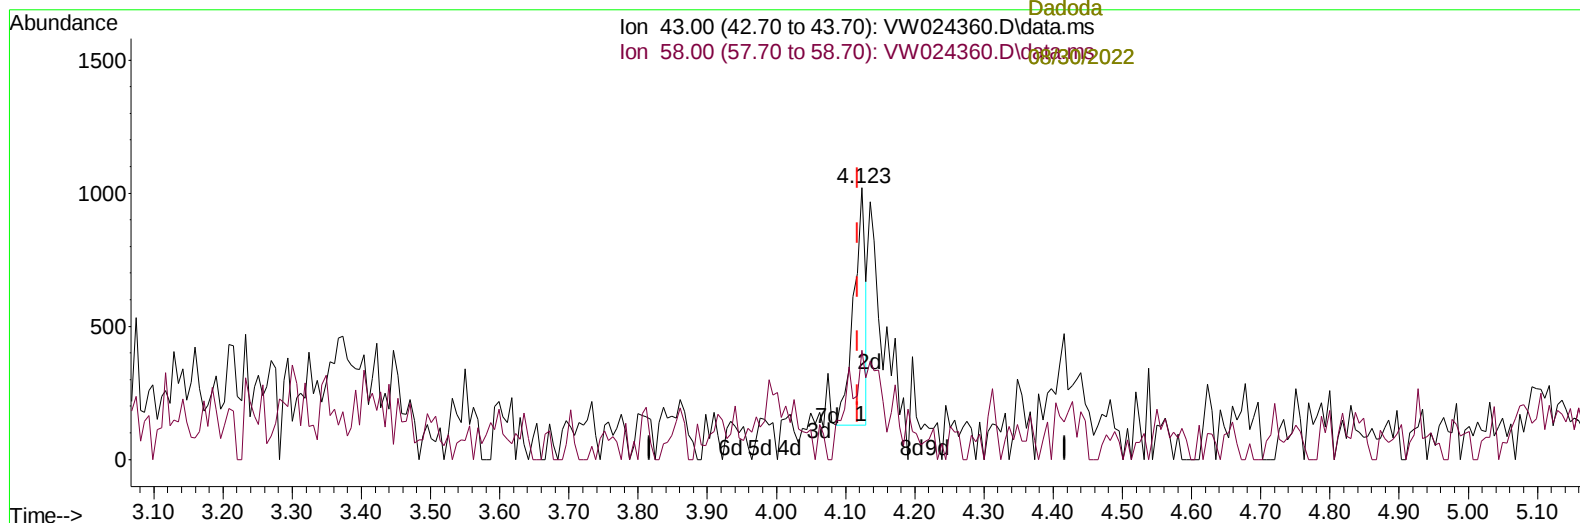

TIC: VW024360.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 3.20 ug/L

response 1062

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	9.42
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024360.D
 Acq On : 26 Aug 2022 19:30
 Operator : SY/VA
 Sample : N4345-10
 Misc : 4.90g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

08/30/2022
 Supervised By :Mahesh
 Dadoda

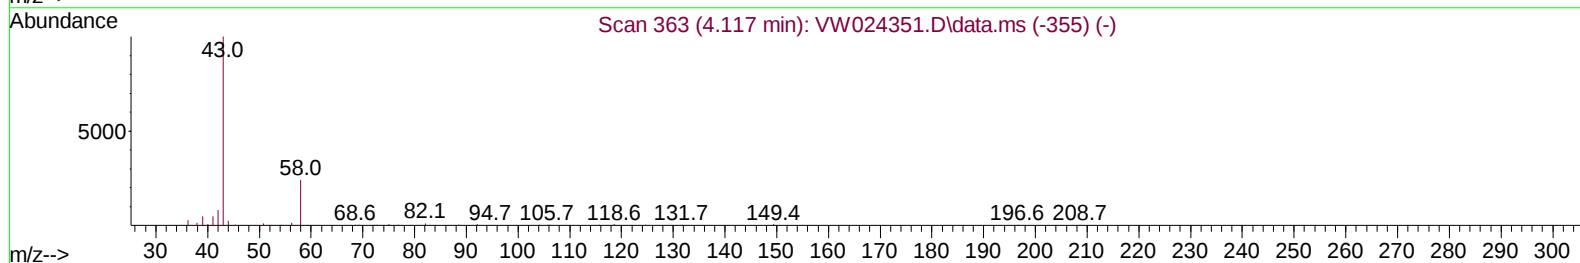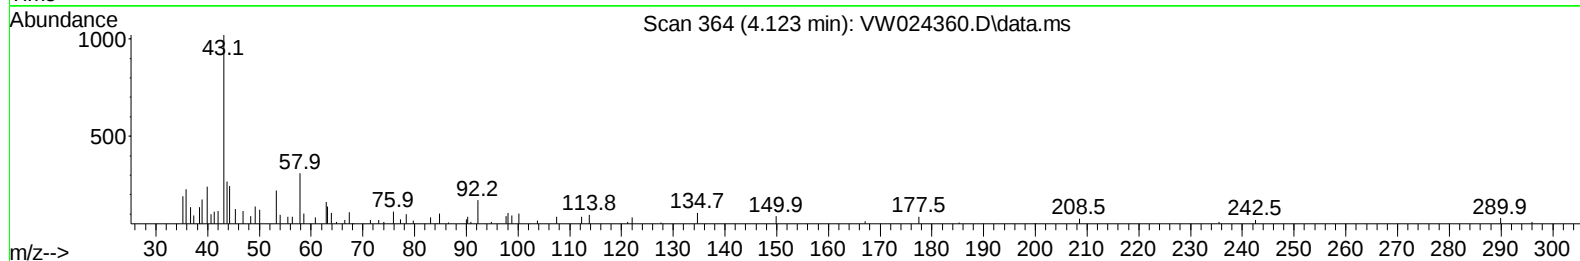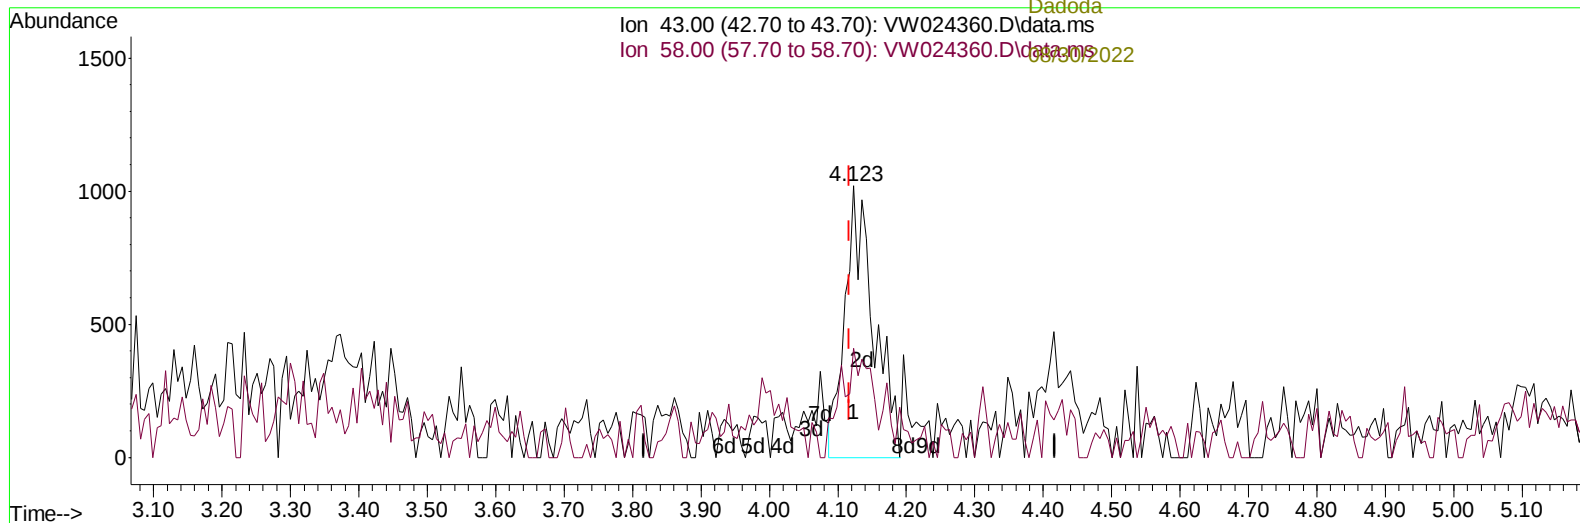

TIC: VW024360.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 8.94 ug/L m

response 2971

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	3.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024360.D
 Acq On : 26 Aug 2022 19:30
 Operator : SY/VA
 Sample : N4345-10
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

08/30/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----08/30/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	109699	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	118544	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	51652	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	91954	30.409	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	121.640%	
7) Chloroethane-d5	2.873	69	50927	22.477	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	89.920%	
11) 1,1-Dichloroethene-d2	4.007	63	46641	17.784	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	71.120%	
21) 2-Butanone-d5	7.086	46	23747	42.635	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	85.280%	
24) Chloroform-d	7.647	84	72971	20.691	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.760%	
26) 1,2-Dichloroethane-d4	8.305	65	46328	21.661	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	86.640%	
32) Benzene-d6	8.269	84	141017	20.762	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.040%	
36) 1,2-Dichloropropane-d6	9.268	67	43933	20.799	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	83.200%	
41) Toluene-d8	10.323	98	126384	19.571	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.280%	
43) trans-1,3-Dichloroprop...	10.579	79	16517	16.709	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	66.840%	
47) 2-Hexanone-d5	10.921	63	15034	31.805	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	63.620%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	42559	17.796	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	71.200%	
66) 1,2-Dichlorobenzene-d4	13.853	152	40416	20.778	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	83.120%	
Target Compounds						
13) Acetone	4.123	43	2971m	8.938	ug/L	
16) Methylene chloride	4.916	84	10765	5.851	ug/L	96
46) Tetrachloroethene	10.860	164	60408	39.985	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024360.D
Acq On : 26 Aug 2022 19:30
Operator : SY/VA
Sample : N4345-10
Misc : 4.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVT0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:43:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 27 00:35:21 2022
Response via : Initial Calibration

08/30/2022
Supervised By :Mahesh
Dadoda

08/30/2022

