




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024401.D
 Acq On : 27 Aug 2022 15:18
 Operator : SY/VA
 Sample : N4346-10MSD
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU8MSD

Manual IntegrationsAPPROVED

Quant Time: Aug 29 01:48:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 01:46:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

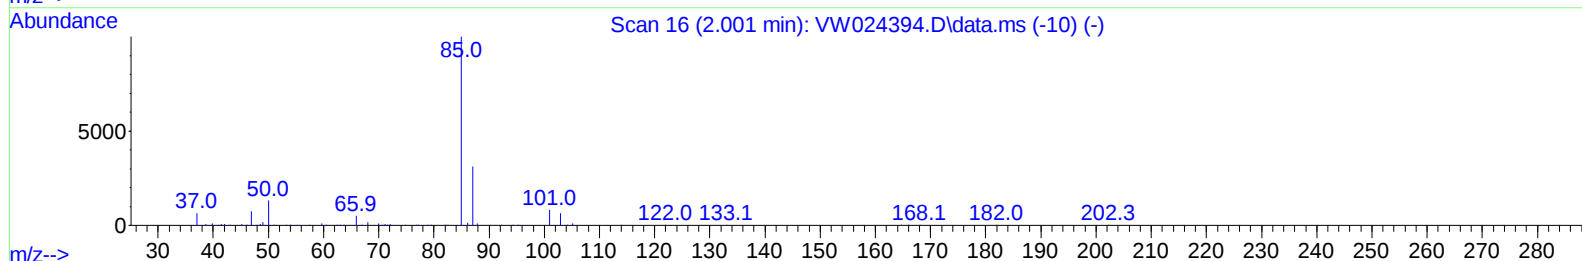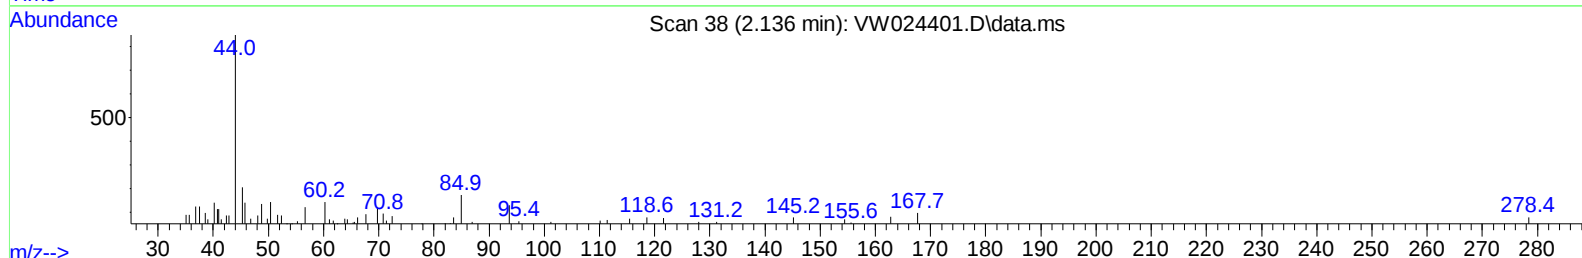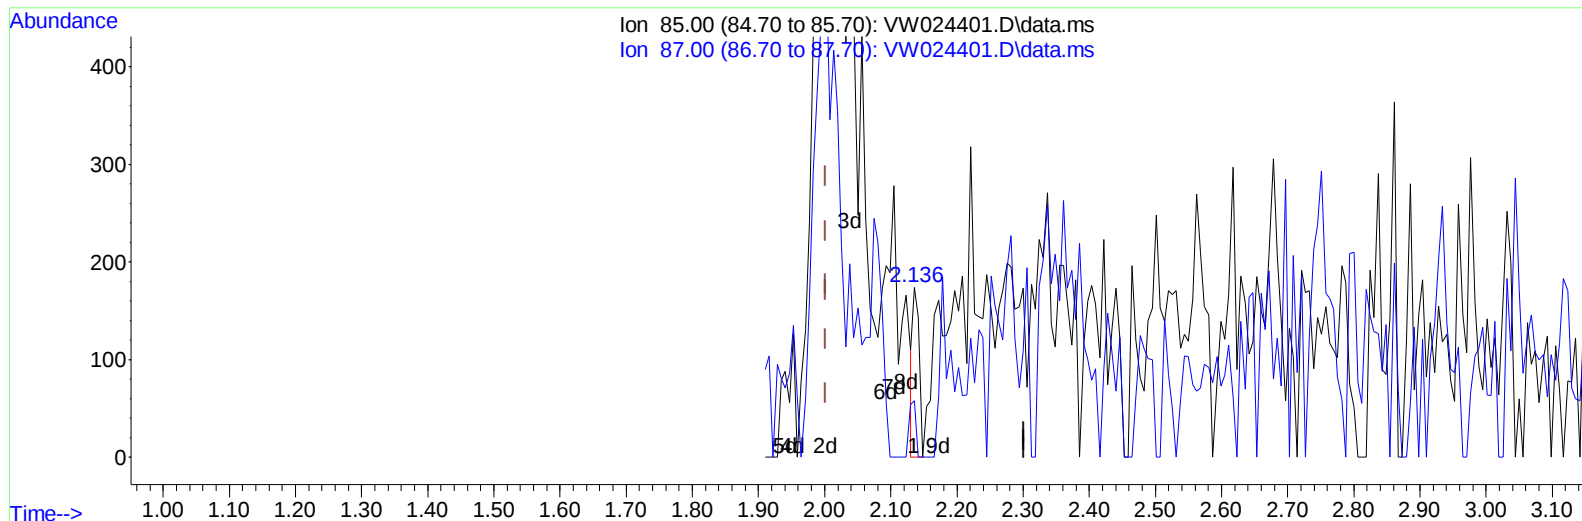

TIC: VW024401.D\data.ms

(2) Dichlorodifluoromethane (T)

2.136min (+ 0.134) 0.07 ug/L

response 116

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	30.90	35.34
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024401.D
 Acq On : 27 Aug 2022 15:18
 Operator : SY/VA
 Sample : N4346-10MSD
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU8MSD

Manual IntegrationsAPPROVED

Quant Time: Aug 29 01:48:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 01:46:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

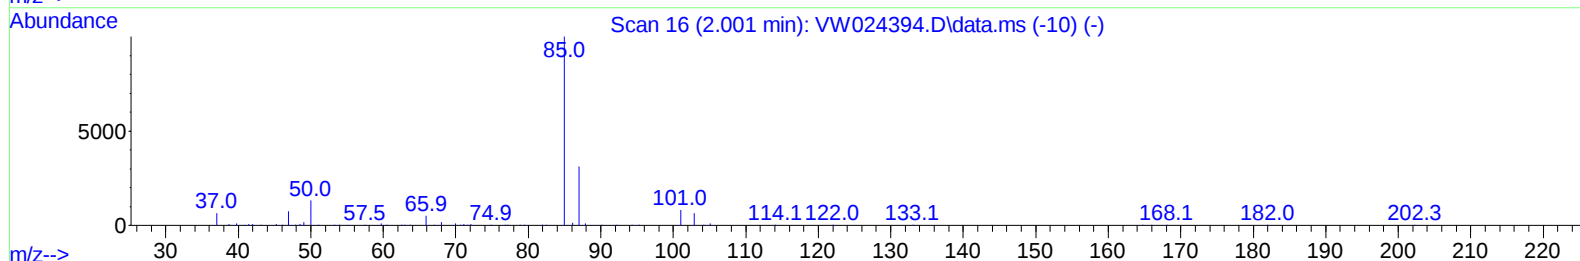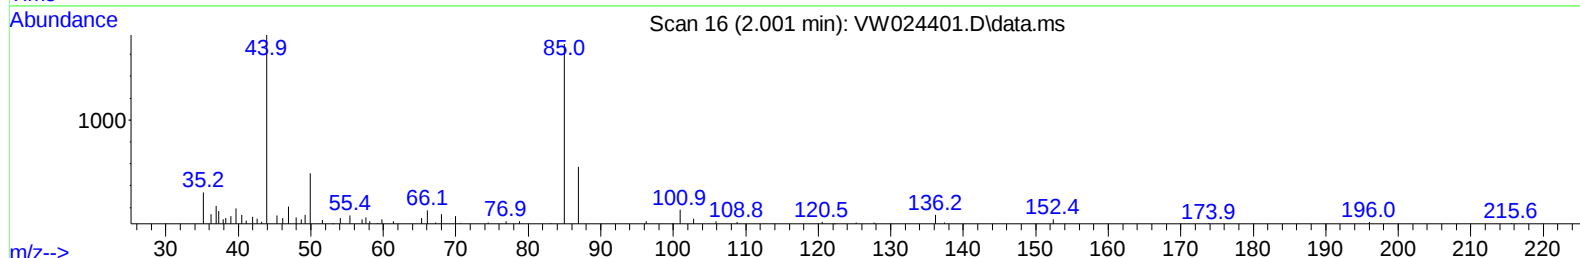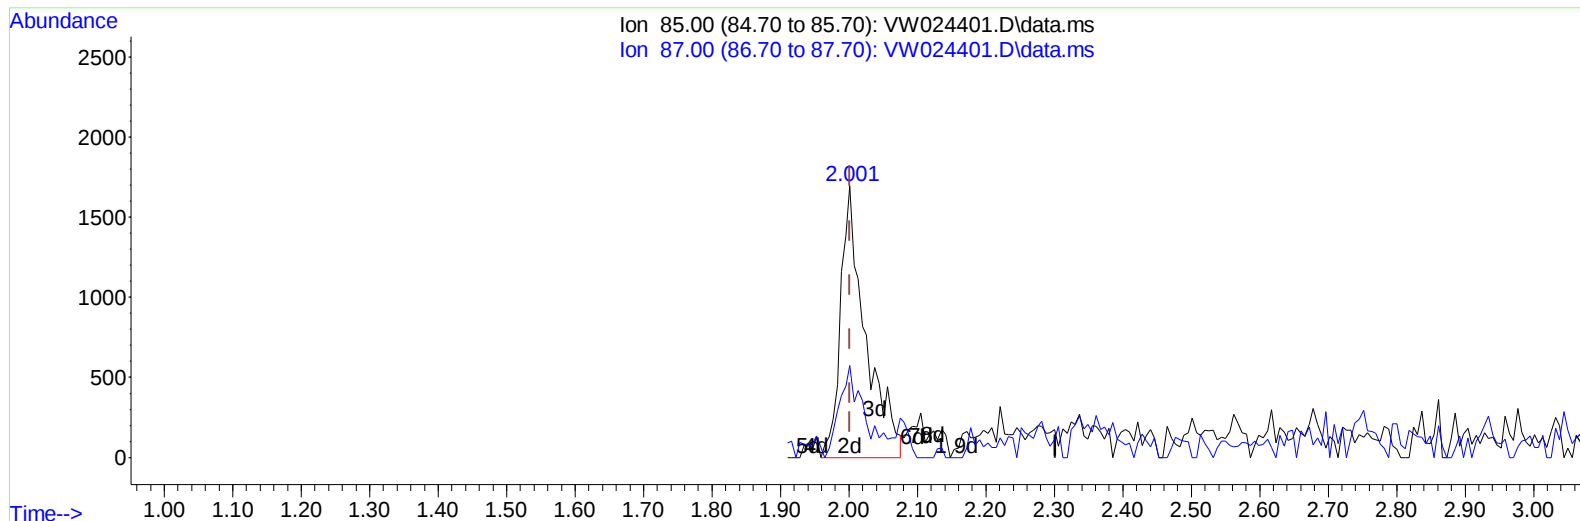

TIC: VW024401.D\data.ms

(2) Dichlorodifluoromethane (T)

2.001min (+ 0.000) 2.42 ug/L m

response 4282

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	30.90	0.96#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024401.D
 Acq On : 27 Aug 2022 15:18
 Operator : SY/VA
 Sample : N4346-10MSD
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU8MSD

Manual IntegrationsAPPROVED

Quant Time: Aug 29 01:48:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 01:46:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

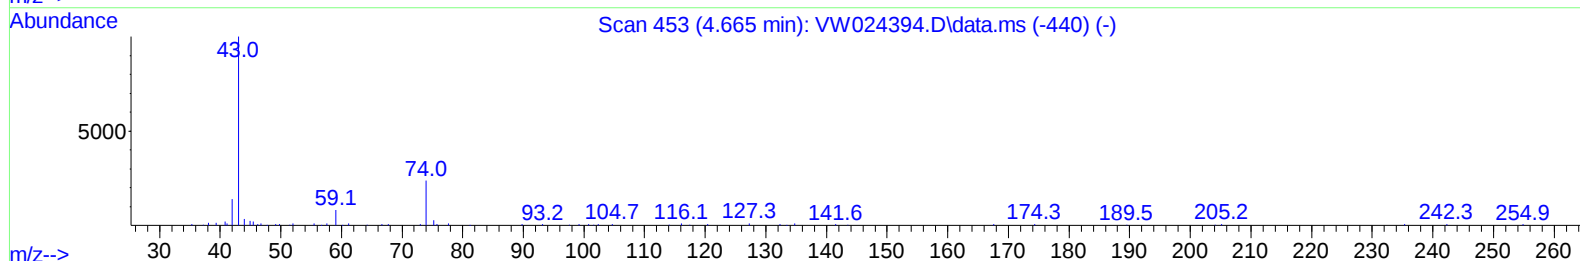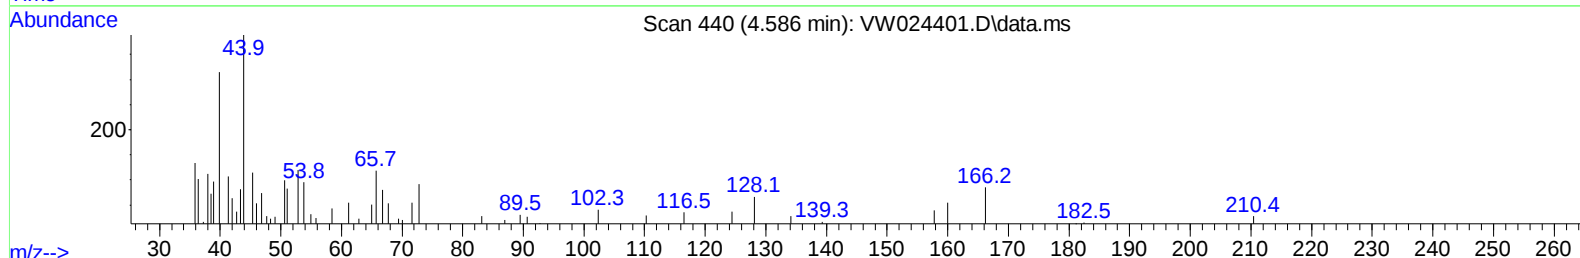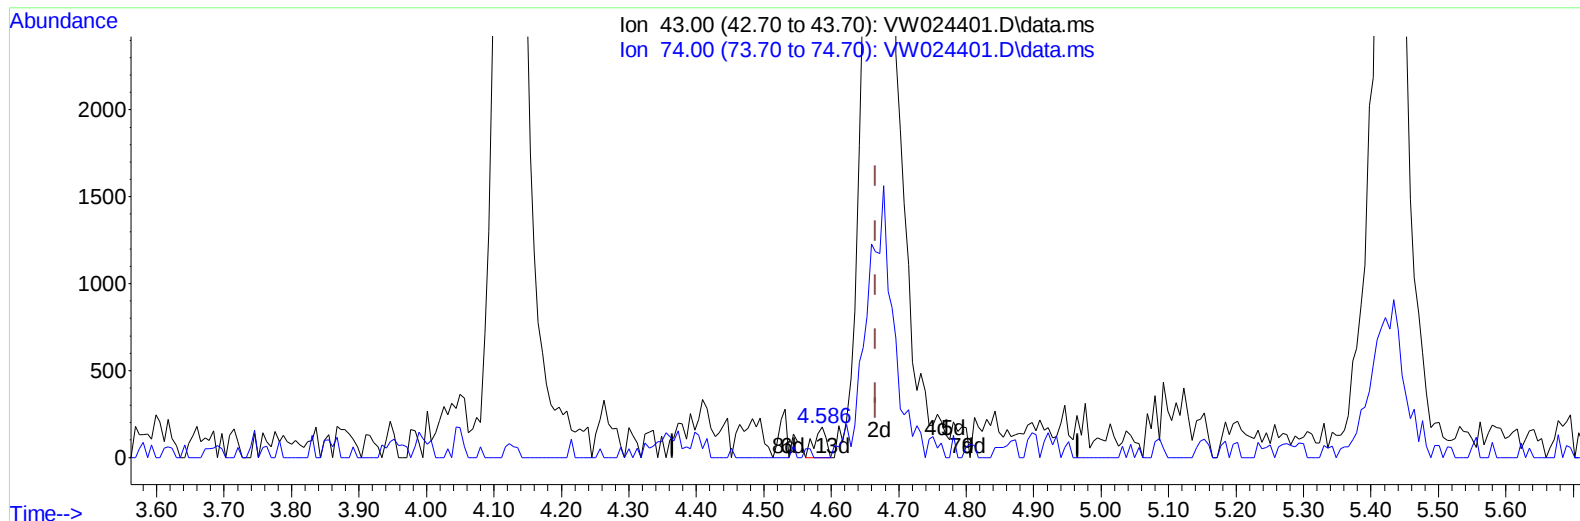

TIC: VW024401.D\data.ms

(15) Methyl Acetate (T)

4.586min (-0.079) 0.16 ug/L

response 212

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	22.40	17.92
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024401.D
Acq On : 27 Aug 2022 15:18
Operator : SY/VA
Sample : N4346-10MSD
Misc : 5.85g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU8MSD

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 01:48:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 01:46:03 2022
Response via : Initial Calibration

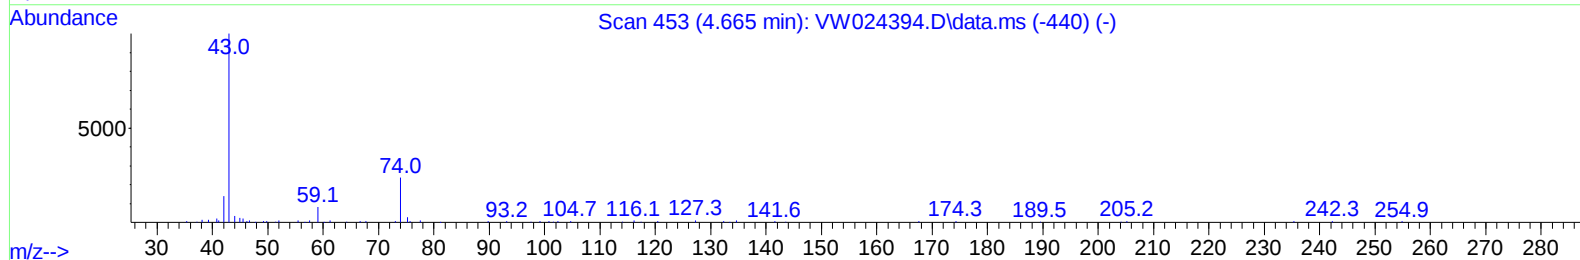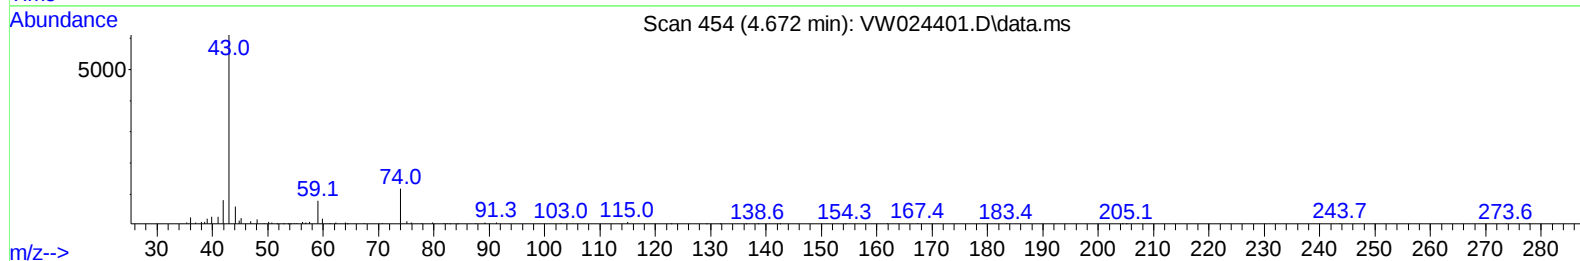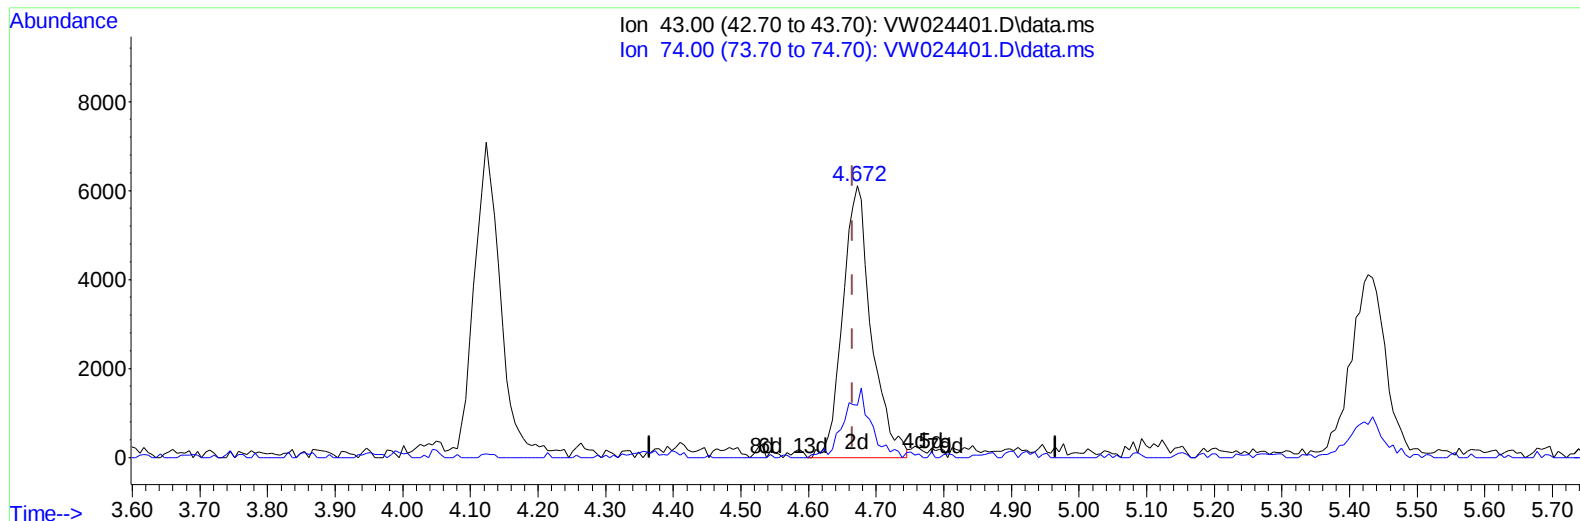

TIC: VW024401.D\data.ms

(15) Methyl Acetate (T)

4.672min (+ 0.006) 13.70 ug/L m

response 17929

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	22.40	0.21#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024401.D
Acq On : 27 Aug 2022 15:18
Operator : SY/VA
Sample : N4346-10MSD
Misc : 5.85g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU8MSD

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 01:48:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 01:46:03 2022
Response via : Initial Calibration

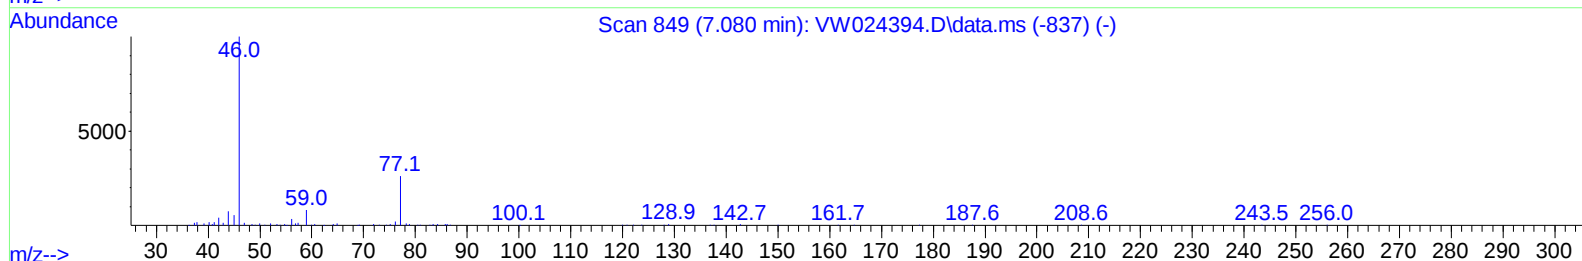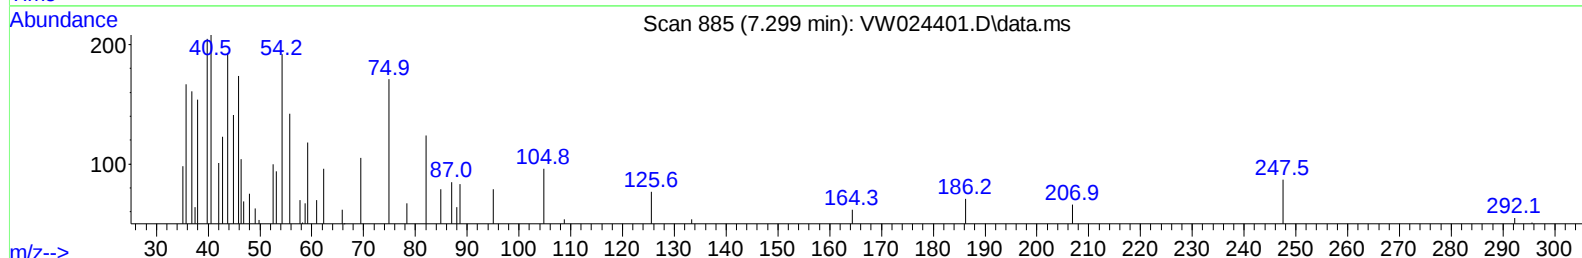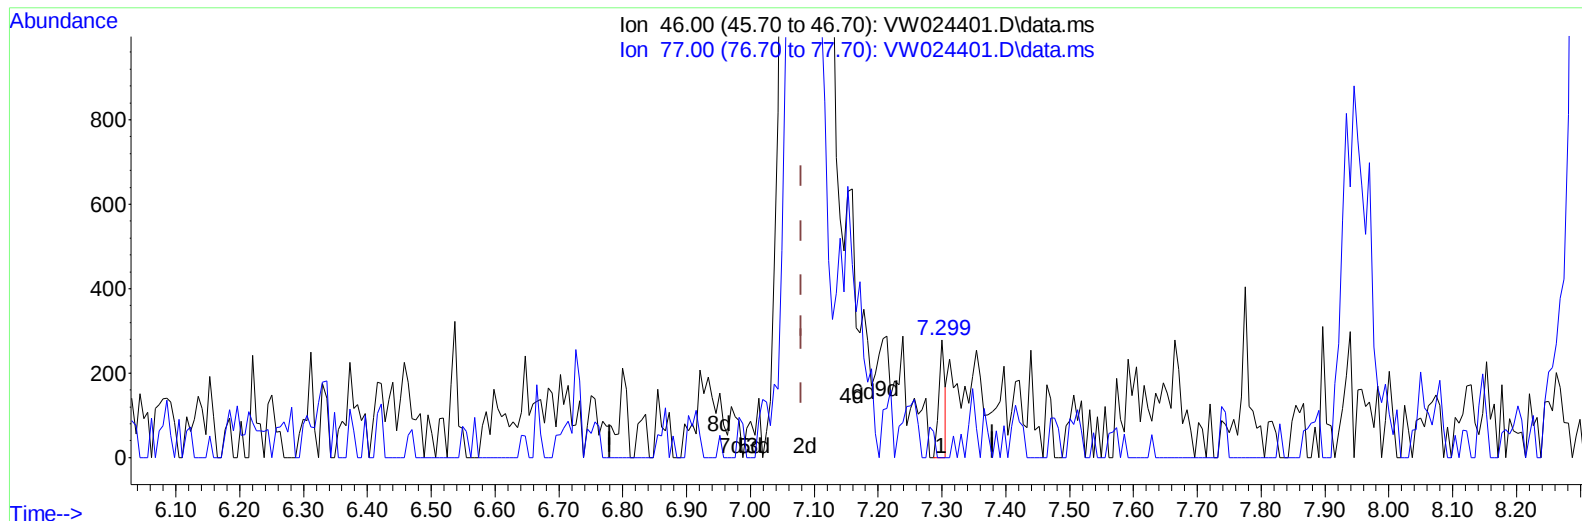

TIC: VW024401.D\data.ms

(21) 2-Butanone-d5 (S)

7.299min (+ 0.220) 0.22 ug/L

response 195

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	9.74
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024401.D
Acq On : 27 Aug 2022 15:18
Operator : SY/VA
Sample : N4346-10MSD
Misc : 5.85g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU8MSD

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 01:48:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 01:46:03 2022
Response via : Initial Calibration

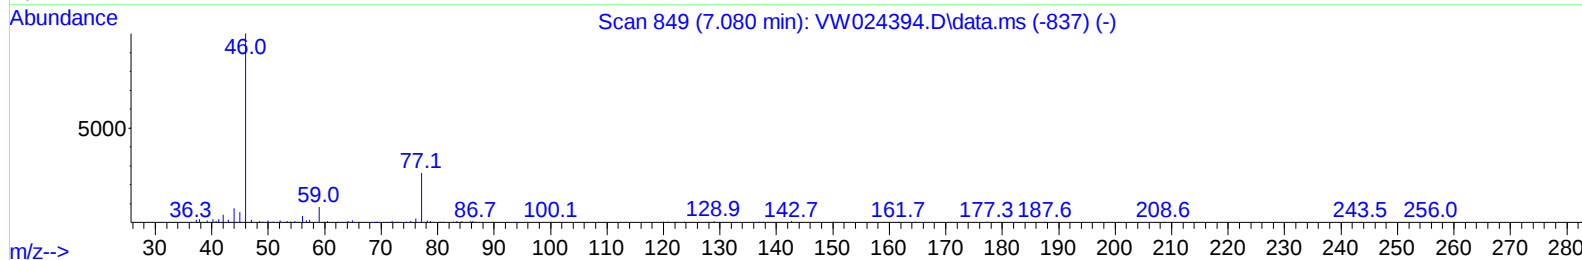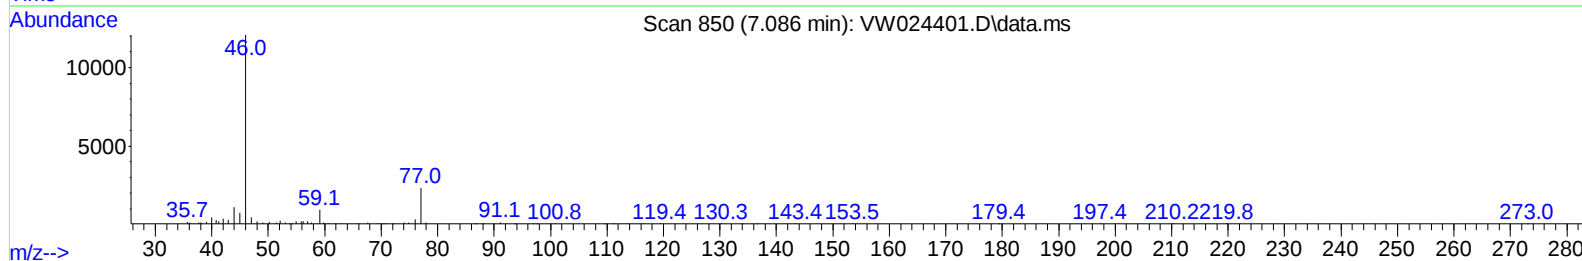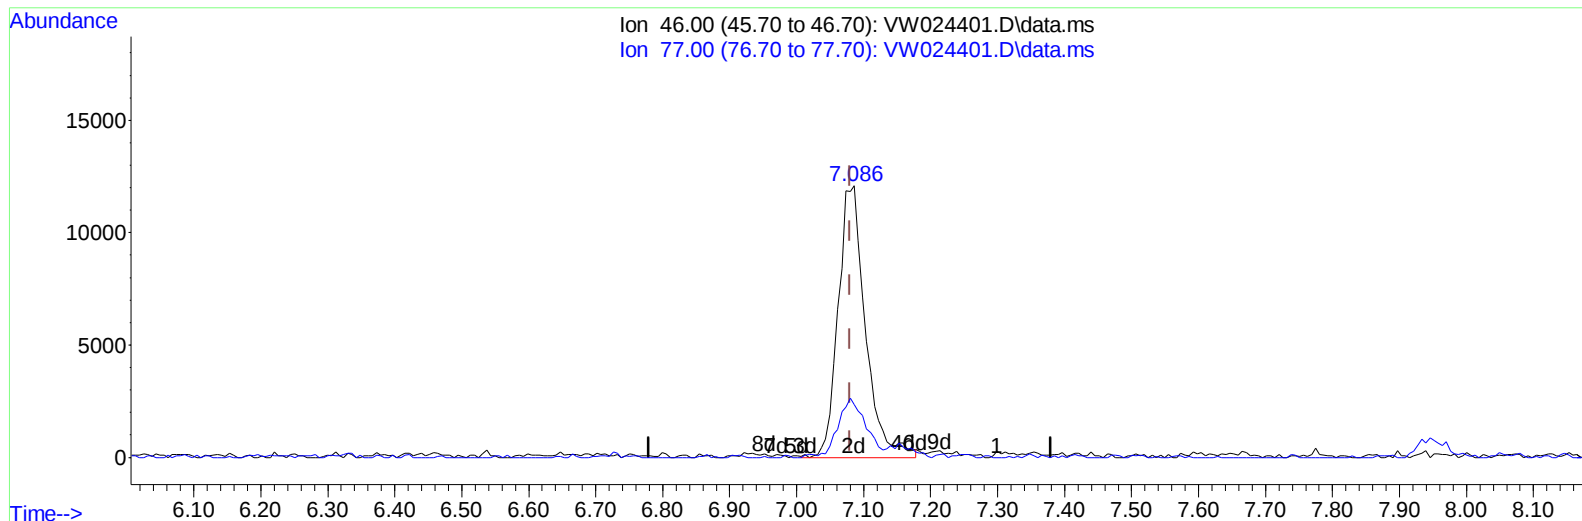

TIC: VW024401.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 38.06 ug/L m

response 34128

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.06#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024401.D
 Acq On : 27 Aug 2022 15:18
 Operator : SY/VA
 Sample : N4346-10MSD
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU8MSD

Manual IntegrationsAPPROVED

Quant Time: Aug 29 01:48:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 01:46:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.836	114	176603	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	167491	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	83397	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	95714	19.661	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.640%	
7) Chloroethane-d5	2.873	69	55279	15.155	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.640%	
11) 1,1-Dichloroethene-d2	4.001	63	63832	15.119	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	60.480%	
21) 2-Butanone-d5	7.086	46	34128m	38.061	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	76.120%	
24) Chloroform-d	7.647	84	108000	19.022	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	76.080%	
26) 1,2-Dichloroethane-d4	8.305	65	78594	22.826	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.320%	
32) Benzene-d6	8.275	84	237970	24.798	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	99.200%	
36) 1,2-Dichloropropane-d6	9.275	67	76952	25.784	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	103.120%	
41) Toluene-d8	10.323	98	222706	24.408	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	97.640%	
43) trans-1,3-Dichloroprop...	10.579	79	32326	23.146	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	92.600%	
47) 2-Hexanone-d5	10.921	63	40568	60.743	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	121.480%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	89365	26.448	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	105.800%	
66) 1,2-Dichlorobenzene-d4	13.847	152	76939	24.499	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	98.000%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.001	85	4282m	2.421	ug/L	
3) Chloromethane	2.209	50	38156	11.546	ug/L	96
5) Vinyl chloride	2.349	62	103328	17.886	ug/L	100
6) Bromomethane	2.763	94	50081	12.350	ug/L	98
8) Chloroethane	2.910	64	38916	12.895	ug/L	99
9) Trichlorofluoromethane	3.245	101	66112	24.336	ug/L	96
10) 1,1,2-Trichloro-1,2,2-...	4.044	101	32573	12.501	ug/L #	70
12) 1,1-Dichloroethene	4.019	96	28318	13.424	ug/L #	73
13) Acetone	4.123	43	17317	32.362	ug/L	92
14) Carbon disulfide	4.367	76	89797	12.809	ug/L	99
15) Methyl Acetate	4.672	43	17929m	13.696	ug/L	
16) Methylene chloride	4.903	84	36803	12.426	ug/L	96
17) trans-1,2-Dichloroethene	5.415	96	31382	12.568	ug/L	98
18) Methyl tert-butyl Ether	5.422	73	58176	14.230	ug/L	99
19) 1,1-Dichloroethane	6.208	63	59063	12.509	ug/L	95
20) cis-1,2-Dichloroethene	7.165	96	37618	13.700	ug/L	98
22) 2-Butanone	7.177	43	30117	31.546	ug/L	76
23) Bromochloromethane	7.513	128	20733	15.464	ug/L	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024401.D
 Acq On : 27 Aug 2022 15:18
 Operator : SY/VA
 Sample : N4346-10MSD
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU8MSD

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 01:48:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 01:46:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
25) Chloroform	7.671	83	86992	16.606	ug/L	95
27) 1,2-Dichloroethane	8.397	62	73871	19.373	ug/L	97
29) Cyclohexane	7.952	56	66912	18.530	ug/L	98
30) 1,1,1-Trichloroethane	7.866	97	78263	19.819	ug/L	99
31) Carbon tetrachloride	8.061	117	68427	18.941	ug/L	100
33) Benzene	8.317	78	229084	21.968	ug/L	100
34) Trichloroethene	9.092	95	61235	22.280	ug/L	97
35) Methylcyclohexane	9.329	83	83095	18.844	ug/L	100
37) 1,2-Dichloropropane	9.366	63	56893	21.141	ug/L #	97
38) Bromodichloromethane	9.640	83	78277	21.359	ug/L	98
39) cis-1,3-Dichloropropene	10.073	75	78541	20.878	ug/L	98
40) 4-Methyl-2-pentanone	10.207	43	88204	46.092	ug/L	99
42) Toluene	10.384	91	247135	21.474	ug/L	91
44) trans-1,3-Dichloropropene	10.604	75	71087	19.447	ug/L	97
45) 1,1,2-Trichloroethane	10.786	97	48295	22.007	ug/L	92
46) Tetrachloroethene	10.860	164	411005	192.549	ug/L	92
48) 2-Hexanone	10.969	43	64591	45.760	ug/L	97
49) Dibromochloromethane	11.128	129	53434	20.586	ug/L	98
50) 1,2-Dibromoethane	11.231	107	47953	22.728	ug/L #	94
51) Chlorobenzene	11.652	112	160605	20.792	ug/L	97
52) Ethylbenzene	11.725	91	266753	20.966	ug/L	98
53) m,p-Xylene	11.835	106	103478	20.709	ug/L	100
54) o-Xylene	12.164	106	96787	20.720	ug/L	93
55) Styrene	12.176	104	176321	21.354	ug/L	98
57) 1,1,2,2-Tetrachloroethane	12.713	83	65038	21.232	ug/L	98
59) Bromoform	12.347	173	30106	22.495	ug/L	96
60) Isopropylbenzene	12.463	105	258696	23.355	ug/L	99
61) 1,2,3-Trichloropropane	12.768	75	46483	24.647	ug/L	98
62) 1,3,5-Trimethylbenzene	12.938	105	196399	21.990	ug/L	97
63) 1,2,4-Trimethylbenzene	13.249	105	194282	22.395	ug/L	99
64) 1,3-Dichlorobenzene	13.499	146	108412	20.471	ug/L	96
65) 1,4-Dichlorobenzene	13.573	146	113462	20.293	ug/L	94
67) 1,2-Dichlorobenzene	13.865	146	104323	21.015	ug/L	98
68) 1,2-Dibromo-3-chloropr...	14.481	75	9681	20.432	ug/L	92
69) 1,3,5-Trichlorobenzene	14.627	180	52774	15.439	ug/L	98
70) 1,2,4-trichlorobenzene	15.127	180	42233	15.894	ug/L	96
71) Naphthalene	15.359	128	107960	18.500	ug/L	98
72) 1,2,3-Trichlorobenzene	15.548	180	38738	15.425	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024401.D
 Acq On : 27 Aug 2022 15:18
 Operator : SY/VA
 Sample : N4346-10MSD
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

Client SampleId :

DBVU8MSD

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 01:48:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 01:46:03 2022
 Response via : Initial Calibration

