

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024366.D
 Acq On : 26 Aug 2022 21:58
 Operator : SY/VA
 Sample : N4344-05
 Misc : 5.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVQ4

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 08/30/2022
 Supervised By : Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:45:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	181066	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	180993	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	75483	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	140938	28.237	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.960%
7) Chloroethane-d5	2.873	69	86844	23.222	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.880%
11) 1,1-Dichloroethene-d2	4.007	63	68266m	15.770	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.080%
21) 2-Butanone-d5	7.086	46	30733m	33.430	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.860%
24) Chloroform-d	7.647	84	107175	18.411	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.640%
26) 1,2-Dichloroethane-d4	8.305	65	64166	18.177	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	72.720%
32) Benzene-d6	8.275	84	208304	20.087	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.360%
36) 1,2-Dichloropropane-d6	9.275	67	61588	19.097	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.400%
41) Toluene-d8	10.323	98	187315	18.998	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.000%
43) trans-1,3-Dichloroprop...	10.573	79	24624	16.316	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.280%
47) 2-Hexanone-d5	10.921	63	25711	35.626	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.260%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	57835	15.839	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	63.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	58290	20.507	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.040%
Target Compounds						Qvalue
16) Methylene chloride	4.922	84	11631	3.830	ug/L	89
34) Trichloroethene	9.092	95	2996	1.009	ug/L #	78
46) Tetrachloroethene	10.860	164	1692491	733.754	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024366.D
Acq On : 26 Aug 2022 21:58
Operator : SY/VA
Sample : N4344-05
Misc : 5.47g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBVQ4

Quant Time: Aug 27 00:45:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 27 00:35:21 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

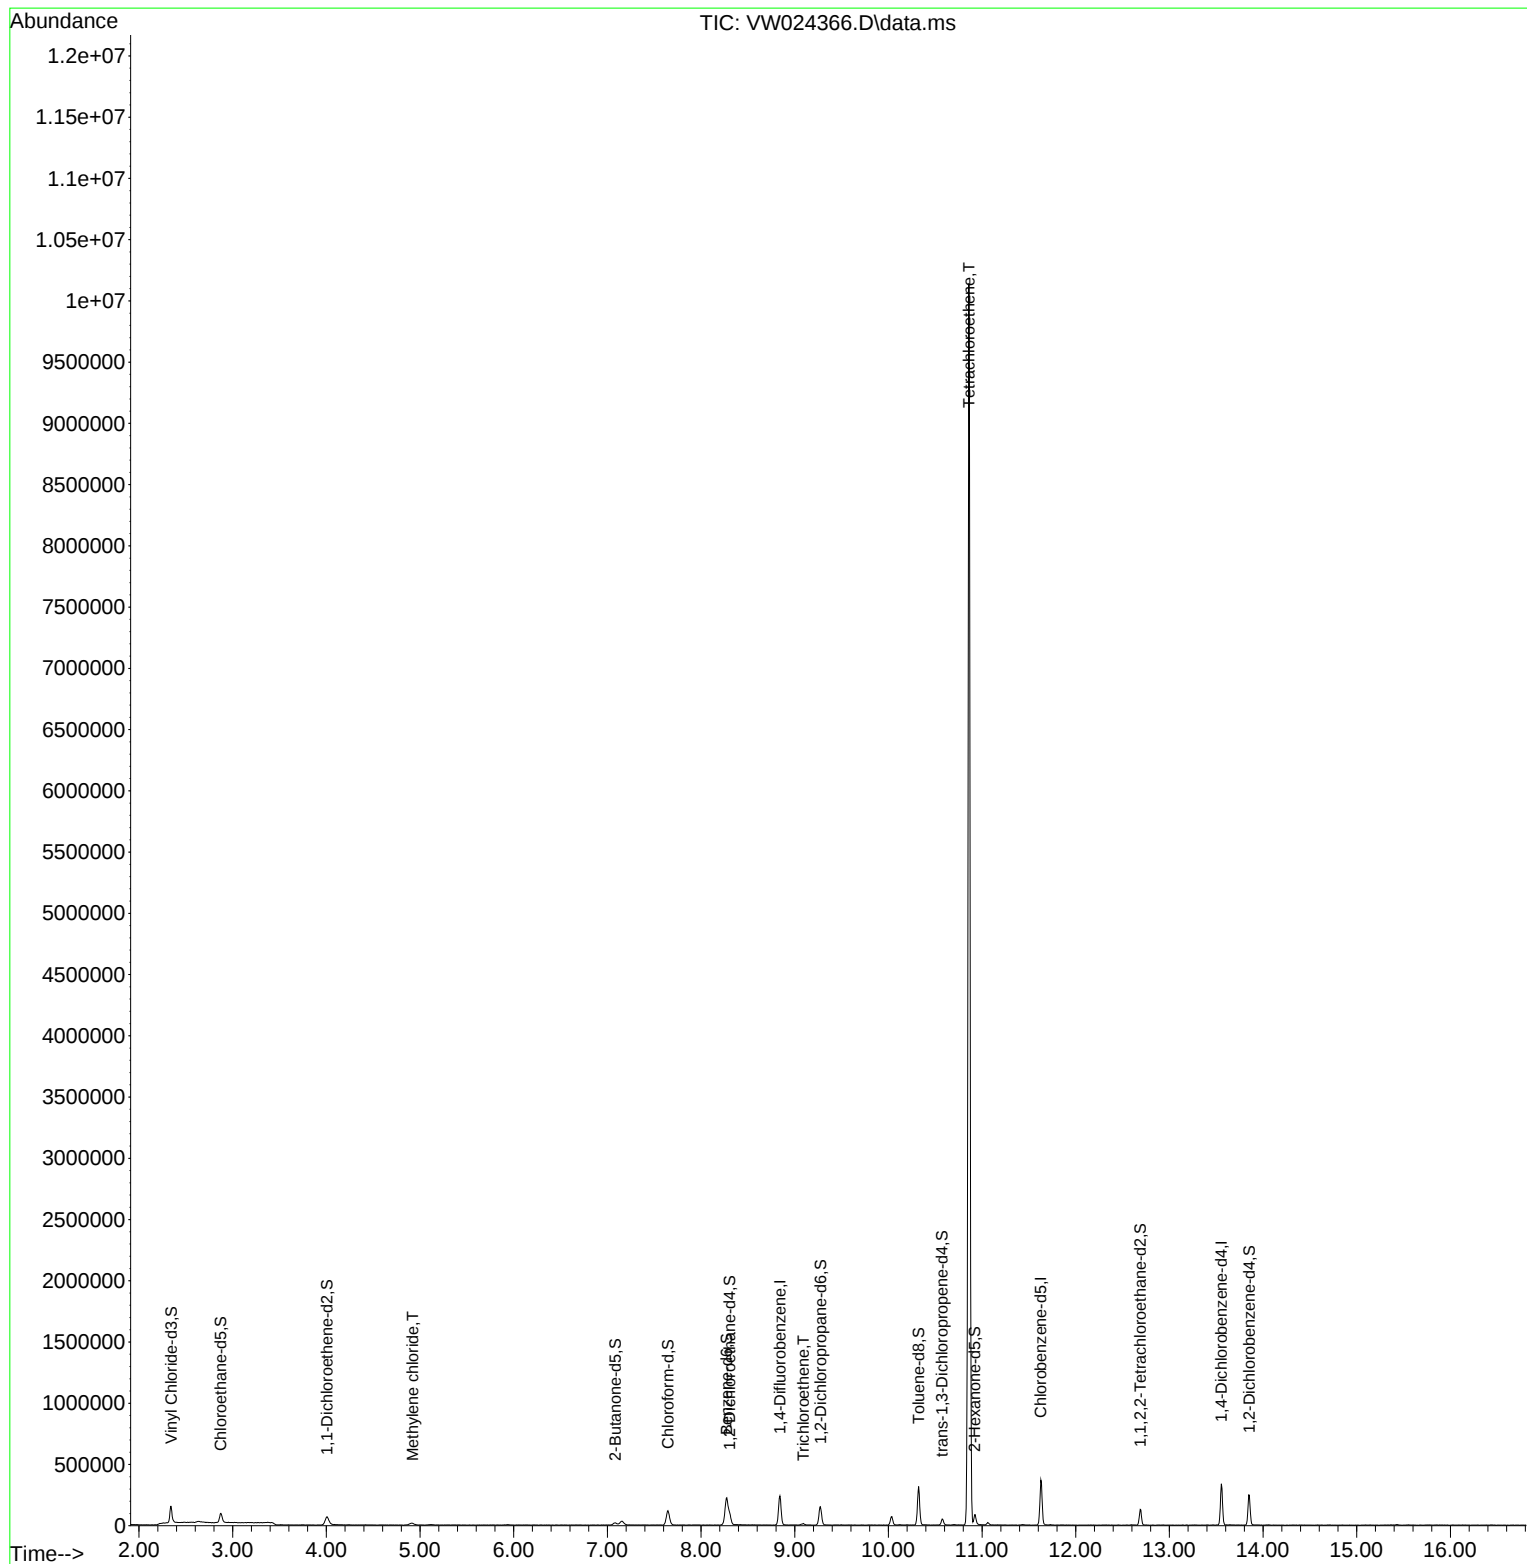

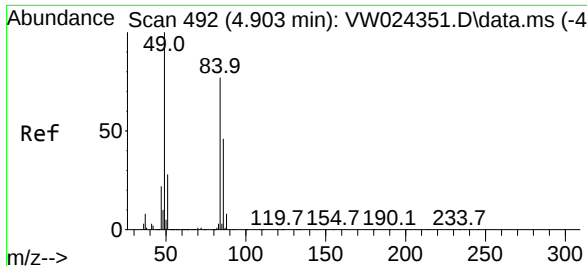

#16
Methylene chloride
Concen: 3.830 ug/L
RT: 4.922 min Scan# 492
Delta R.T. 0.019 min
Lab File: VW024366.D
Acq: 26 Aug 2022 21:58




Instrument :
MSVOA_W
ClientSampleId :
DBVQ4

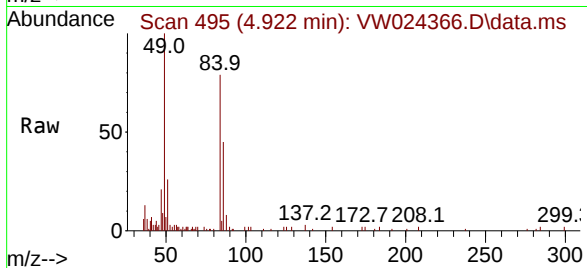

Tgt Ion: 84 Resp: 1163
Ion Ratio Lower Upper
84 100
86 56.3 47.7 88.7
49 126.3 96.6 179.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

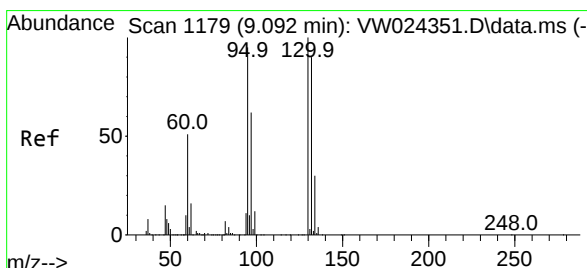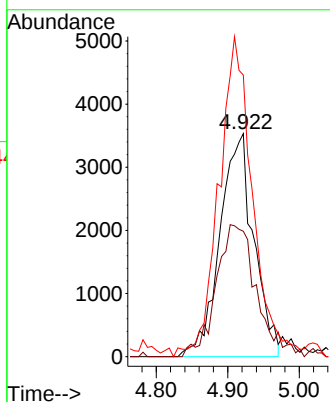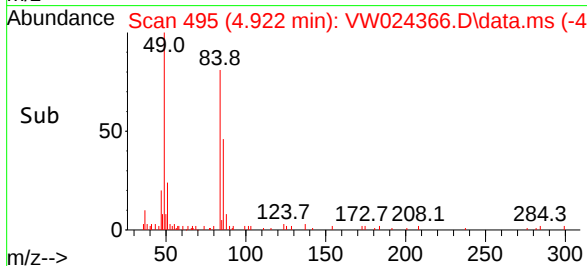

#34
Trichloroethene
Concen: 1.009 ug/L
RT: 9.092 min Scan# 1179
Delta R.T. 0.000 min
Lab File: VW024366.D
Acq: 26 Aug 2022 21:58


Tgt Ion: 95 Resp: 2996
Ion Ratio Lower Upper
95 100
97 44.8 48.4 89.8#
132 75.6 68.6 127.4
130 88.2 72.6 134.8

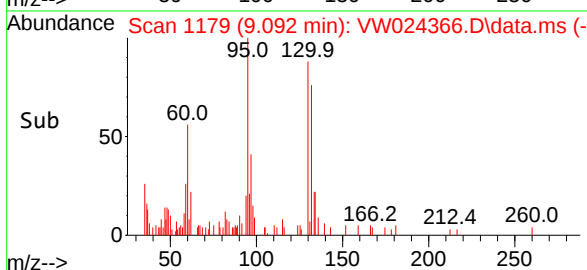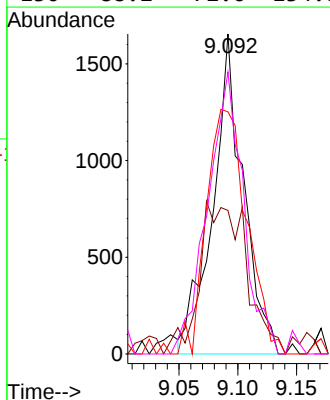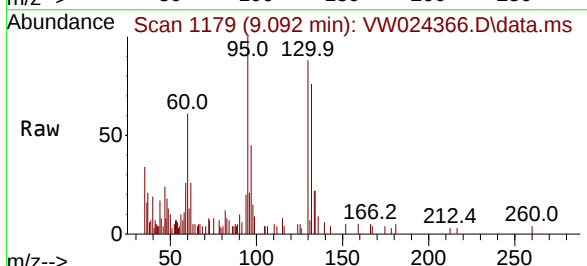

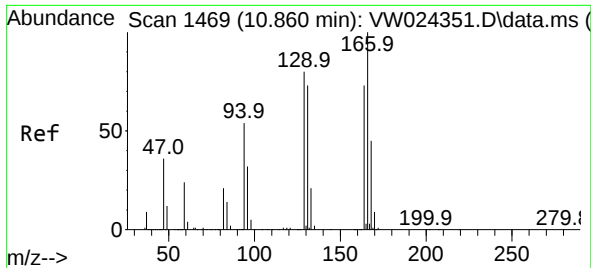

#46
Tetrachloroethene
Concen: 733.754 ug/L
RT: 10.860 min Scan# 1469
Delta R.T. 0.000 min
Lab File: VW024366.D
Acq: 26 Aug 2022 21:58

Instrument :
MSVOA_W
ClientSampleId :
DBVQ4

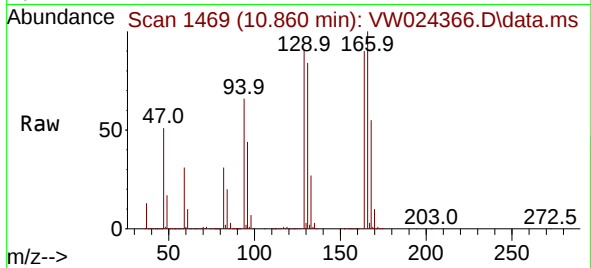

Tgt Ion:164 Resp: 169249
Ion Ratio Lower Upper
164 100
129 101.2 72.9 135.3
131 93.5 63.7 118.3
166 111.0 86.2 160.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

