

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024369.D
 Acq On : 26 Aug 2022 23:12
 Operator : SY/VA
 Sample : N4344-09
 Misc : 5.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVQ8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:46:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	204171	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	212497	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	92347	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	142672	25.350	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	101.400%	
7) Chloroethane-d5	2.873	69	87454	20.739	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	82.960%	
11) 1,1-Dichloroethene-d2	4.013	63	70189	14.380	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	57.520%	
21) 2-Butanone-d5	7.080	46	29131	28.101	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	56.200%	
24) Chloroform-d	7.647	84	116557	17.757	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	71.040%	
26) 1,2-Dichloroethane-d4	8.305	65	67956m	17.072	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	68.280%#	
32) Benzene-d6	8.275	84	223822	18.384	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	73.520%	
36) 1,2-Dichloropropane-d6	9.274	67	67705	17.881	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	71.520%	
41) Toluene-d8	10.323	98	205672	17.767	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	71.080%	
43) trans-1,3-Dichloroprop...	10.573	79	26032	14.691	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	58.760%	
47) 2-Hexanone-d5	10.920	63	24593	29.024	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	58.040%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	58107	13.555	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	54.200%	
66) 1,2-Dichlorobenzene-d4	13.853	152	62388	17.940	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	71.760%#	
Target Compounds						Qvalue
25) Chloroform	7.677	83	5914	0.977	ug/L	99
34) Trichloroethene	9.085	95	3709	1.064	ug/L #	83
46) Tetrachloroethene	10.866	164	2131812	787.194	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024369.D
Acq On : 26 Aug 2022 23:12
Operator : SY/VA
Sample : N4344-09
Misc : 5.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBVQ8

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 08/30/2022
Supervised By : Mahesh Dadoda 08/30/2022


Quant Time: Aug 27 00:46:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 27 00:35:21 2022
Response via : Initial Calibration

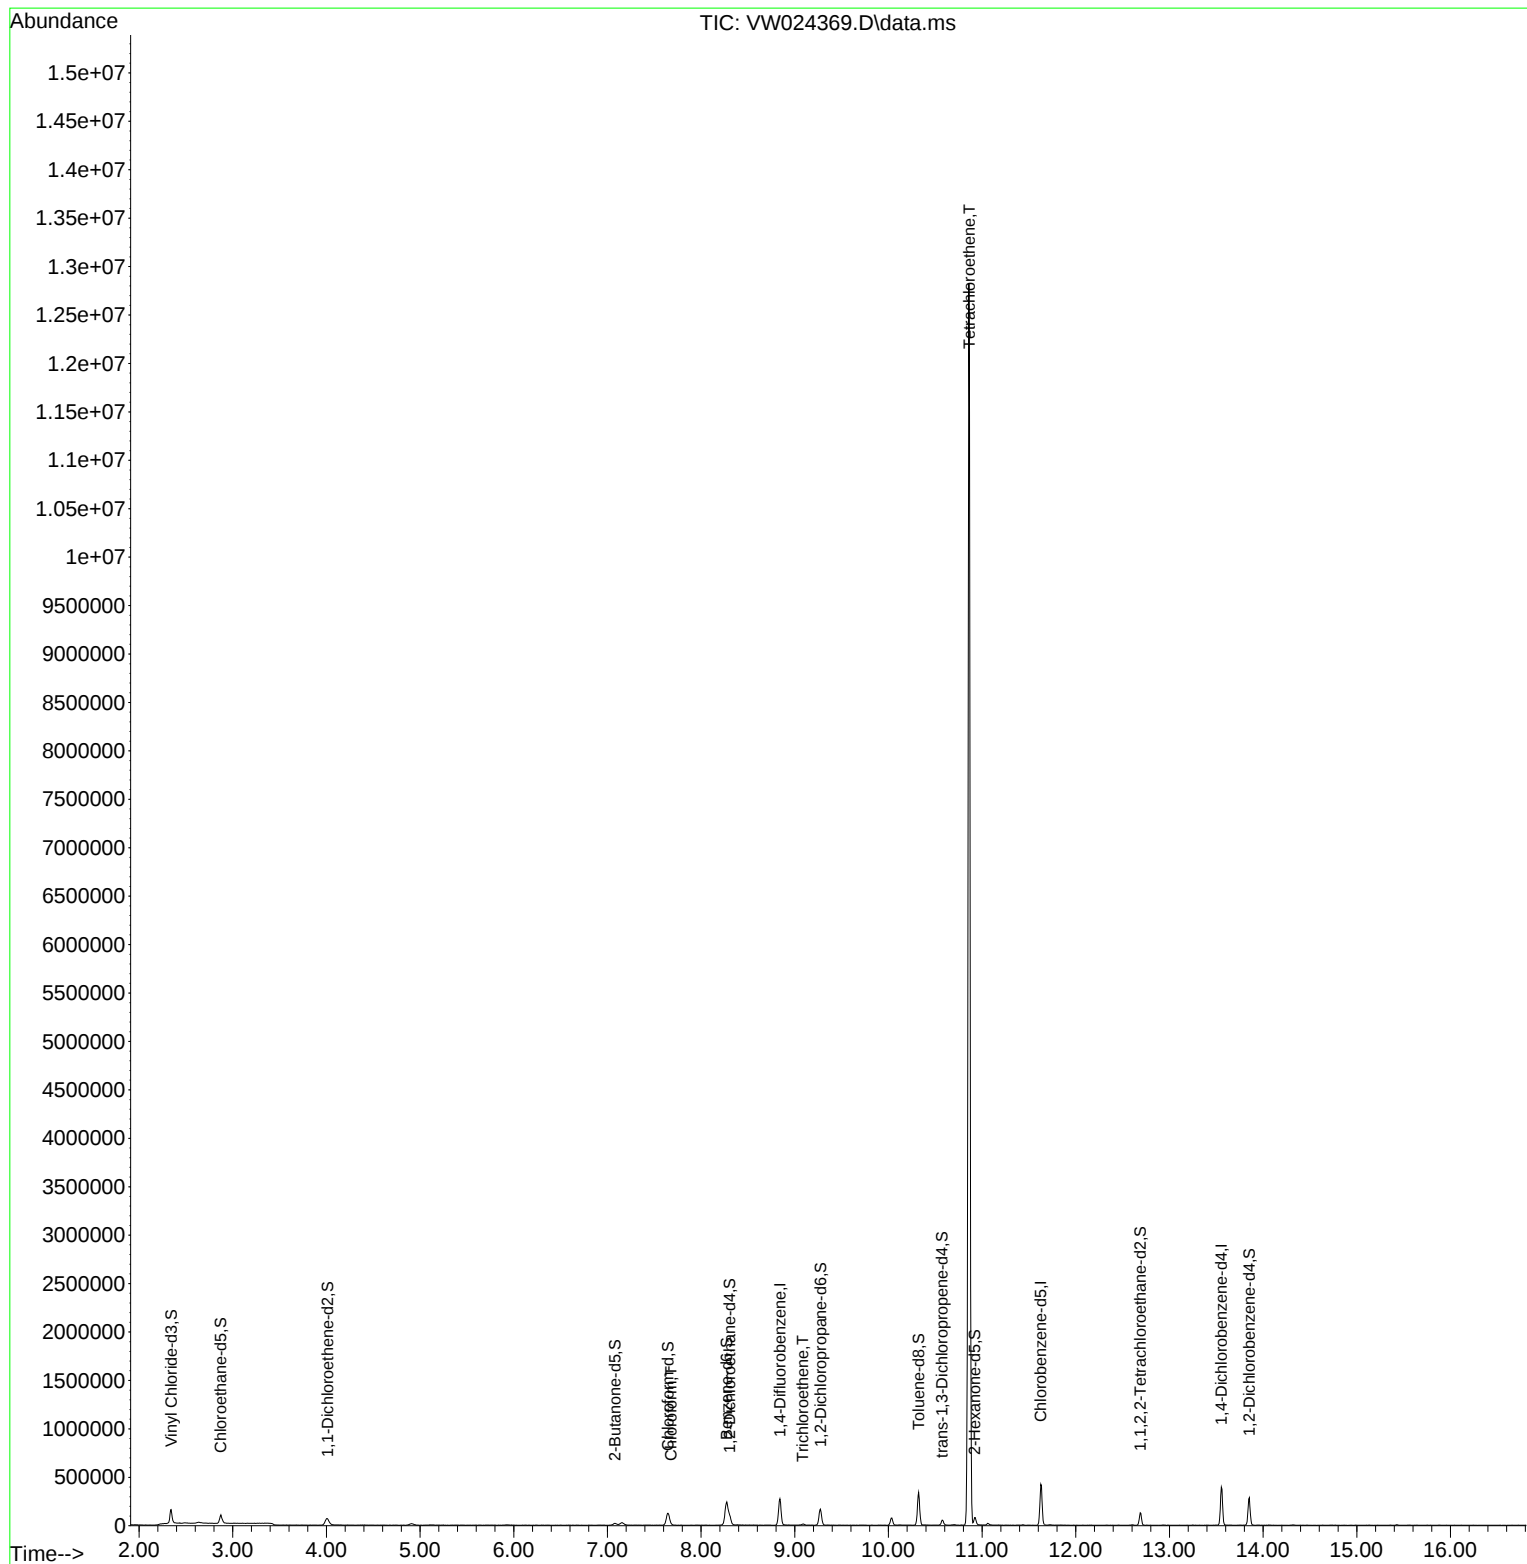

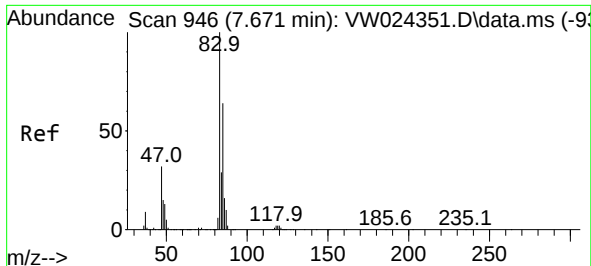

#25
Chloroform
Concen: 0.977 ug/L
RT: 7.677 min Scan# 946
Delta R.T. 0.006 min
Lab File: VW024369.D
Acq: 26 Aug 2022 23:12




Instrument :
MSVOA_W
ClientSampleId :
DBVQ8

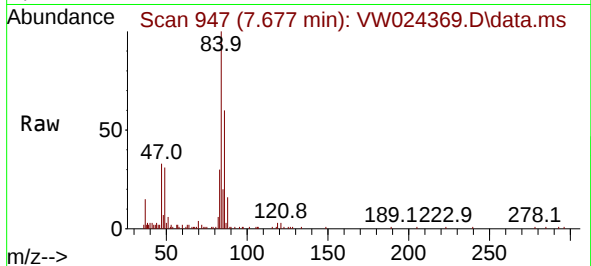

Tgt Ion: 83 Resp: 5914
Ion Ratio Lower Upper
83 100
85 68.8 47.5 88.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

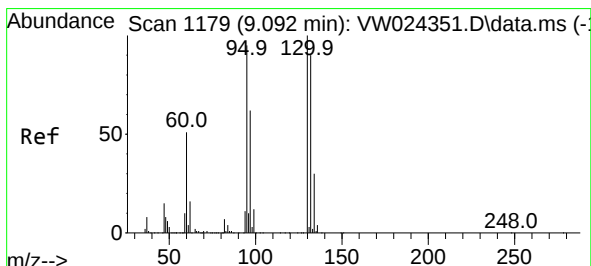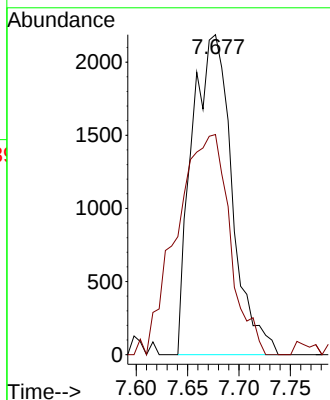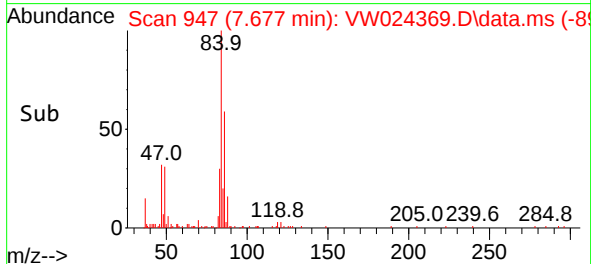

#34
Trichloroethene
Concen: 1.064 ug/L
RT: 9.085 min Scan# 1178
Delta R.T. -0.006 min
Lab File: VW024369.D
Acq: 26 Aug 2022 23:12


Tgt Ion: 95 Resp: 3709
Ion Ratio Lower Upper
95 100
97 47.3 48.4 89.8#
132 99.9 68.6 127.4
130 78.5 72.6 134.8

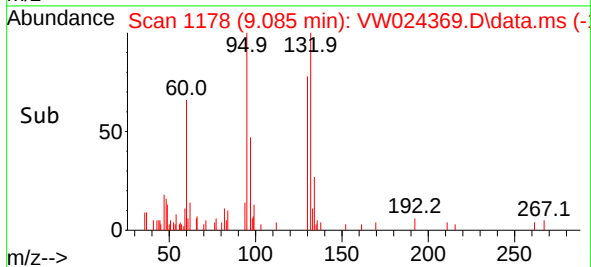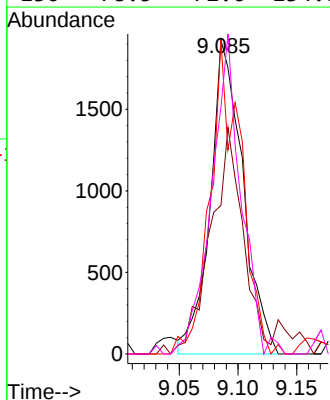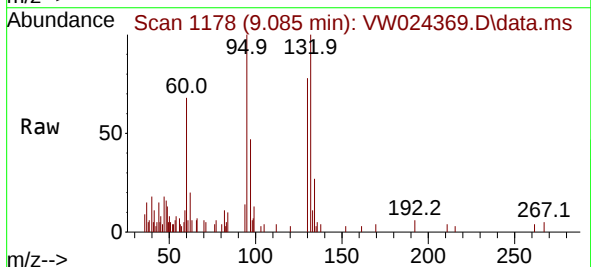

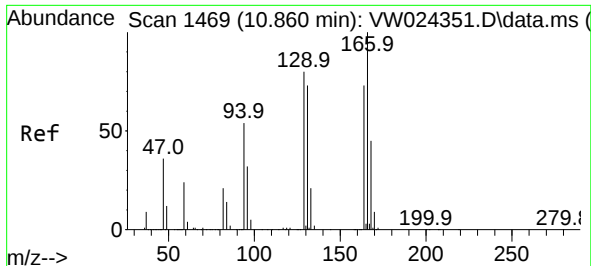

#46
Tetrachloroethene
Concen: 787.194 ug/L
RT: 10.866 min Scan# 14
Delta R.T. 0.006 min
Lab File: VW024369.D
Acq: 26 Aug 2022 23:12

Instrument :
MSVOA_W
ClientSampleId :
DBVQ8

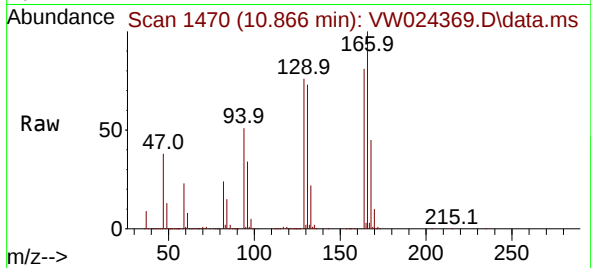

Tgt Ion:164 Resp: 213181
Ion Ratio Lower Upper
164 100
129 94.0 72.9 135.3
131 90.3 63.7 118.3
166 123.0 86.2 160.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

