

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082718\
 Data File : VW004970.D
 Acq On : 27 Aug 2018 18:00
 Operator : SY/AP
 Sample : J4634-13
 Misc : 5.70G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB3H4

Quant Time: Aug 28 01:40:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 28 01:39:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	605100	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	641686	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	280962	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	227341	19.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.52%
7) Chloroethane-d5	2.89	69	182567	21.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.12%
10) 1,1-Dichloroethene-d2	4.02	63	248078	16.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.96%
20) 2-Butanone-d5	7.09	46	96348	41.39	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.78%
24) Chloroform-d	7.65	84	308854	22.99	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.96%
26) 1,2-Dichloroethane-d4	8.31	65	179678	24.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.44%
29) Benzene-d6	8.28	84	696720	21.11	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.44%
33) 1,2-Dichloropropane-d6	9.28	67	210352	21.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.76%
37) Toluene-d8	10.33	98	741067	21.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.76%
38) trans-1,3-Dichloropropene-	10.58	79	84544	20.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.04%
39) 2-Hexanone-d5	10.93	63	96538	40.18	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.36%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	212531	21.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.24%
61) 1,2-Dichlorobenzene-d4	13.86	152	272135	24.11	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.44%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	13.57	75	30414	3.942	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082718\
Data File : VW004970.D
Acq On : 27 Aug 2018 18:00
Operator : SY/AP
Sample : J4634-13
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB3H4

Quant Time: Aug 28 01:40:48 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 28 01:39:39 2018
Response via : Initial Calibration

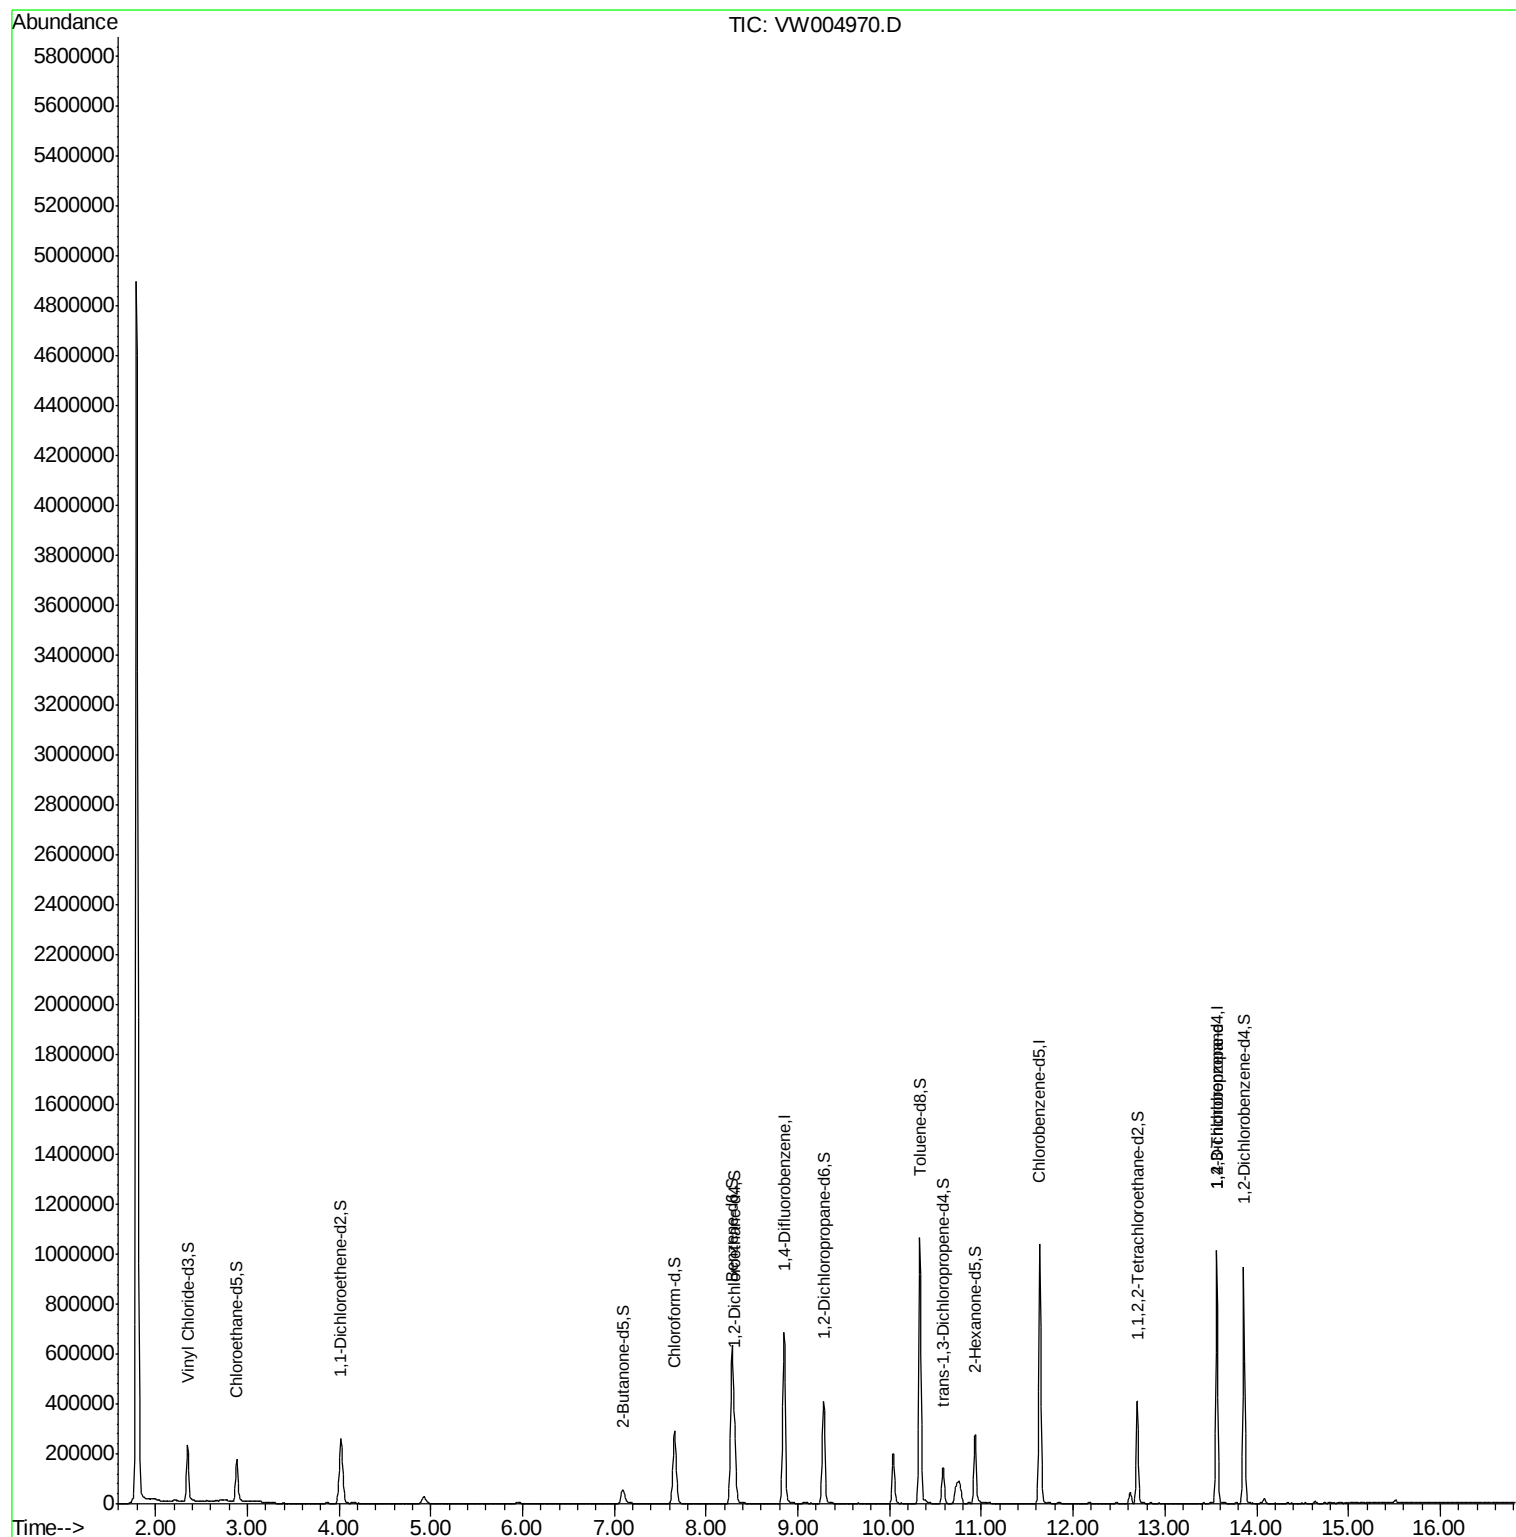

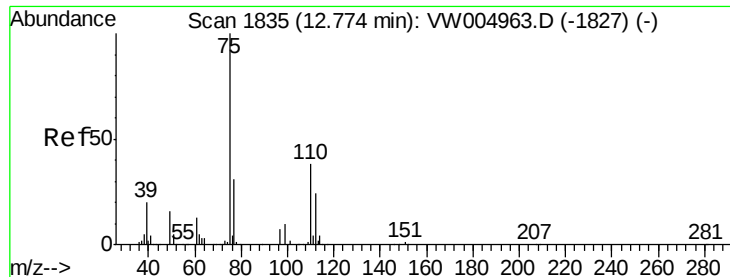

#59

1,2,3-Trichloropropane

Concen: 3.942 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW004970.D

Acq: 27 Aug 2018 18:00

Instrument :

MSVOA_W

ClientSampleId :

DB3H4

Tgt Ion: 75 Resp: 30414

Ion Ratio Lower Upper

75 100

77 36.1 25.3 37.9

