

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082720\
 Data File : VW016383.D
 Acq On : 27 Aug 2020 11:22
 Operator : SY/VA
 Sample : L3800-08
 Misc : 6.58G/10ML/MSVOA W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3H7

Manual Integrations
 APPROVED

MMDadoda
 8/28/2020 3:18:22 PM

Quant Time: Aug 28 08:10:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 28 08:08:30 2020
 Response via : Initial Calibration

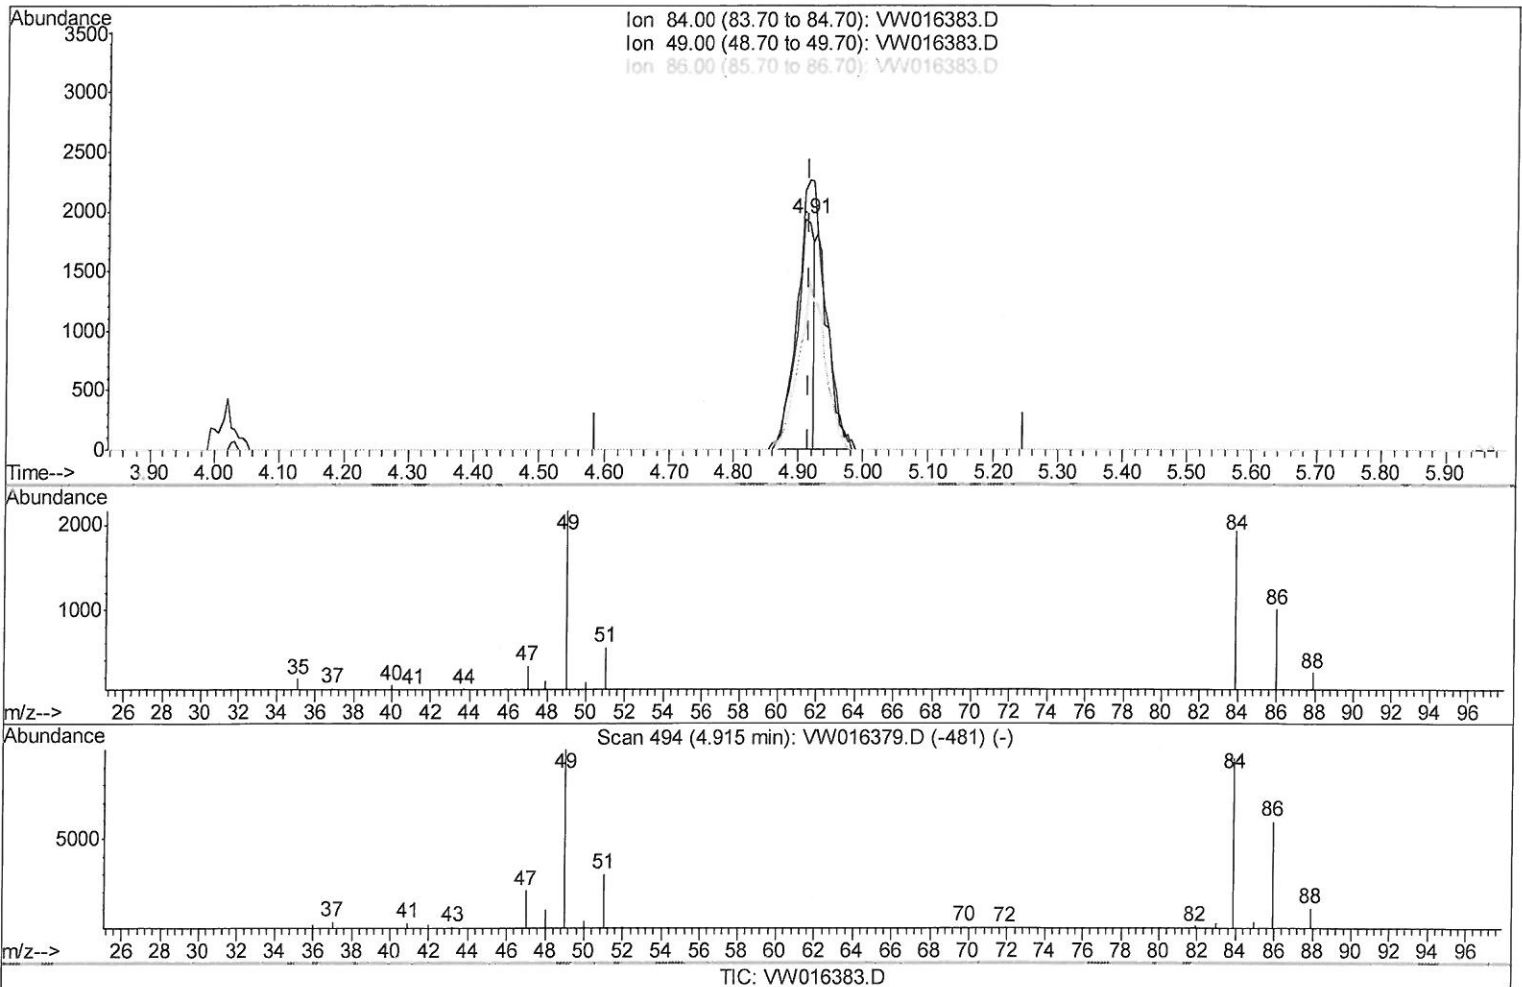

(16) Methylene chloride (T)

4.909min (-0.006) 2.70ug/L

response 3539

Ion	Exp%	Act%
84.00	100	100
49.00	107.60	112.00
86.00	61.80	51.96
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082720\
 Data File : VW016383.D
 Acq On : 27 Aug 2020 11:22
 Operator : SY/VA
 Sample : L3800-08
 Misc : 6.58G/10ML/MSVOA W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG3H7

Manual Integrations
 APPROVED

MMDadoda
 8/28/2020 3:18:22 PM

Quant Time: Aug 28 08:10:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 28 08:08:30 2020
 Response via : Initial Calibration

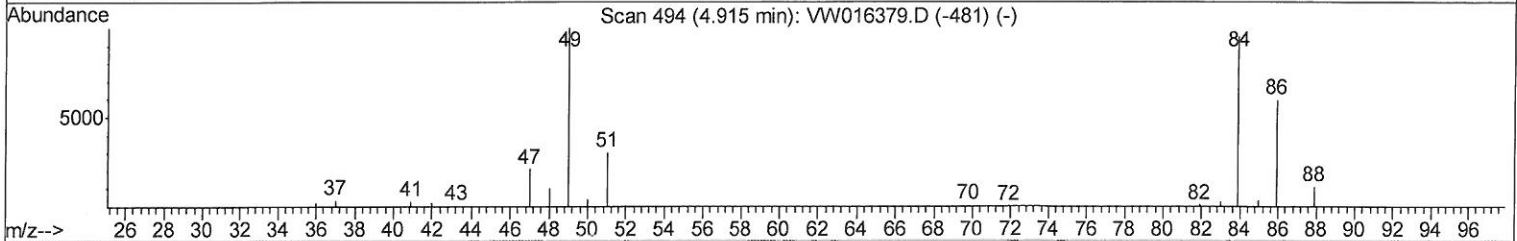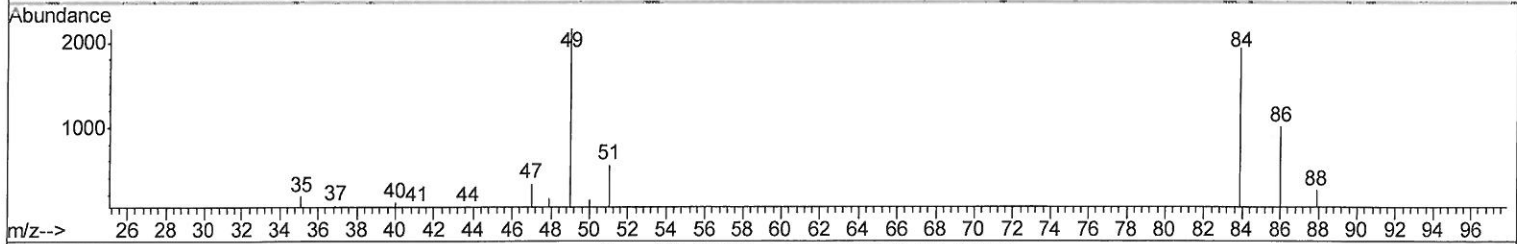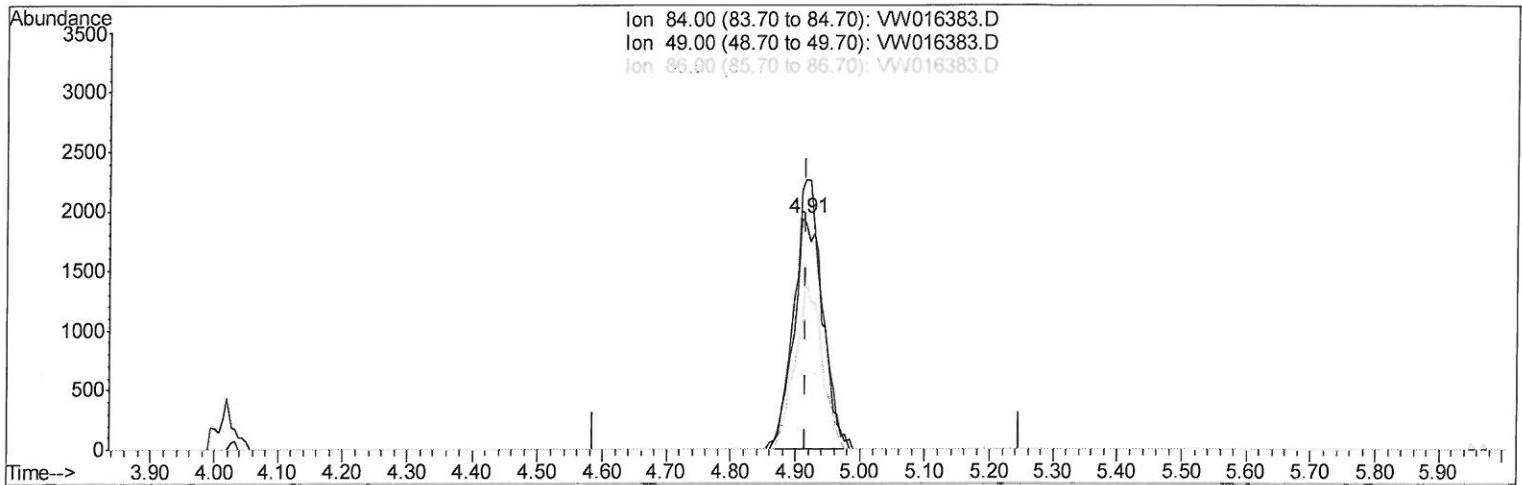

TIC: VW016383.D

(16) Methylene chloride (T)

4.909min (-0.006) 4.66ug/L m

response 6102

Ion	Exp%	Act%
84.00	100	100
49.00	107.60	112.00
86.00	61.80	51.96
0.00	0.00	0.00

208/28/20 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082720\
 Data File : VW016383.D
 Acq On : 27 Aug 2020 11:22
 Operator : SY/VA
 Sample : L3800-08
 Misc : 6.58G/10ML/MSVOA W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3H7

Manual Integrations
 APPROVED

MMDadoda
 8/28/2020 3:18:22 PM

Quant Time: Aug 28 08:28:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 28 08:08:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	70863	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	60532	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	15763	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	12719	16.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.24%
7) Chloroethane-d5	2.89	69	12178	21.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.80%
10) 1,1-Dichloroethene-d2	4.02	63	24113	13.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.68%
20) 2-Butanone-d5	7.08	46	9558	44.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.84%
24) Chloroform-d	7.65	84	41731	22.59	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.36%
26) 1,2-Dichloroethane-d4	8.31	65	22690	23.83	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.32%
29) Benzene-d6	8.27	84	71879	21.27	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.08%
33) 1,2-Dichloropropane-d6	9.27	67	22517	24.08	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.32%
37) Toluene-d8	10.33	98	58270	18.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.12%
38) trans-1,3-Dichloropropene-	10.59	79	8982	19.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.60%
39) 2-Hexanone-d5	10.93	63	6871	45.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.72%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	18355	23.58	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.32%
61) 1,2-Dichlorobenzene-d4	13.86	152	12839	21.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.96%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.12	43	2415	13.524	ug/L	59
16) Methylene chloride	4.91	84	6102m	4.658	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082720\
Data File : VW016383.D
Acq On : 27 Aug 2020 11:22
Operator : SY/VA
Sample : L3800-08
Misc : 6.58G/10ML/MSVOA W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3H7

Manual Integrations
APPROVED

MMDadoda
8/28/2020 3:18:22 PM

Quant Time: Aug 28 08:28:48 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082420S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 28 08:08:30 2020
Response via : Initial Calibration

