

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082721\
 Data File : VW019924.D
 Acq On : 27 Aug 2021 10:04
 Operator : SY/VA
 Sample : VW0827SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 28 00:42:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 28 00:41:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	360730	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	335566	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	160480	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	119835	21.441	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.760%
7) Chloroethane-d5	2.898	69	109165	22.252	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	4.025	63	152526	15.727	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.920%
21) 2-Butanone-d5	7.086	46	50737	44.691	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.380%
24) Chloroform-d	7.653	84	225660	22.747	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	8.311	65	122653	22.942	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.760%
32) Benzene-d6	8.281	84	450929	23.568	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.280%
36) 1,2-Dichloropropane-d6	9.274	67	136938	23.634	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.520%
41) Toluene-d8	10.323	98	405940	23.152	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.600%
43) trans-1,3-Dichloroprop...	10.579	79	54536	22.784	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.120%
47) 2-Hexanone-d5	10.927	63	34919	43.261	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.520%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	108345	22.975	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	140764	25.571	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.280%
Target Compounds						Qvalue
34) Trichloroethene	8.848	95	10487	1.959	ug/L	# 5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082721\
Data File : VW019924.D
Acq On : 27 Aug 2021 10:04
Operator : SY/VA
Sample : VW0827SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 28 00:42:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 28 00:41:11 2021
Response via : Initial Calibration

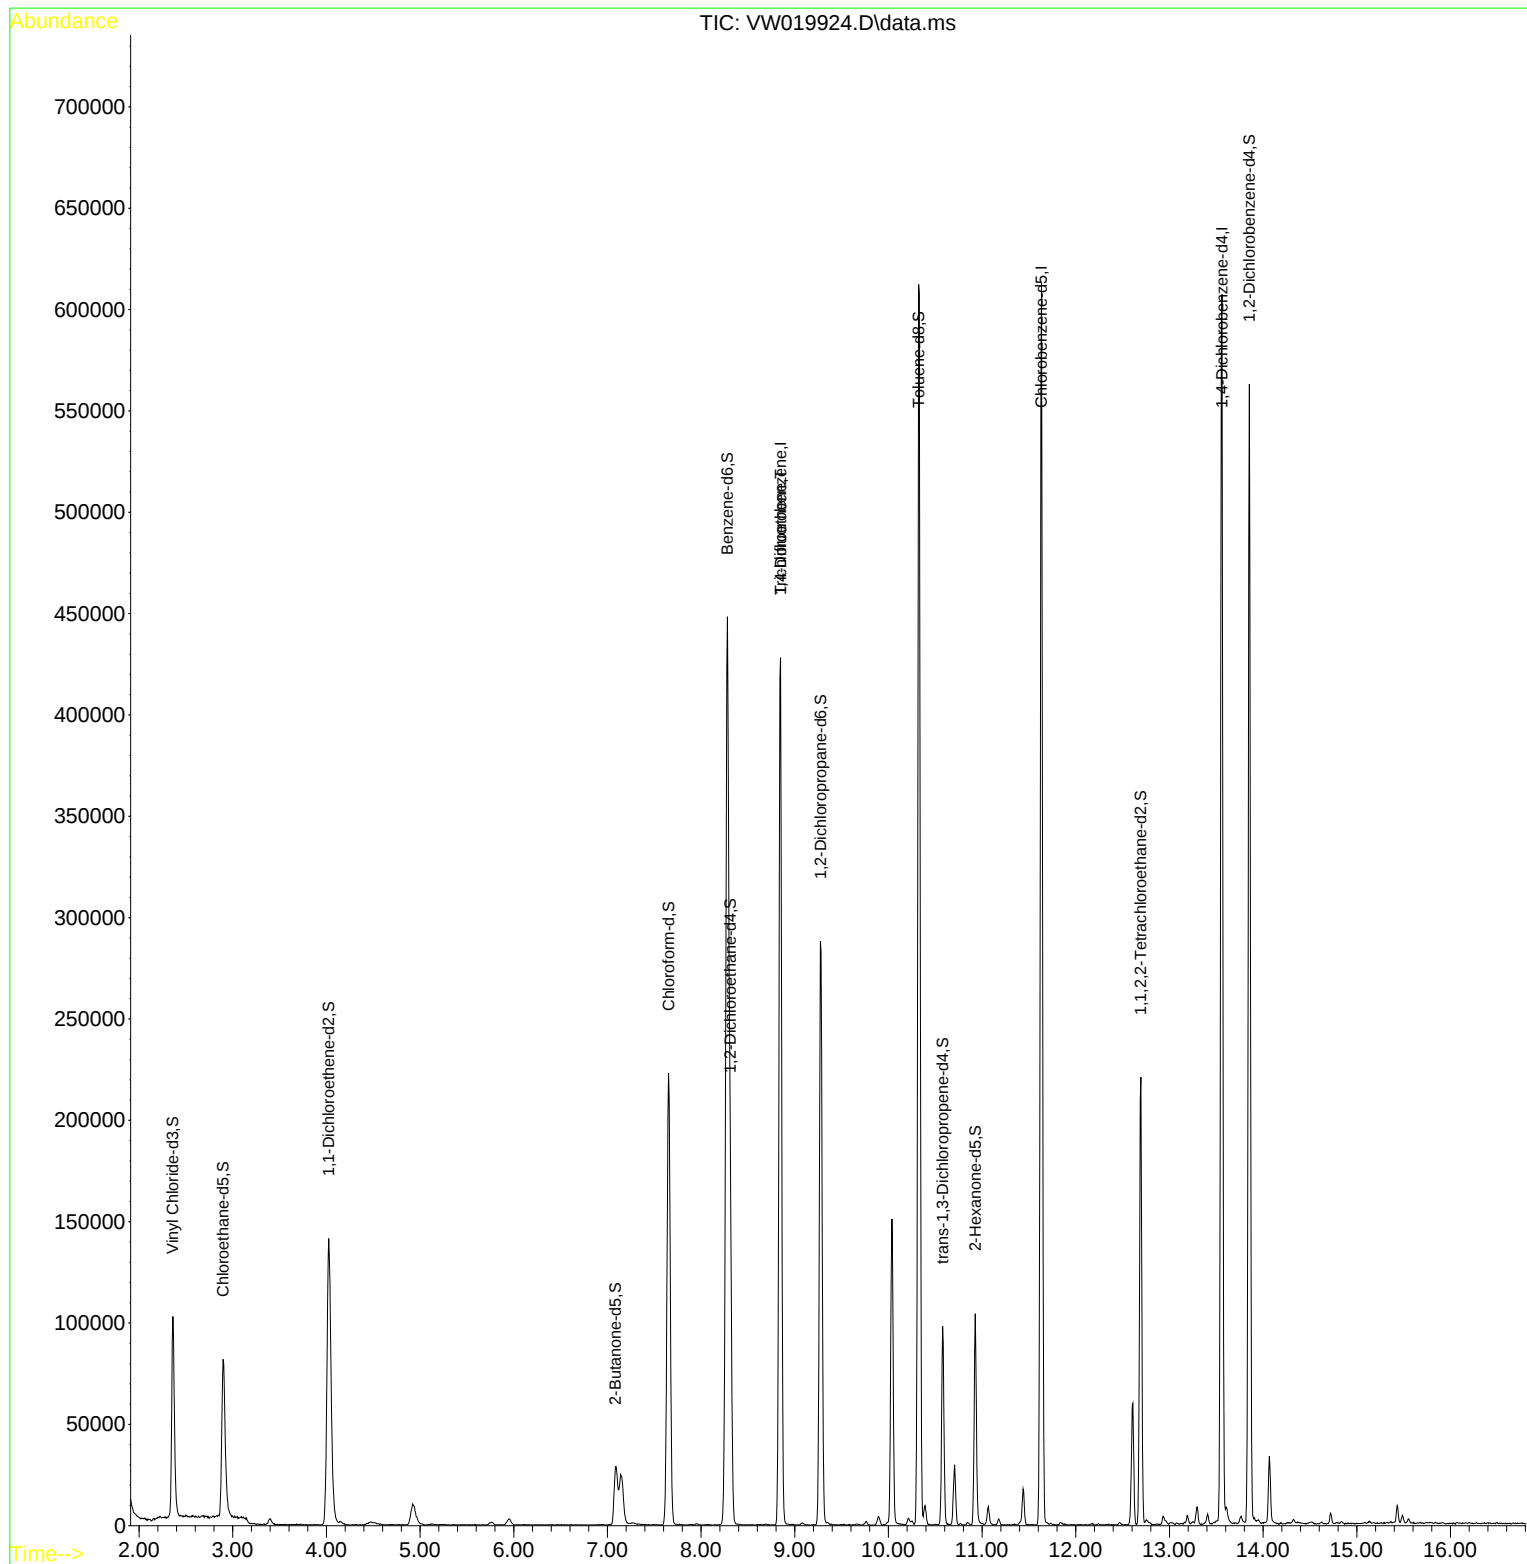

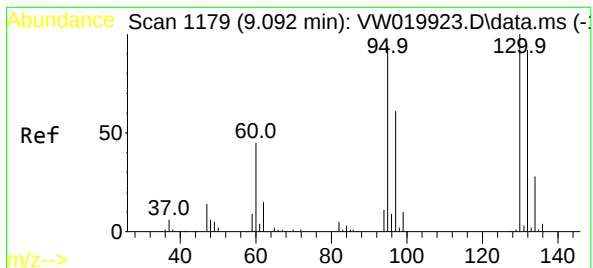

#34
 Trichloroethene
 Concen: 1.959 ug/L
 RT: 8.848 min Scan# 1139
 Delta R.T. -0.244 min
 Lab File: VW019924.D
 Acq: 27 Aug 2021 10:04

Instrument :
 MSVOA_W
 ClientSampleId :

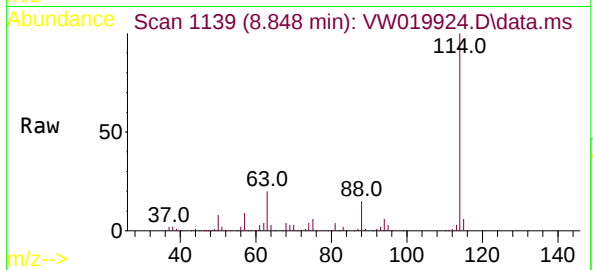

Tgt Ion: 95 Resp: 10487
 Ion Ratio Lower Upper
 95 100
 97 0.0 47.3 87.8#
 132 0.0 71.0 131.8#
 130 0.0 65.1 120.9#

