

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082819\
 Data File : VW012255.D
 Acq On : 28 Aug 2019 15:41
 Operator : SY/VA
 Sample : K4509-05
 Misc : 5.05G/5ML/MSVOA W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-50-10.5-11.0

Quant Time: Aug 28 18:42:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 26 07:18:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	239790	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	395963	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	315201	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	114388	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	144002	50.52	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.04%	
35) Dibromofluoromethane	7.88	113	117756	49.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.64%	
50) Toluene-d8	10.32	98	480953	50.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.38%	
62) 4-Bromofluorobenzene	12.62	95	143888	42.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	85.18%	
Target Compounds						
20) Methylene Chloride	4.92	84	25414	9.226	ug/l	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW082819\
Data File : VW012255.D
Acq On : 28 Aug 2019 15:41
Operator : SY/VA
Sample : K4509-05
Misc : 5.05G/5ML/MSVOA W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-50-10.5-11.0

Quant Time: Aug 28 18:42:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 26 07:18:31 2019
Response via : Initial Calibration

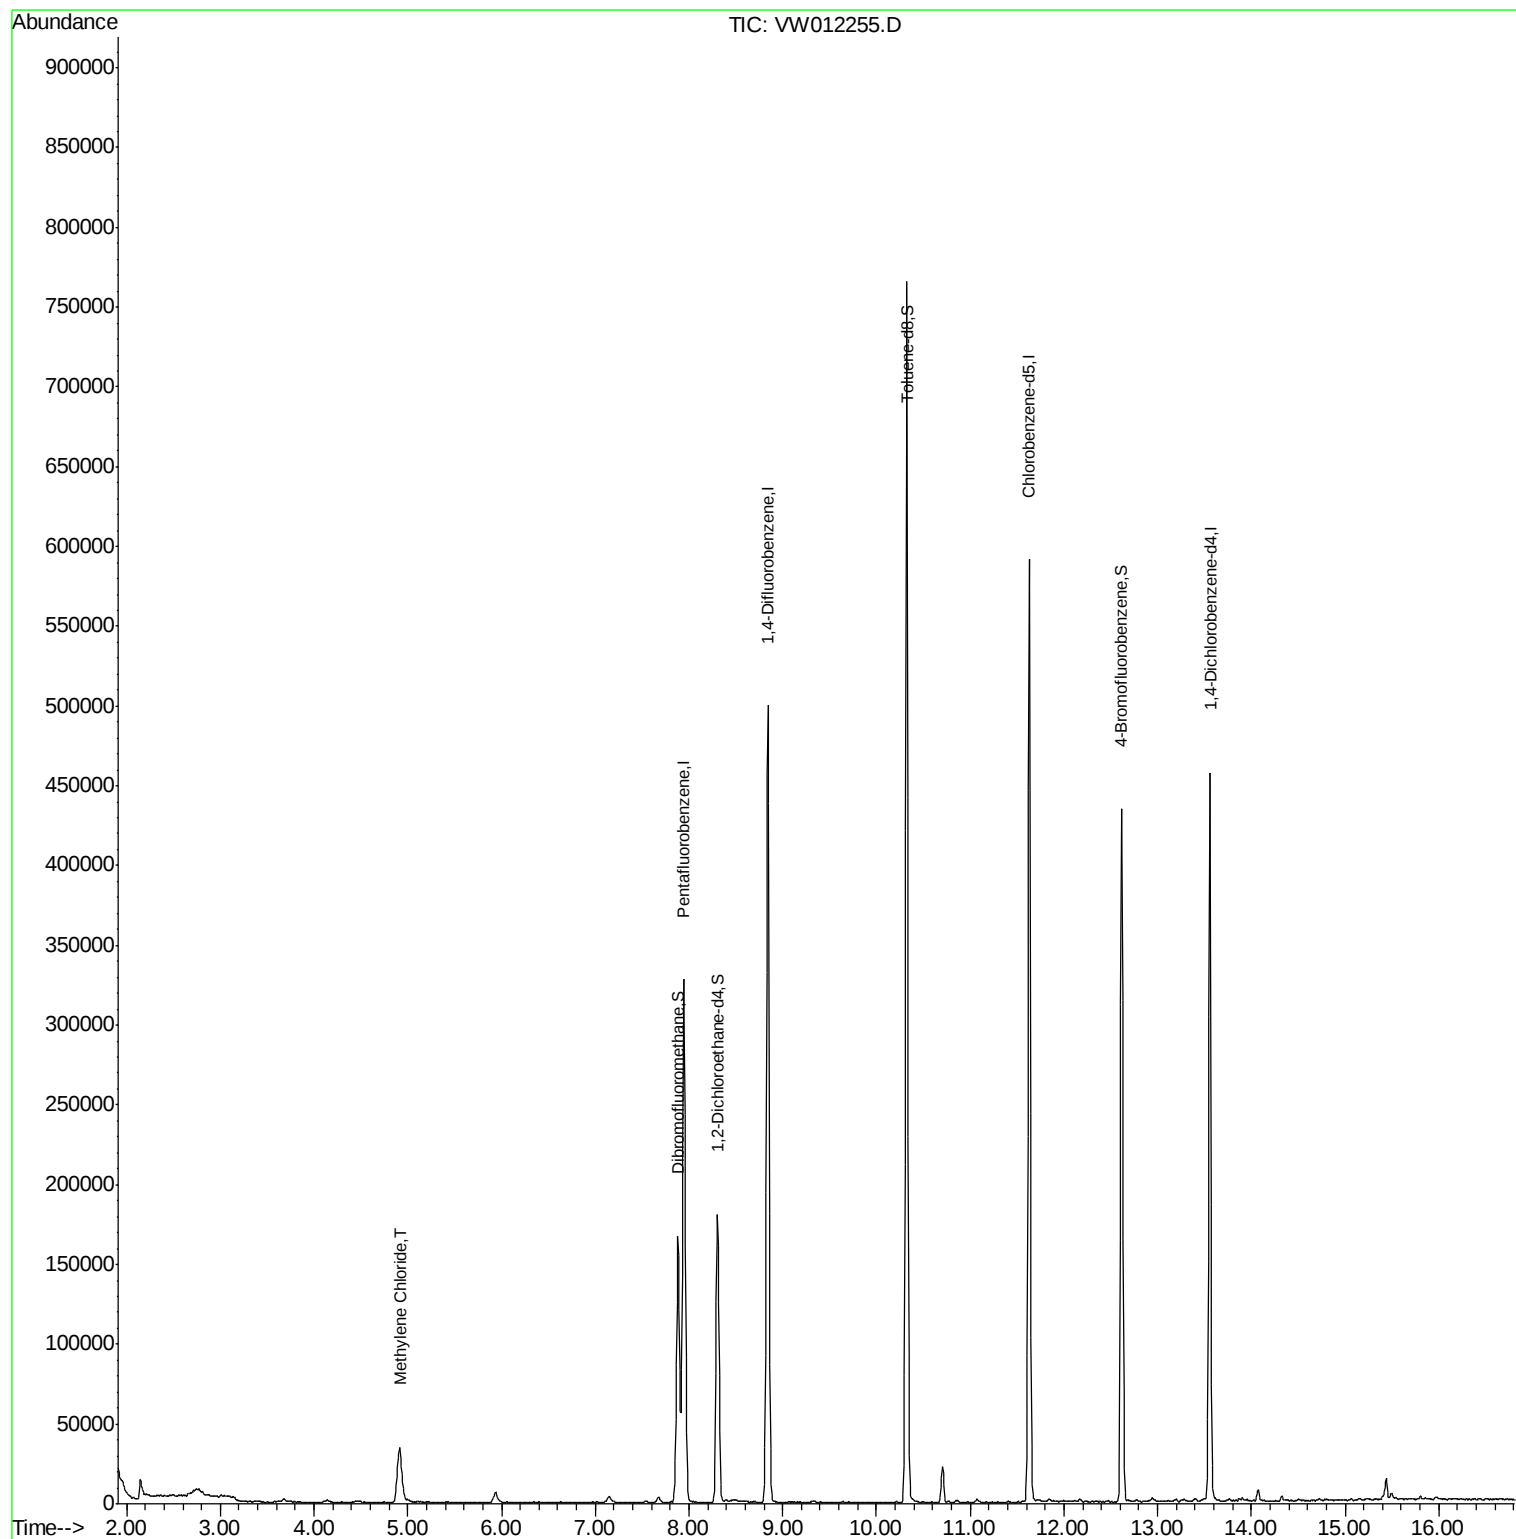



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.01 min

Lab File: VW012255.D

Acq: 28 Aug 2019 15:41

Instrument :

MSVOA_W

ClientSampleId :


SB-50-10.5-11.0

Tot Ion:168 Resp: 239790

Ion Ratio Lower Upper

168 100

99 55.8 49.2 73.8

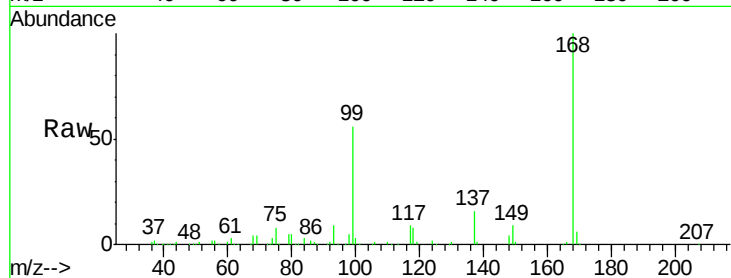

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

120000

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00

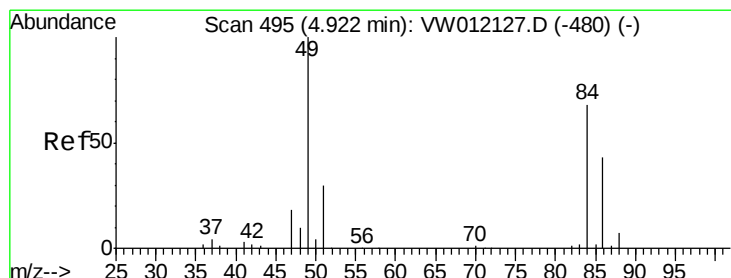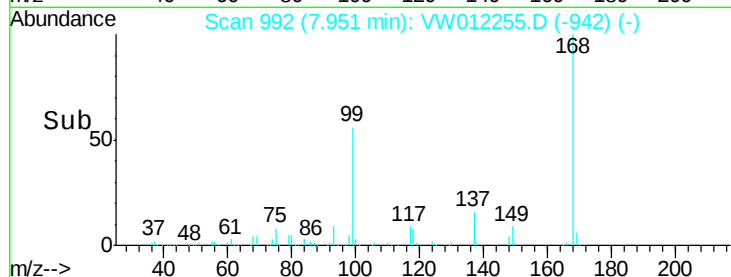

#20

Methylene Chloride

Concen: 9.226 ug/l

RT: 4.92 min Scan# 494

Delta R.T. -0.01 min

Lab File: VW012255.D

Acq: 28 Aug 2019 15:41

Tgt Ion: 84 Resp: 25414


Ion Ratio Lower Upper

84 100

49 146.7 117.8 176.8

51 39.0 35.6 53.4

86 58.4 51.2 76.8

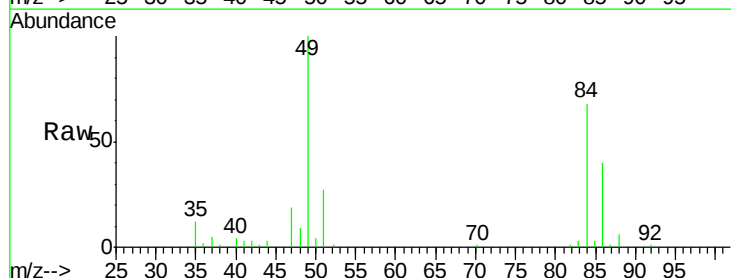

Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW


15000


10000

5000

0

Time--> 4.80 4.90 5.00 5.10

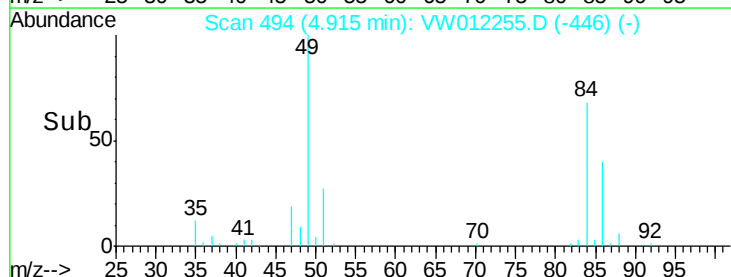

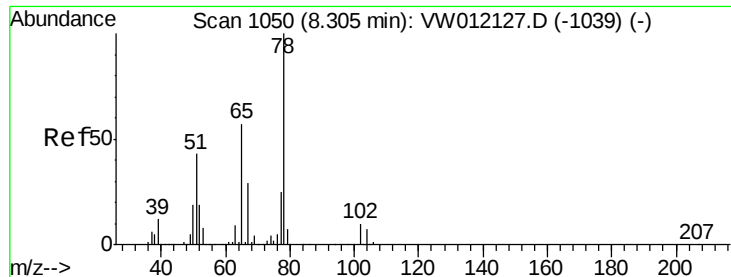

#33

1,2-Dichloroethane-d4

Concen: 50.518 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW012255.D

Acq: 28 Aug 2019 15:41

Instrument :

MSVOA_W

ClientSampleId :





SB-50-10.5-11.0

Tot Ion: 65 Resp: 144002

Ion Ratio Lower Upper

65 100

67 51.7 0.0 102.6

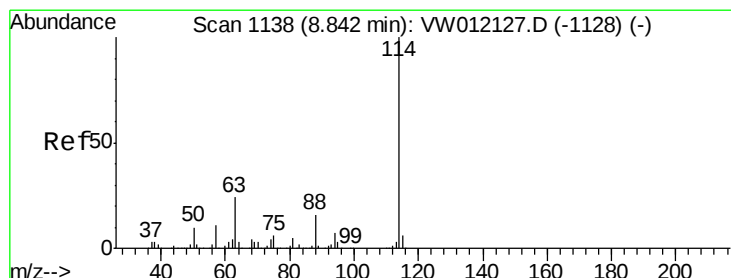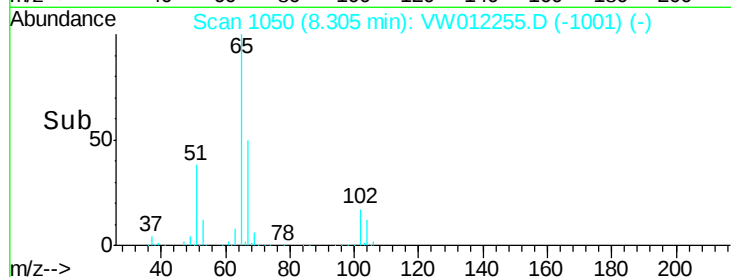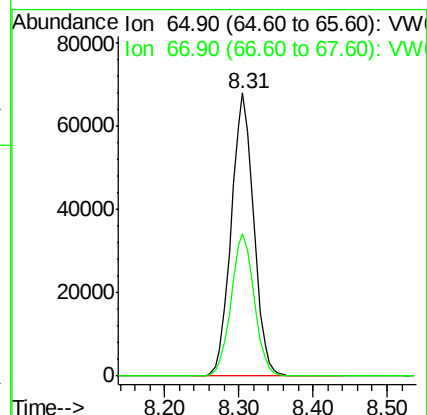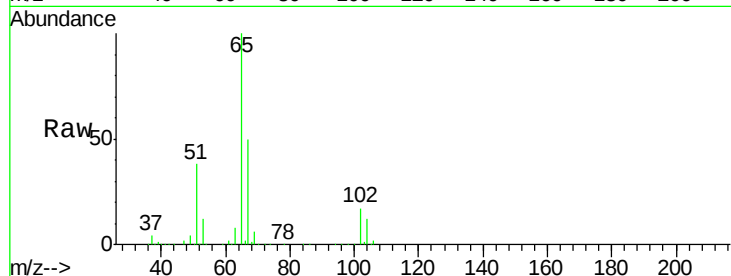

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. -0.00 min

Lab File: VW012255.D

Acq: 28 Aug 2019 15:41




Tgt Ion: 114 Resp: 395963

Ion Ratio Lower Upper

114 100

63 23.2 0.0 48.6

88 16.1 0.0 32.2


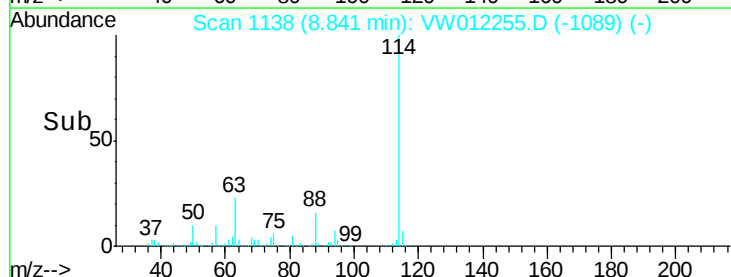
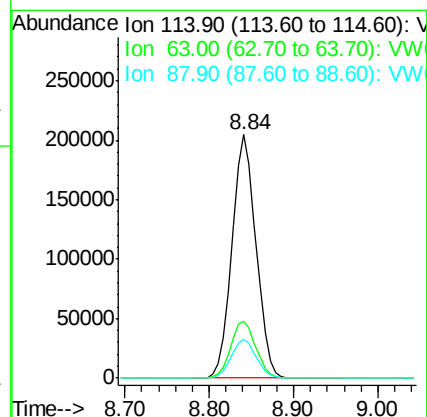
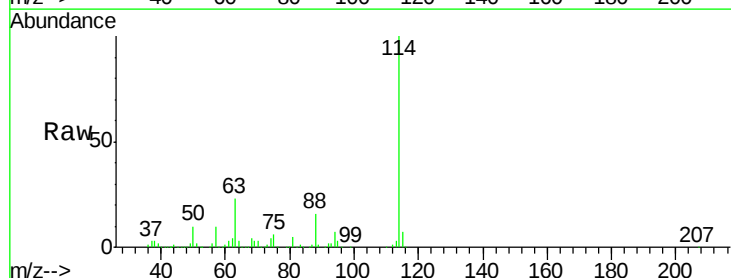




#35
 Dibromofluoromethane
 Concen: 49.822 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW012255.D
 Acq: 28 Aug 2019 15:41




Instrument :
 MSVOA_W
 ClientSampleId :
 SB-50-10.5-11.0


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.7	82.7	124.1
192	20.2	16.2	24.2

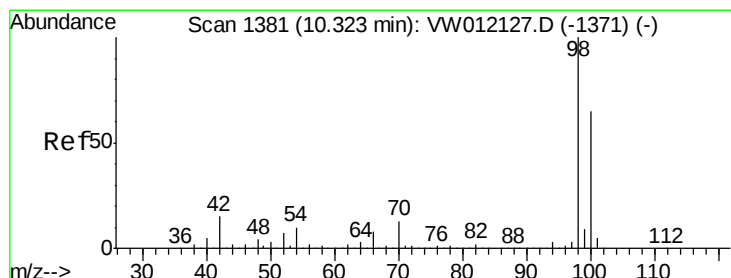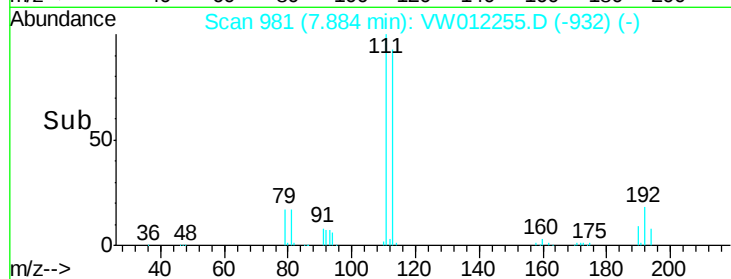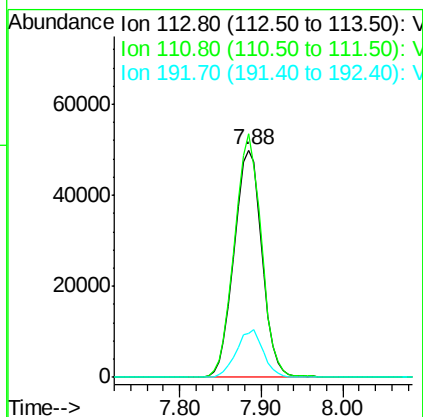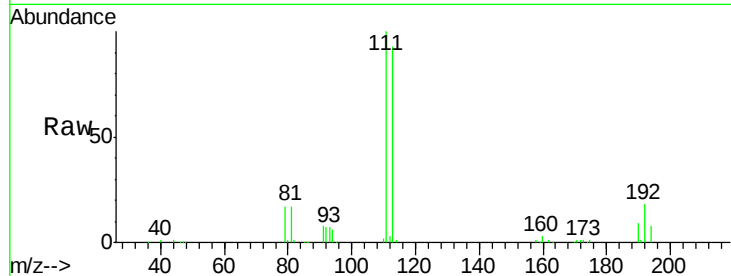

#50
 Toluene-d8
 Concen: 50.186 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. -0.00 min
 Lab File: VW012255.D
 Acq: 28 Aug 2019 15:41

Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.4	52.4	78.6

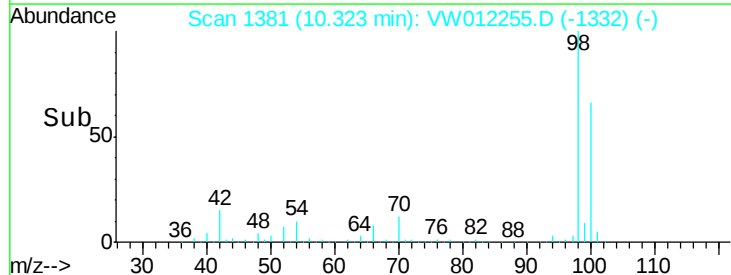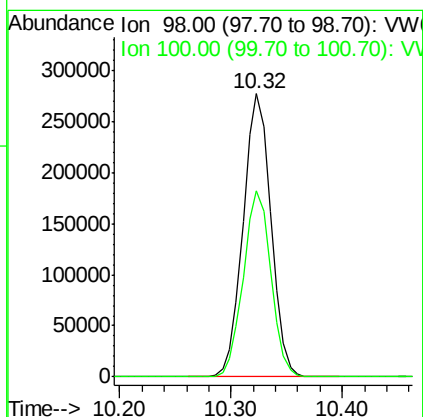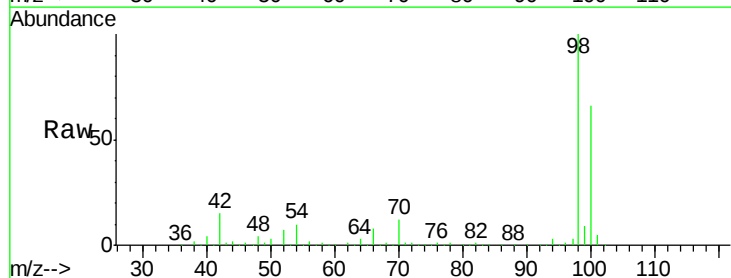

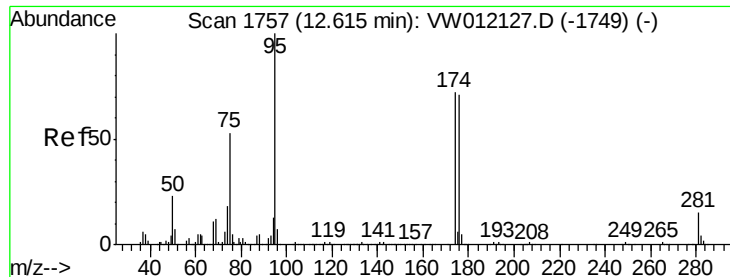

#62

4-Bromofluorobenzene

Concen: 42.594 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. -0.00 min

Lab File: VW012255.D

Acq: 28 Aug 2019 15:41

Instrument :

MSVOA_W

ClientSampleId :

SB-50-10.5-11.0





Tot Ion: 95 Resp: 143888

Ion Ratio Lower Upper

95 100

174 76.2 0.0 150.8

176 73.1 0.0 148.6

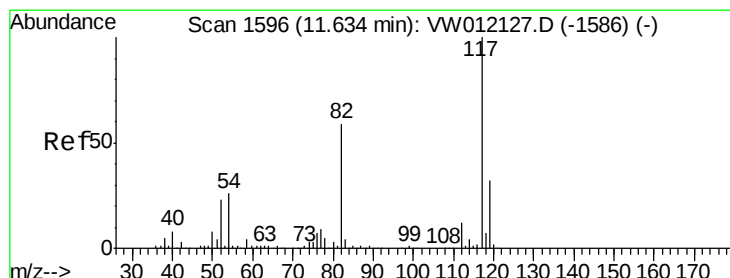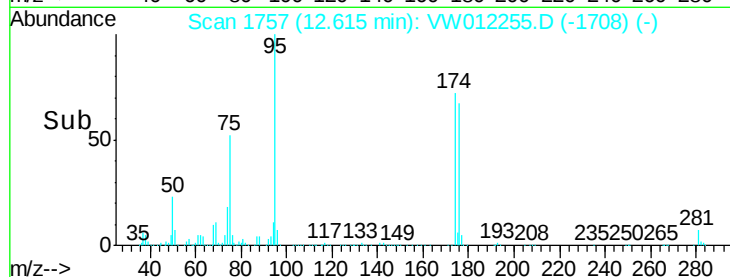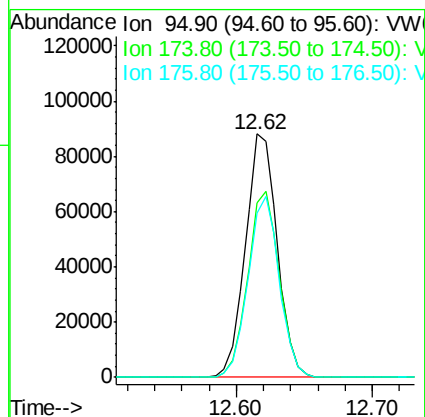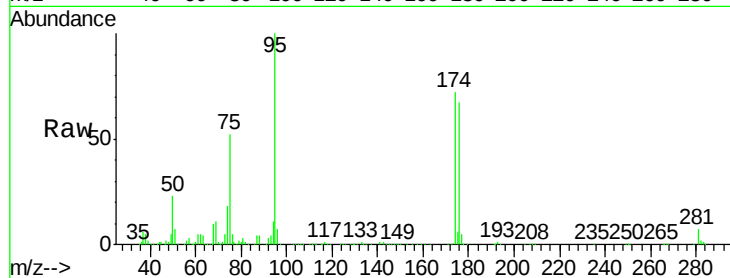

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. -0.00 min

Lab File: VW012255.D

Acq: 28 Aug 2019 15:41




Tgt Ion: 117 Resp: 315201


Ion Ratio Lower Upper

117 100

82 59.9 47.4 71.2

119 32.3 25.4 38.2

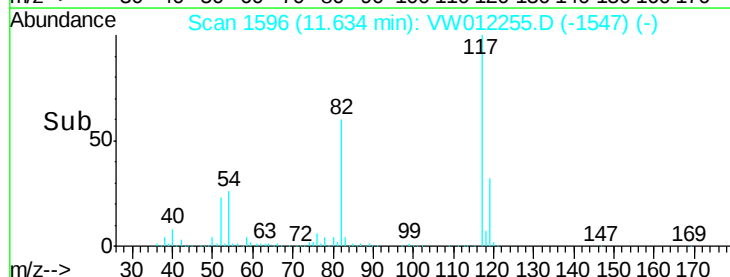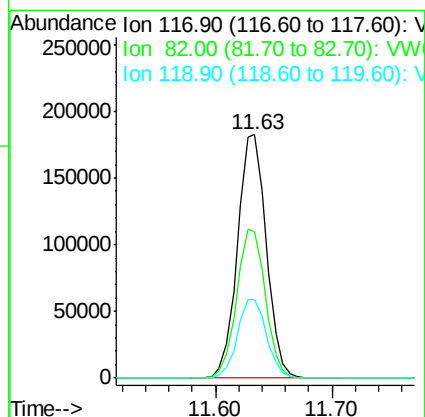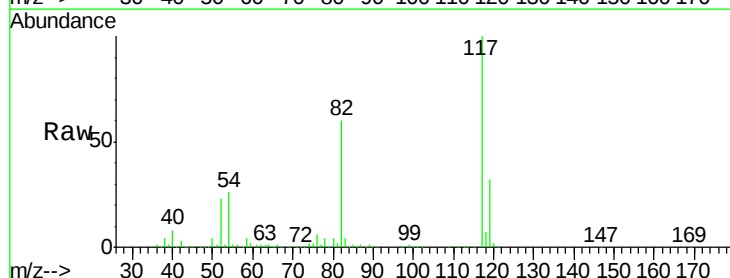

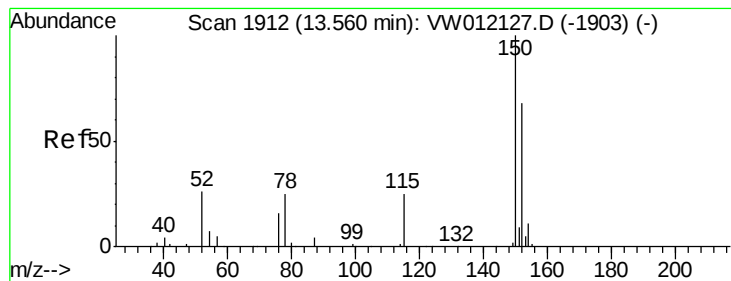

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. -0.00 min

Lab File: VW012255.D

Acq: 28 Aug 2019 15:41

Instrument :

MSVOA_W

ClientSampleId :

SB-50-10.5-11.0


Tot Ion:152 Resp: 114388

Ion Ratio Lower Upper

152 100

115 60.2 30.1 90.3

150 158.2 0.0 345.8

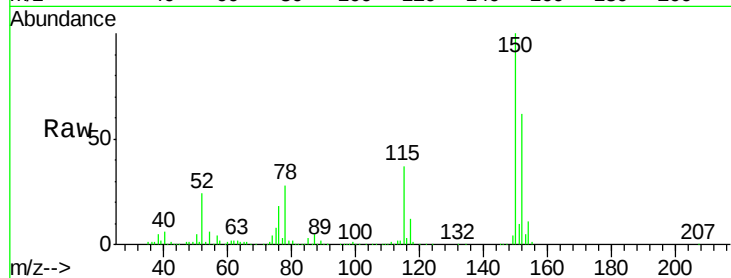

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

