


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW082819\
 Data File : VW012242.D
 Acq On : 28 Aug 2019 09:37
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
 Title : SW846 8260
 Last Update : Mon Aug 26 07:18:31 2019

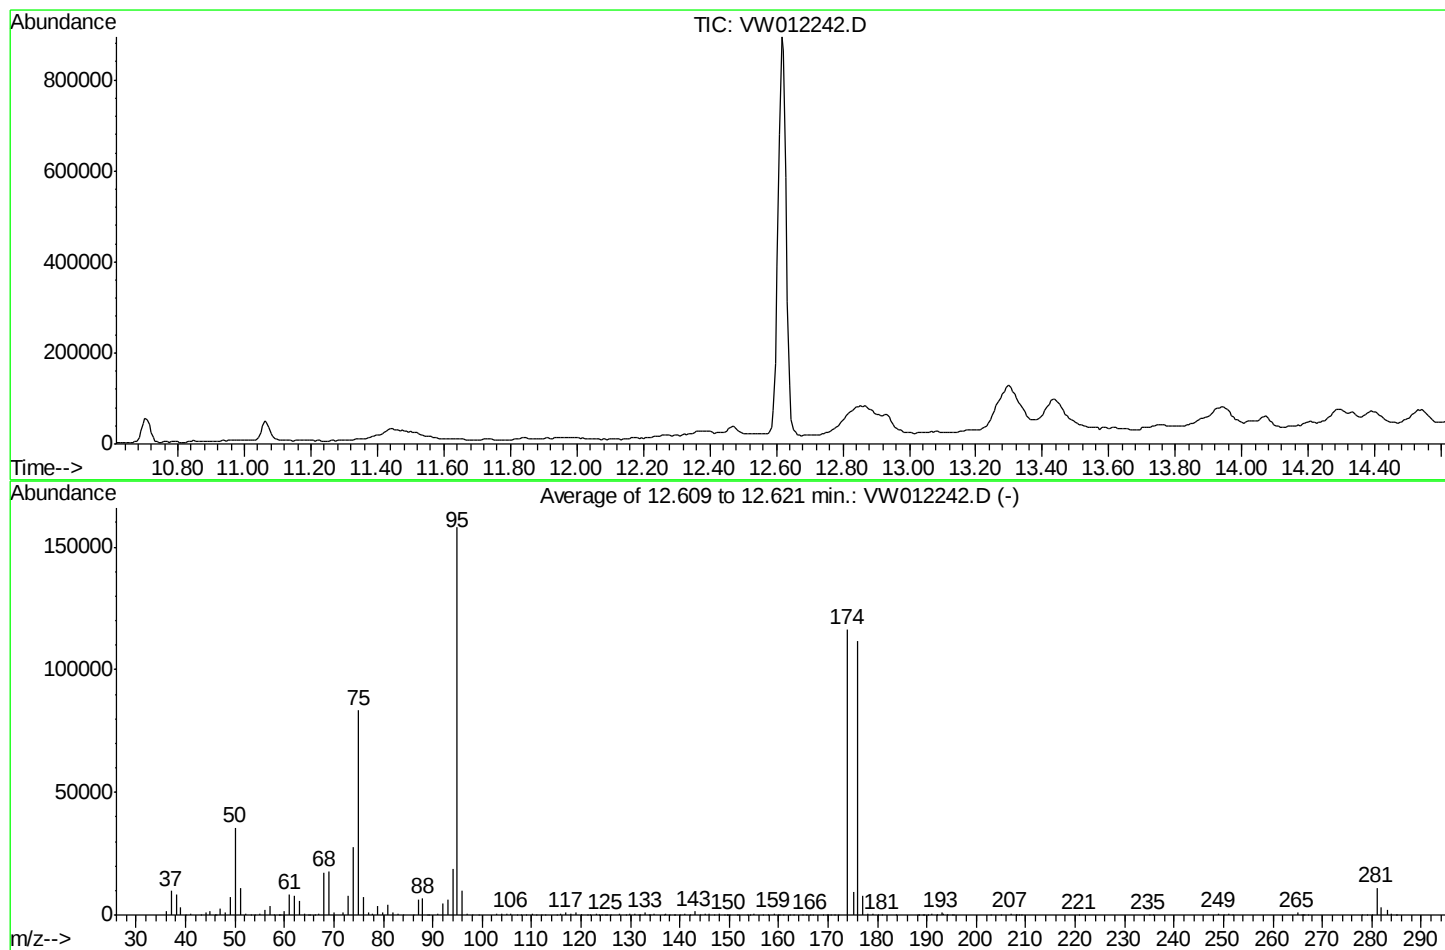

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	35728	PASS
75	95	30	60	52.8	83418	PASS
95	95	100	100	100.0	158003	PASS
96	95	5	9	6.4	10187	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.6	116325	PASS
175	174	5	9	8.1	9437	PASS
176	174	95	101	96.0	111642	PASS
177	176	5	9	7.0	7764	PASS