


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW082820\
 Data File : VW016394.D
 Acq On : 28 Aug 2020 10:02
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082820S.M
 Title : SW846 8260
 Last Update : Fri Aug 28 15:01:43 2020

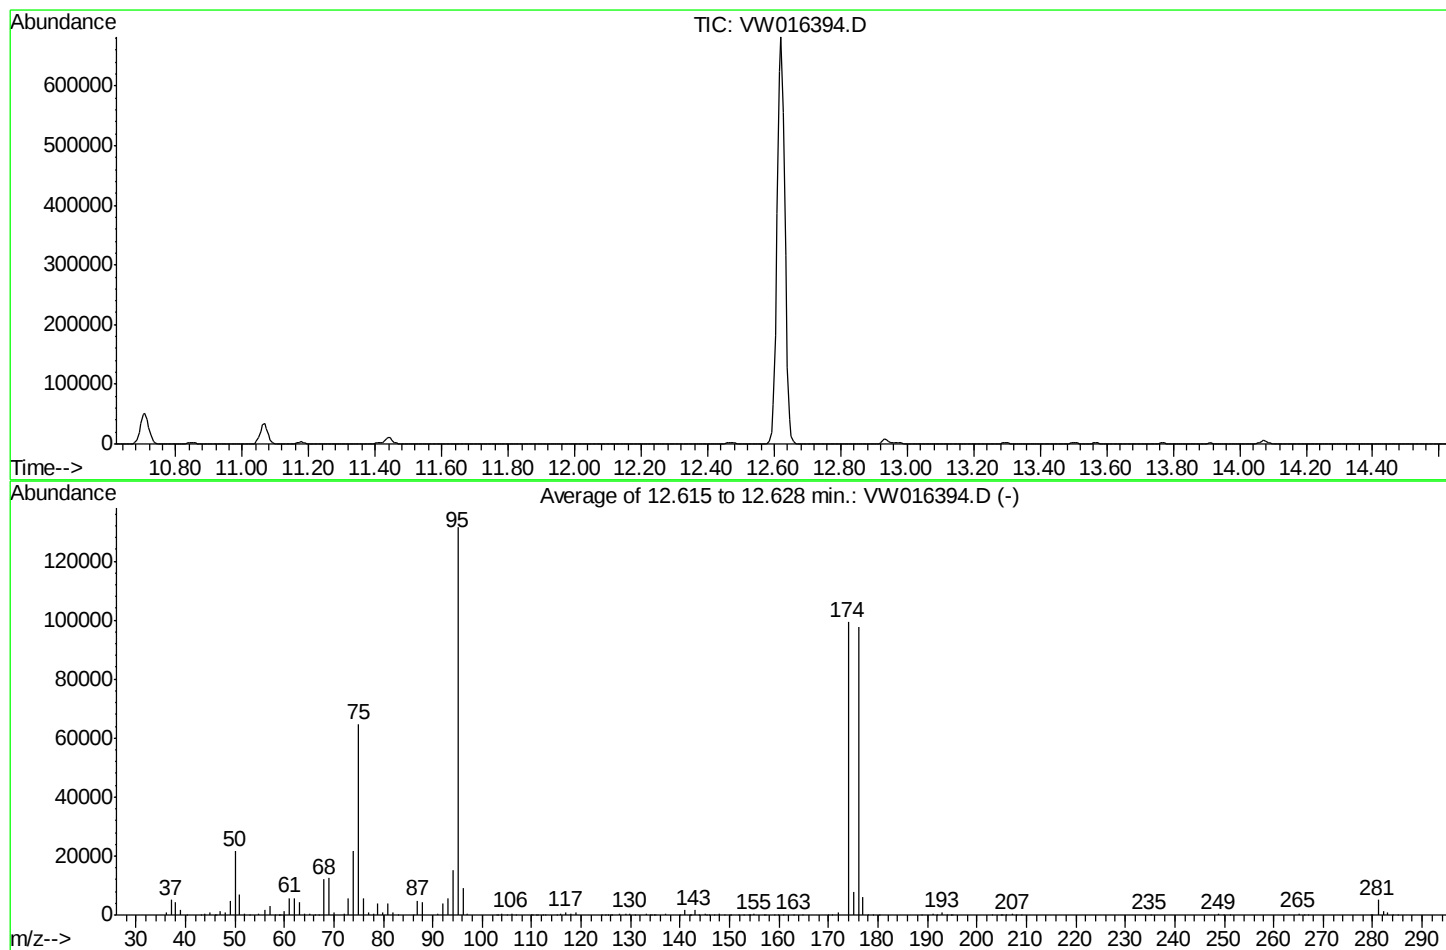

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	21594	PASS
75	95	30	60	49.1	64514	PASS
95	95	100	100	100.0	131442	PASS
96	95	5	9	6.8	8993	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.5	99205	PASS
175	174	5	9	7.9	7850	PASS
176	174	95	101	98.4	97653	PASS
177	176	5	9	6.4	6253	PASS