


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082918\
 Data File : VW004996.D
 Acq On : 29 Aug 2018 11:12
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082918S.M
 Title : SW846 8260
 Last Update : Thu Aug 30 01:51:13 2018

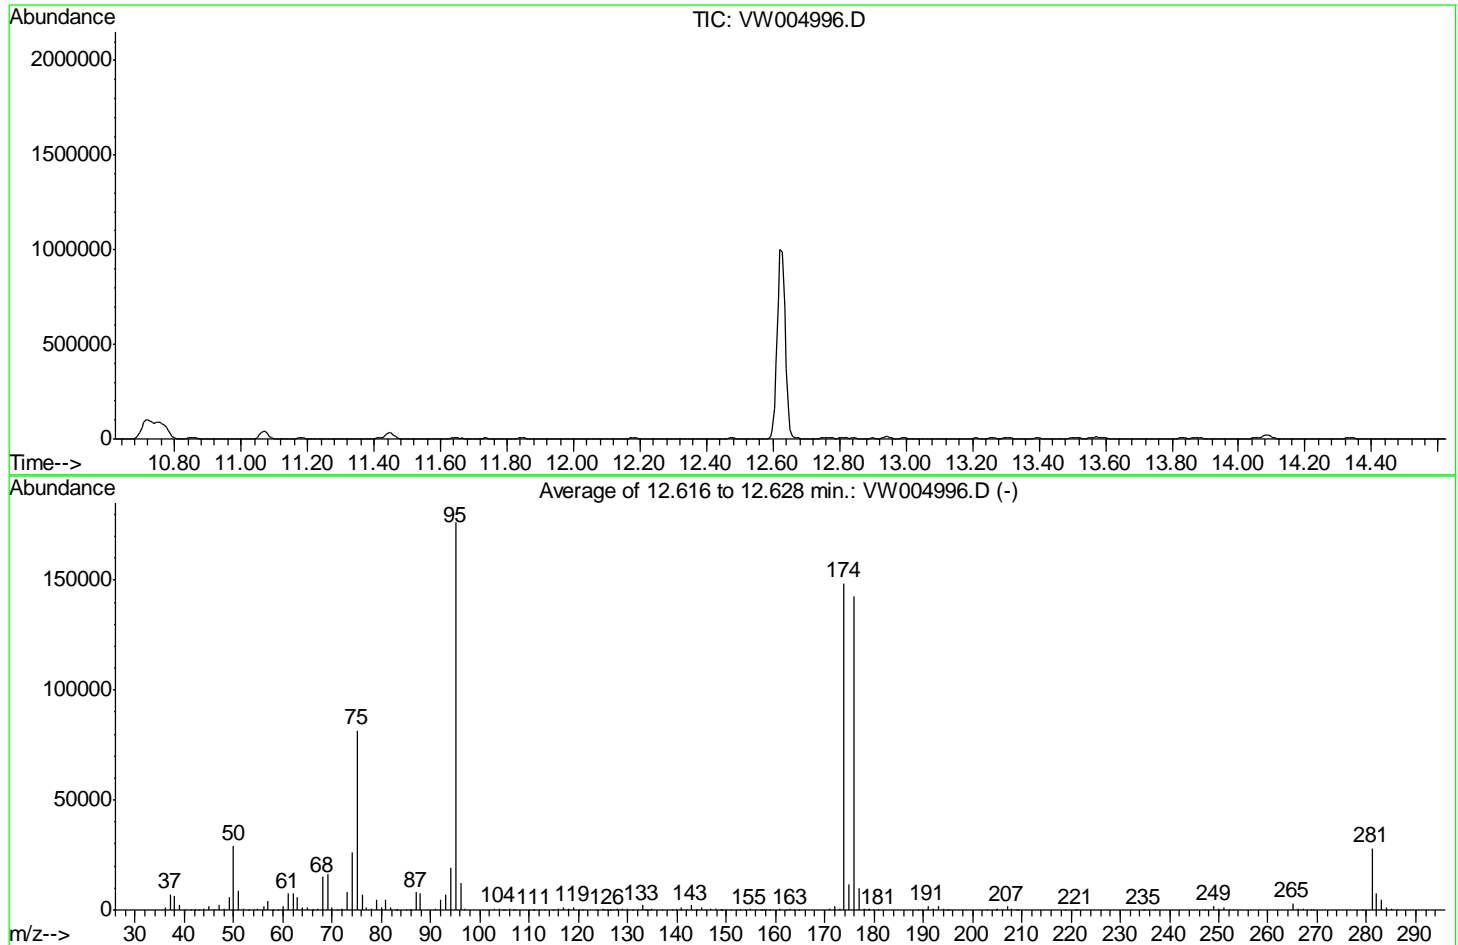

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	29314	PASS
75	95	30	60	46.4	81778	PASS
95	95	100	100	100.0	176298	PASS
96	95	5	9	7.0	12290	PASS
173	174	0.00	2	0.4	540	PASS
174	95	50	100	84.2	148501	PASS
175	174	5	9	8.0	11928	PASS
176	174	95	101	96.0	142586	PASS
177	176	5	9	7.0	9919	PASS