




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082923\
 Data File : VW026948.D
 Acq On : 29 Aug 2023 14:11
 Operator : SY/MD
 Sample : 04175-19
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2023
 Supervised By :Mahesh Dadoda 09/01/2023

Quant Time: Aug 29 20:49:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 29 20:47:20 2023
 Response via : Initial Calibration

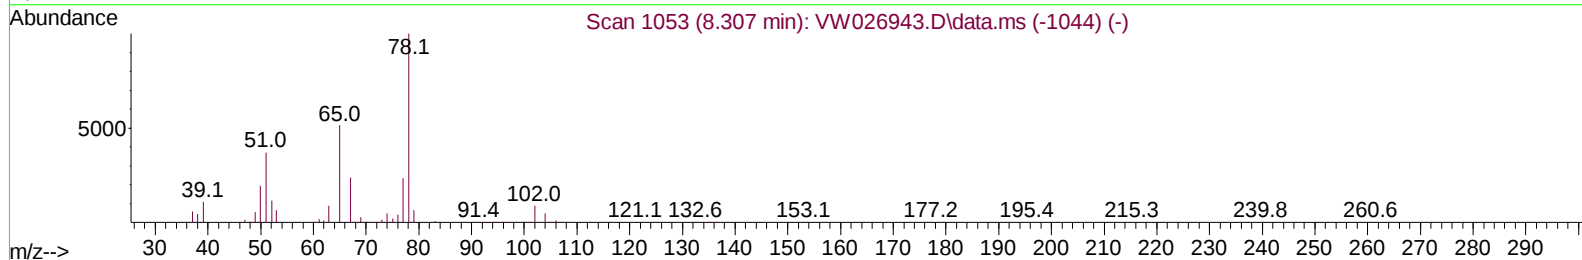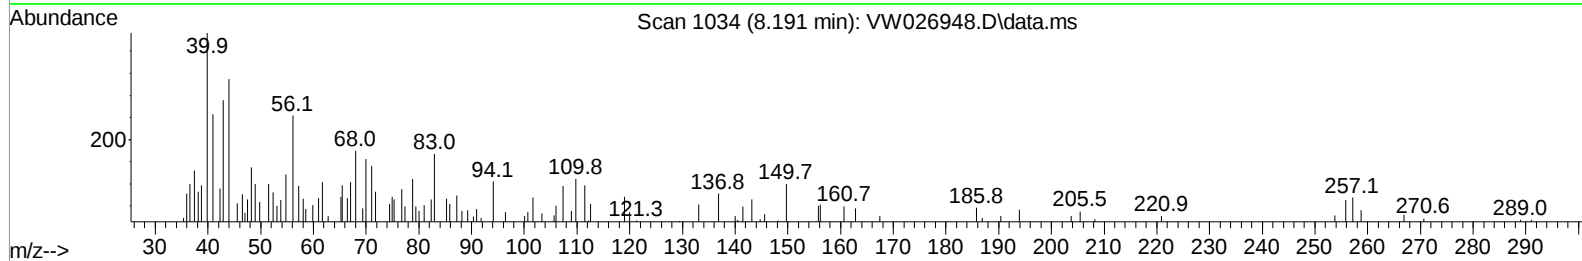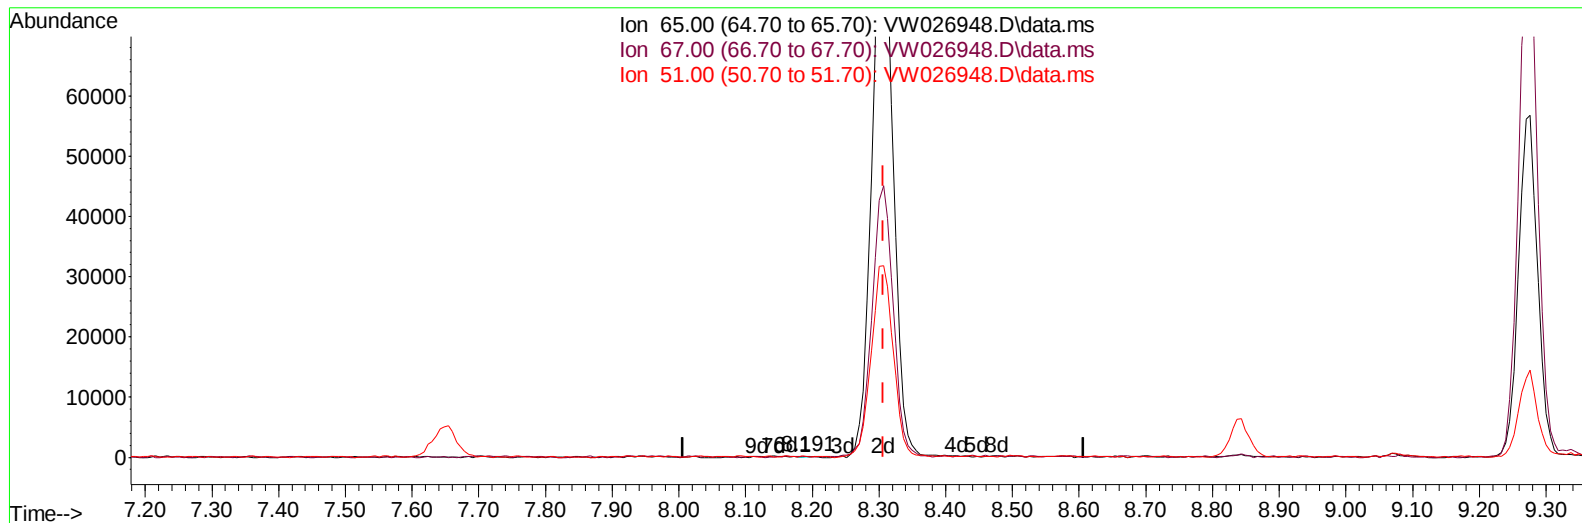

TIC: VW026948.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.191min (-0.116) 0.01 ug/L

response 82

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	46.34
51.00	112.90	102.44
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082923\
 Data File : VW026948.D
 Acq On : 29 Aug 2023 14:11
 Operator : SY/MD
 Sample : 04175-19
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2023
 Supervised By :Mahesh Dadoda 09/01/2023

Quant Time: Aug 29 20:49:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 29 20:47:20 2023
 Response via : Initial Calibration

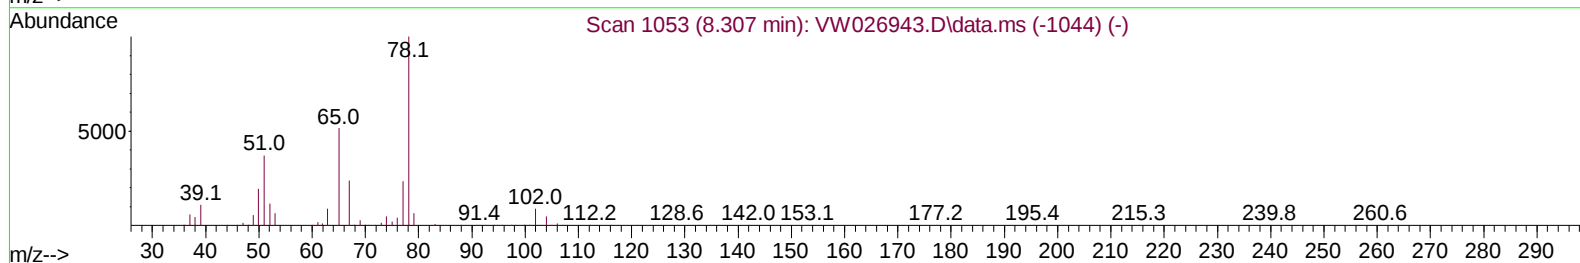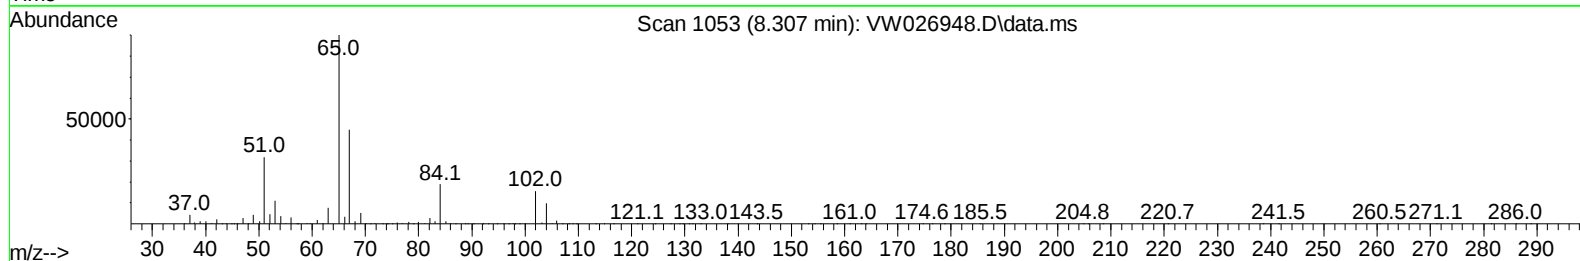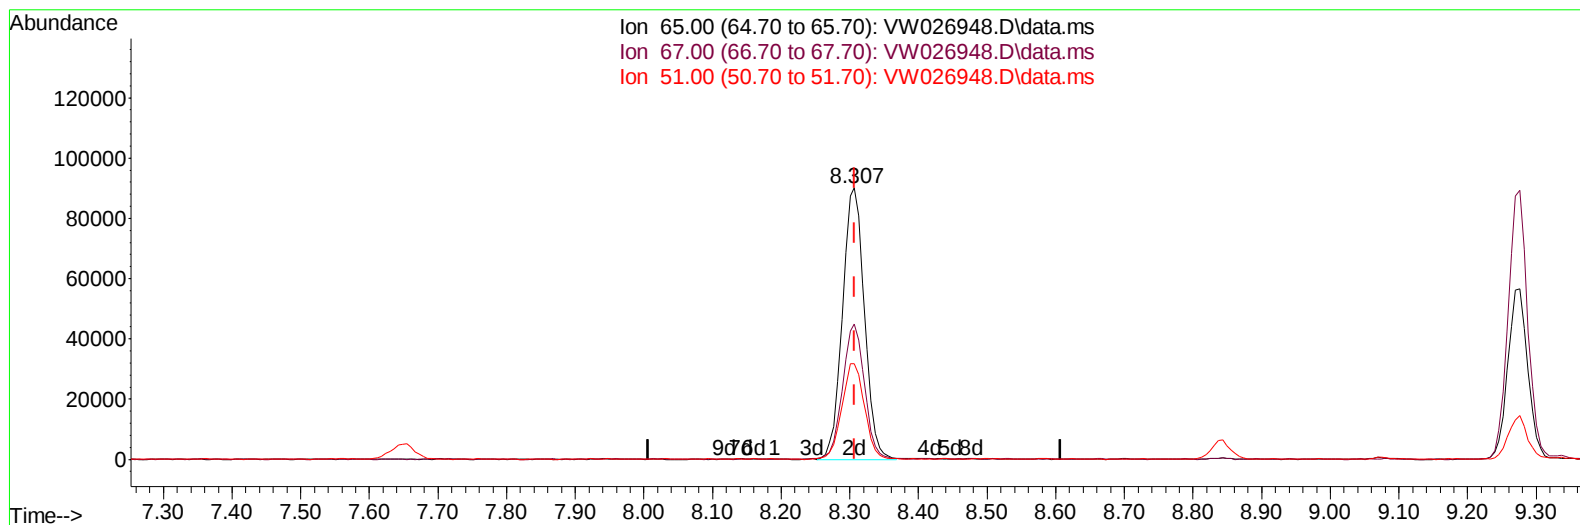

TIC: VW026948.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (0.000) 23.75 ug/L m

response 200893

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	0.02#
51.00	112.90	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082923\
 Data File : VW026948.D
 Acq On : 29 Aug 2023 14:11
 Operator : SY/MD
 Sample : 04175-19
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYD2

Manual IntegrationsAPPROVED

Quant Time: Aug 29 20:49:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 29 20:47:20 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2023
 Supervised By :Mahesh Dadoda 09/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	456596	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	376210	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	138462	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	77533	10.330	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	41.320%	
7) Chloroethane-d5	2.893	69	75324	13.496	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	54.000%	
11) 1,1-Dichloroethene-d2	4.021	65	45746	12.392	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	49.560%	
21) 2-Butanone-d5	7.075	46	114026	52.855	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	105.700%	
24) Chloroform-d	7.648	84	270779	17.670	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	70.680%	
26) 1,2-Dichloroethane-d4	8.307	65	200893m	23.755	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	95.000%	
32) Benzene-d6	8.276	84	498716	19.235	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	76.920%	
36) 1,2-Dichloropropane-d6	9.276	67	173971	21.541	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	86.160%	
41) Toluene-d8	10.318	98	400316	17.986	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	71.960%	
43) trans-1,3-Dichloroprop...	10.575	79	69830	20.941	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.760%	
47) 2-Hexanone-d5	10.922	63	56006	65.995	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	132.000%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	123842	19.417	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	77.680%	
66) 1,2-Dichlorobenzene-d4	13.848	152	100219	20.222	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	80.880%	
Target Compounds						
					Qvalue	
13) Acetone	4.124	43	9762	4.551	ug/L	86
14) Carbon disulfide	4.393	76	20718	0.853	ug/L	100
25) Chloroform	7.679	83	30110	2.011	ug/L	96
35) Methylcyclohexane	9.331	83	13399	1.122	ug/L #	79
53) m,p-Xylene	11.830	106	11632	1.010	ug/L	97
54) o-Xylene	12.166	106	6869	0.639	ug/L	85
63) 1,2,4-Trimethylbenzene	13.251	105	17459	1.095	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082923\
Data File : VW026948.D
Acq On : 29 Aug 2023 14:11
Operator : SY/MD
Sample : 04175-19
Misc : 4.72g/10mL/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2023
Supervised By :Mahesh Dadoda 09/01/2023

Quant Time: Aug 29 20:49:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 29 20:47:20 2023
Response via : Initial Calibration

