


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW083019\
Data File : VW012341.D
Acq On : 30 Aug 2019 08:56
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
Title : SW846 8260
Last Update : Mon Aug 26 07:18:31 2019

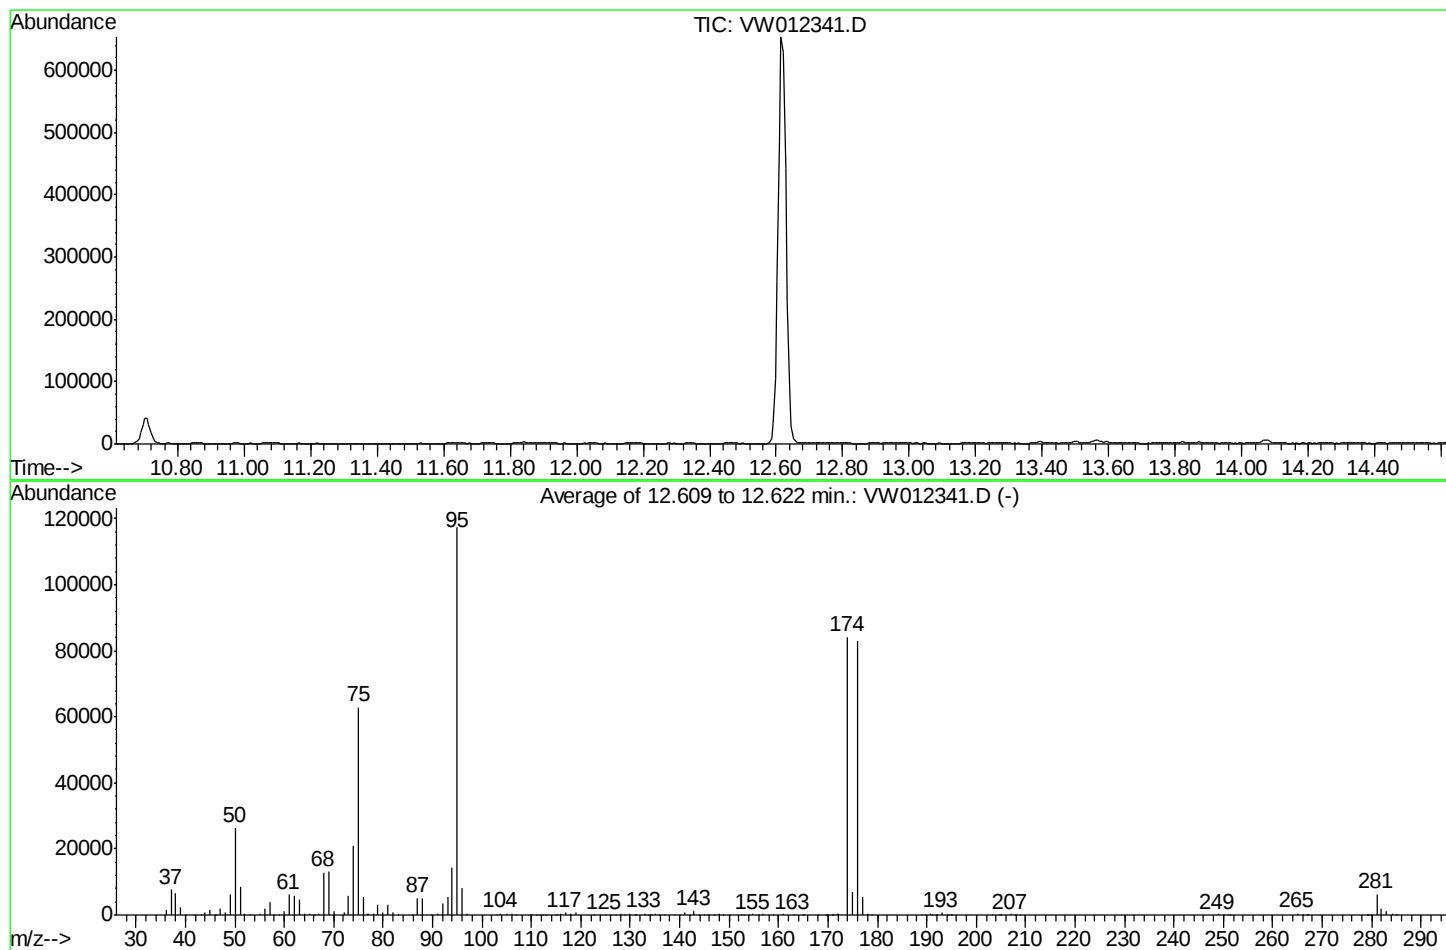

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	26360	PASS
75	95	30	60	53.7	62970	PASS
95	95	100	100	100.0	117344	PASS
96	95	5	9	7.1	8291	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.7	84173	PASS
175	174	5	9	8.4	7066	PASS
176	174	95	101	98.6	82954	PASS
177	176	5	9	6.6	5505	PASS