


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW083019\
Data File : VW012363.D
Acq On : 30 Aug 2019 21:18
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
Title : SW846 8260
Last Update : Mon Aug 26 07:18:31 2019

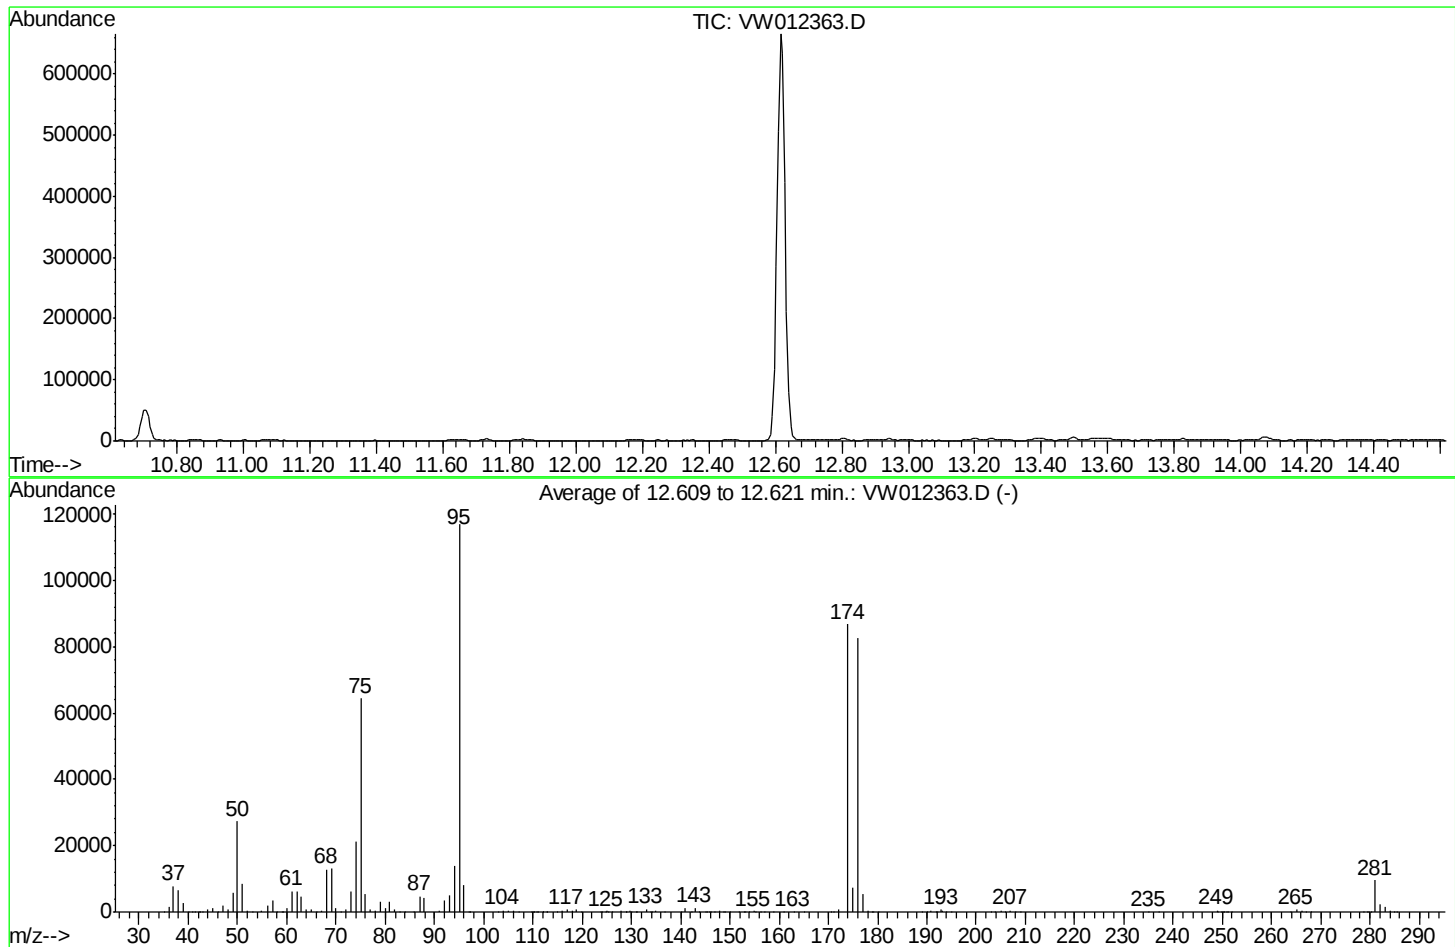

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	27384	PASS
75	95	30	60	55.1	64357	PASS
95	95	100	100	100.0	116866	PASS
96	95	5	9	6.8	7960	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.2	86690	PASS
175	174	5	9	8.4	7311	PASS
176	174	95	101	95.1	82469	PASS
177	176	5	9	6.7	5519	PASS