

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083021\
 Data File : VW019943.D
 Acq On : 30 Aug 2021 17:22
 Operator : SY/VA
 Sample : VIBLK423
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK423

Manual Integrations
 APPROVED

MMDadoda
 9/1/2021 6:40:27 PM

Quant Time: Aug 31 01:05:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 31 01:00:58 2021
 Response via : Initial Calibration

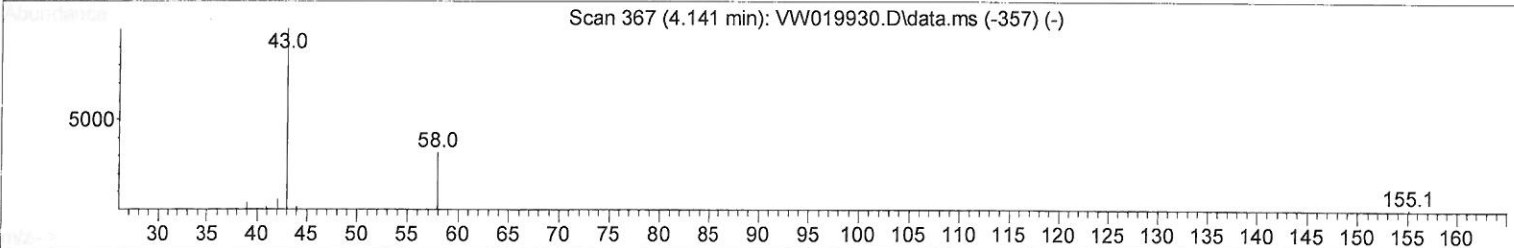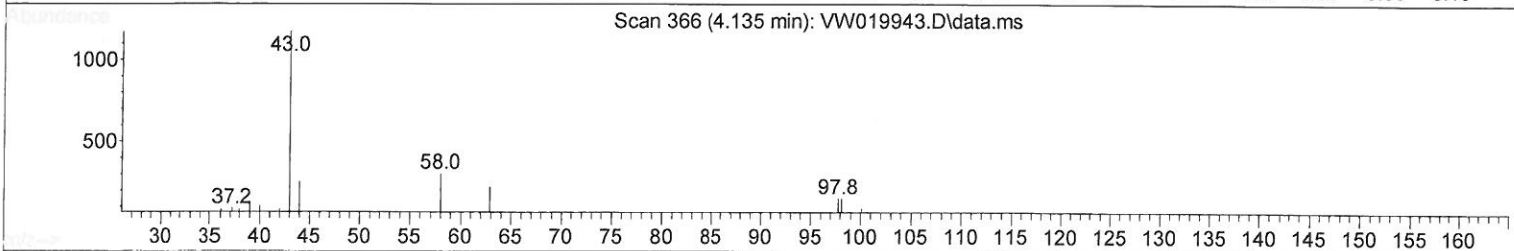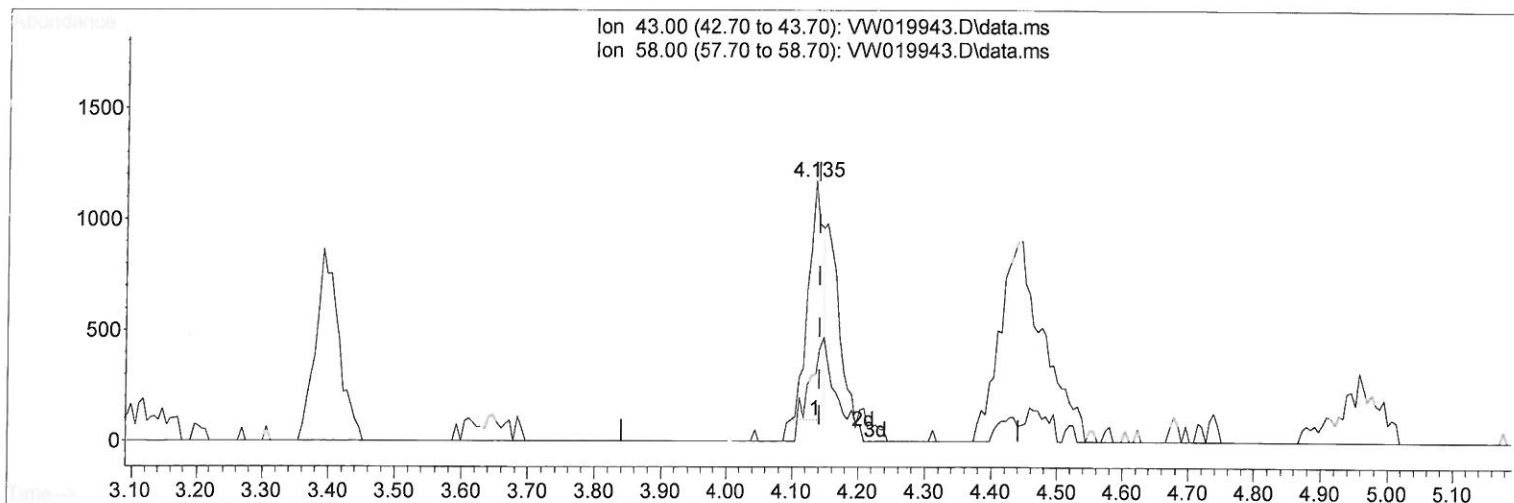

TIC: VW019943.D\data.ms

(13) Acetone (T)

4.135min (-0.006) 2.07 ug/L

response 1687

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	70.66#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083021\
 Data File : VW019943.D
 Acq On : 30 Aug 2021 17:22
 Operator : SY/VA
 Sample : VIBLK423
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK423

Manual Integrations
 APPROVED

MMDadoda
 9/1/2021 6:40:27 PM

Quant Time: Aug 31 01:05:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 31 01:00:58 2021
 Response via : Initial Calibration

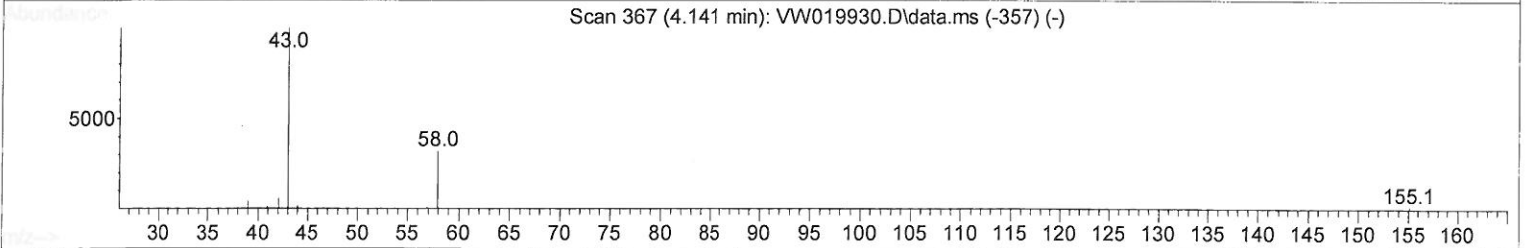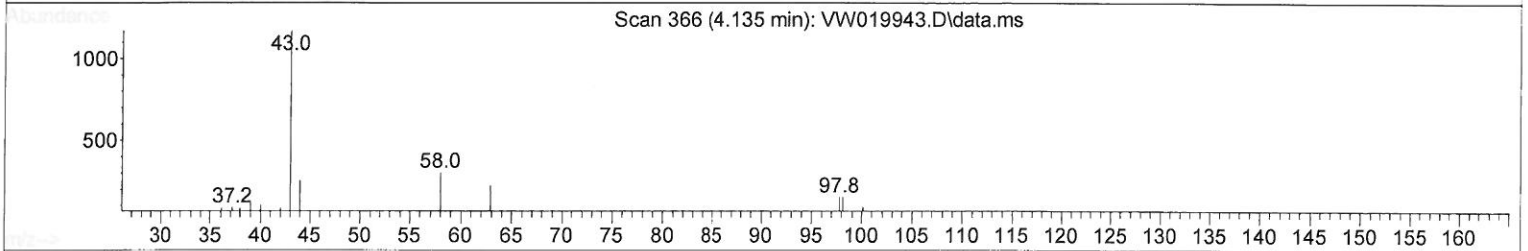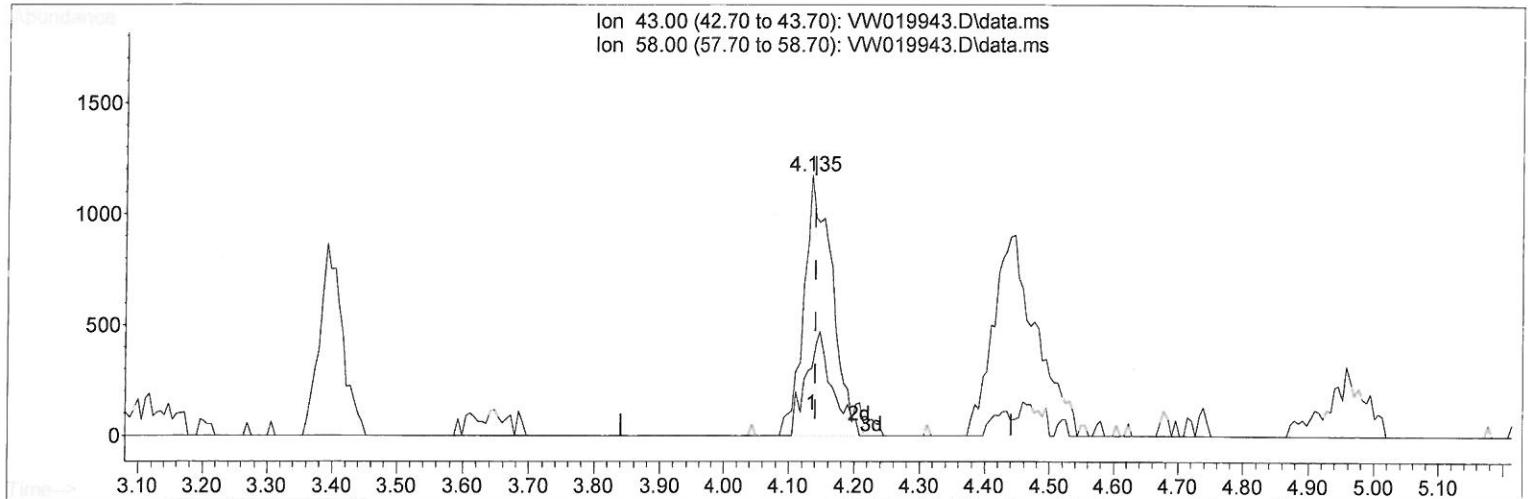

TIC: VW019943.D\data.ms

(13) Acetone (T)

4.135min (-0.006) 4.40 ug/L m

response 3589

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	33.21
0.00	0.00	0.00
0.00	0.00	0.00

508/02/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083021\
 Data File : VW019943.D
 Acq On : 30 Aug 2021 17:22
 Operator : SY/VA
 Sample : VIBLK423
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK423

Manual Integrations
 APPROVED

MMDadoda
 9/1/2021 6:40:27 PM

Quant Time: Aug 31 01:05:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 31 01:00:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	303928	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	297694	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	132837	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	106532	22.623	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.480%		
7) Chloroethane-d5	2.897	69	95566	23.121	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.480%		
11) 1,1-Dichloroethene-d2	4.025	63	127425	15.594	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.360%		
21) 2-Butanone-d5	7.086	46	51398	53.735	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	107.460%		
24) Chloroform-d	7.653	84	202707	24.252	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	97.000%		
26) 1,2-Dichloroethane-d4	8.311	65	113871	25.280	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	101.120%		
32) Benzene-d6	8.281	84	399511	23.537	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.160%		
36) 1,2-Dichloropropane-d6	9.280	67	123053	23.940	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.760%		
41) Toluene-d8	10.329	98	348148	22.382	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.520%		
43) trans-1,3-Dichloroprop...	10.579	79	48341	22.765	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.040%		
47) 2-Hexanone-d5	10.926	63	34881	48.712	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.420%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	108245	25.874	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.480%		
66) 1,2-Dichlorobenzene-d4	13.853	152	123510	27.106	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	108.440%		
Target Compounds						
13) Acetone	4.135	43	3589m	4.395	ug/L	Qvalue 99/02/21 Sy
16) Methylene chloride	4.921	84	16232	3.112	ug/L	95
46) Tetrachloroethene	10.859	164	3721	1.034	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083021\
Data File : VW019943.D
Acq On : 30 Aug 2021 17:22
Operator : SY/VA
Sample : VIBLK423
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK423

Manual Integrations
APPROVED

MMDadoda
9/1/2021 6:40:27 PM

Quant Time: Aug 31 01:05:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 31 01:00:58 2021
Response via : Initial Calibration

