

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083021\
 Data File : VW019934.D
 Acq On : 30 Aug 2021 13:09
 Operator : SY/VA
 Sample : M3579-01
 Misc : 6.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 GB6A3

Manual Integrations
 APPROVED

MMDadoda
 9/1/2021 6:40:10 PM

Quant Time: Aug 31 01:03:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 31 01:00:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	434085	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	403136	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	180208	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	136398	20.280	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.120%
7) Chloroethane-d5	2.898	69	130070	22.033	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.120%
11) 1,1-Dichloroethene-d2	4.026	63	163557m	14.014	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.040%
21) 2-Butanone-d5	7.086	46	57857	42.351	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.700%
24) Chloroform-d	7.653	84	245688	20.580	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.320%
26) 1,2-Dichloroethane-d4	8.311	65	138700	21.559	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.240%
32) Benzene-d6	8.281	84	493592	21.474	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.880%
36) 1,2-Dichloropropane-d6	9.275	67	152101	21.851	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.400%
41) Toluene-d8	10.323	98	446227	21.184	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.720%
43) trans-1,3-Dichloroprop...	10.579	79	63269	22.002	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.000%
47) 2-Hexanone-d5	10.927	63	46806	48.269	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.540%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	126774	22.377	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	140855	22.786	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.160%
Target Compounds						Qvalue
13) Acetone	4.160	43	6341m	5.437	ug/L	
16) Methylene chloride	4.928	84	12347	1.657	ug/L	95
34) Trichloroethene	9.092	95	3559	0.553	ug/L	95
42) Toluene	10.390	91	9568	0.365	ug/L	90
46) Tetrachloroethene	10.866	164	201108	41.276	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083021\
Data File : VW019934.D
Acq On : 30 Aug 2021 13:09
Operator : SY/VA
Sample : M3579-01
Misc : 6.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GB6A3

Manual Integrations
APPROVED

MMDadoda
9/1/2021 6:40:10 PM

Quant Time: Aug 31 01:03:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 31 01:00:58 2021
Response via : Initial Calibration

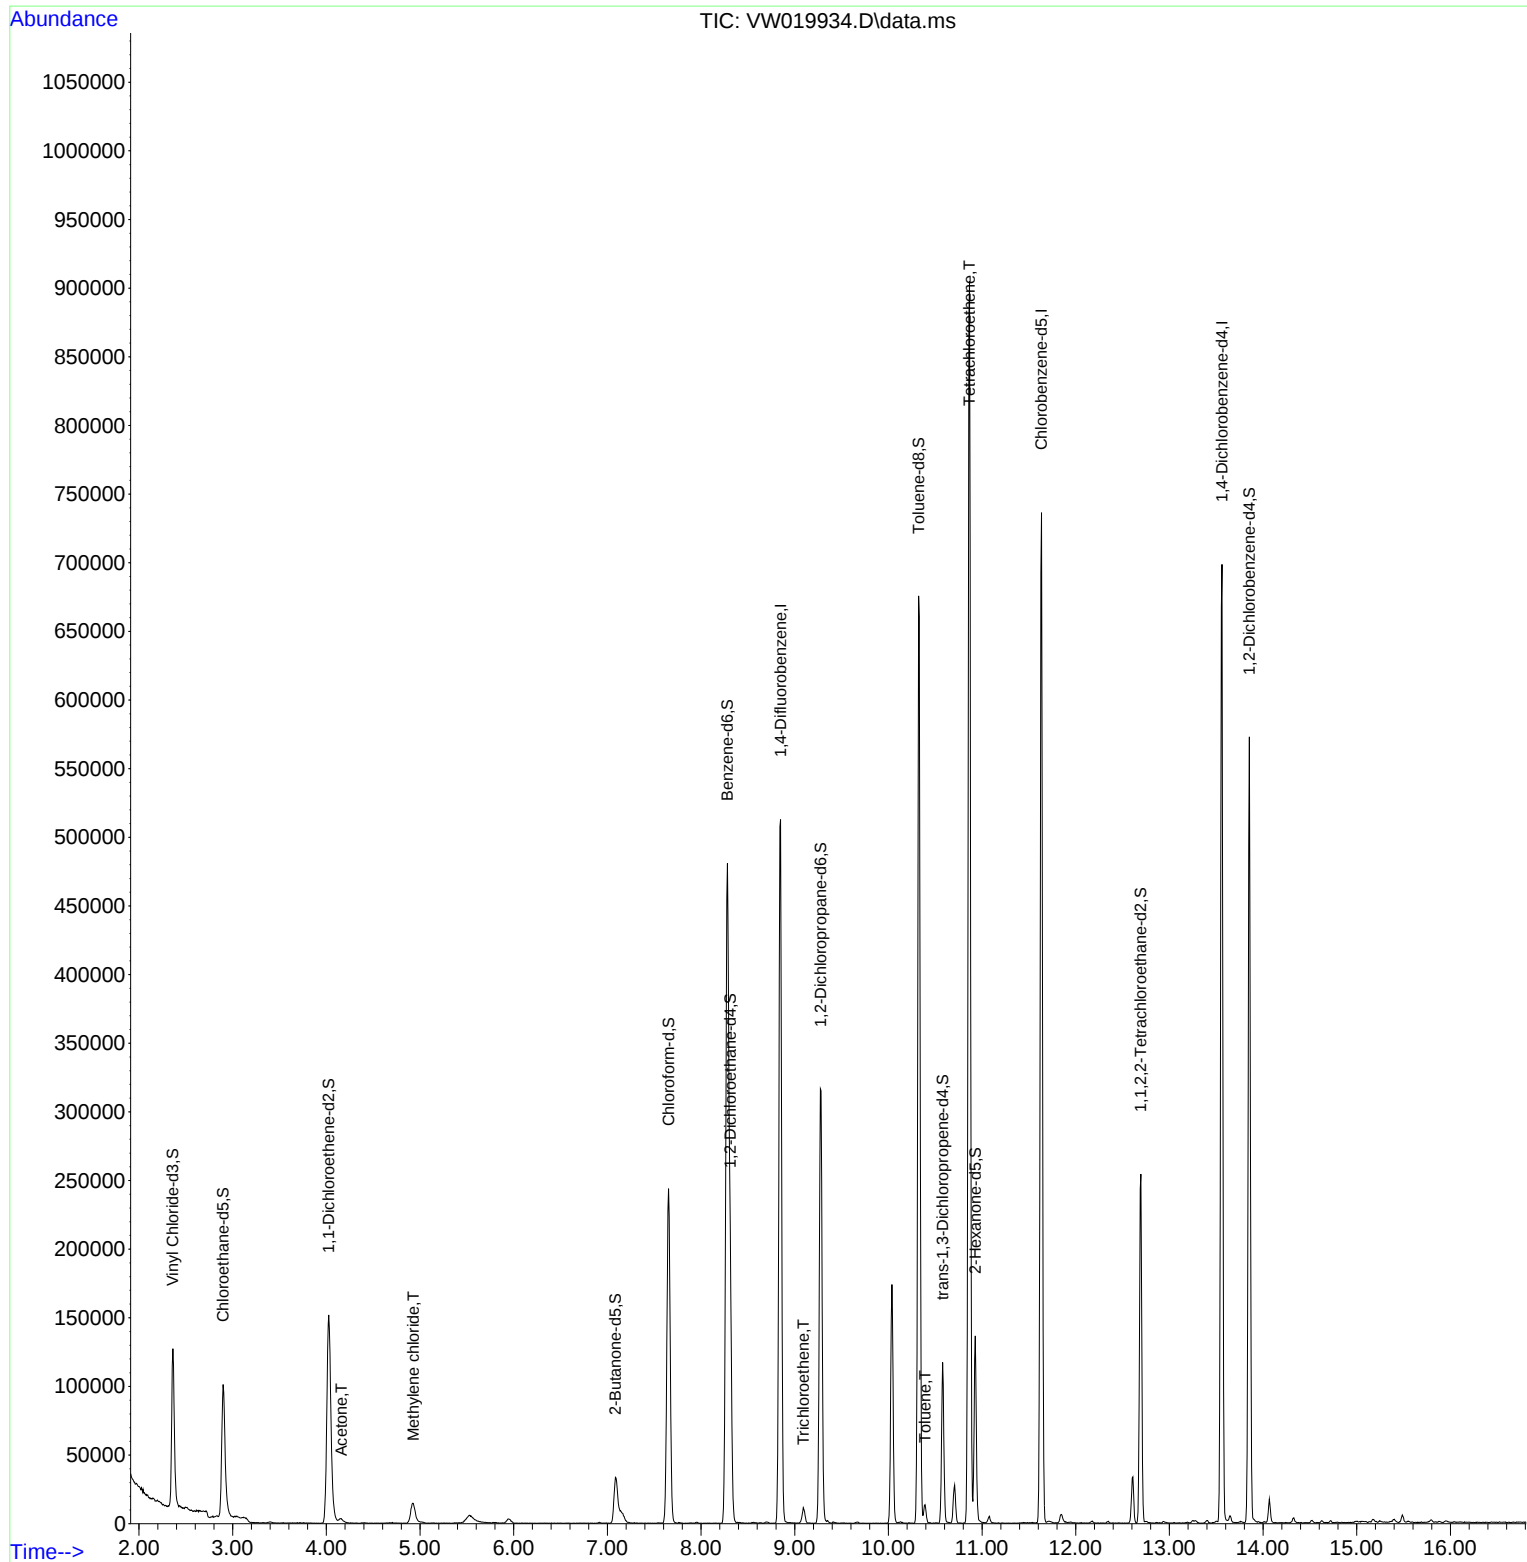

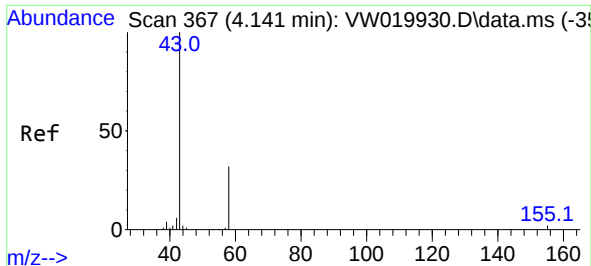





#13
Acetone
Concen: 5.437 ug/L m
RT: 4.160 min Scan# 370
Delta R.T. 0.019 min
Lab File: VW019934.D
Acq: 30 Aug 2021 13:09

Tgt Ion: 43 Resp: 6341
Ion Ratio Lower Upper
43 100
58 27.6 0.0 53.8

Instrument :
MSVOA_W
ClientSampled :
GB6A3




Manual Integrations
APPROVED


MMDadoda
9/1/2021 6:40:10 PM

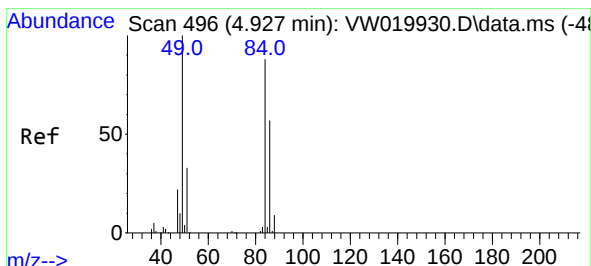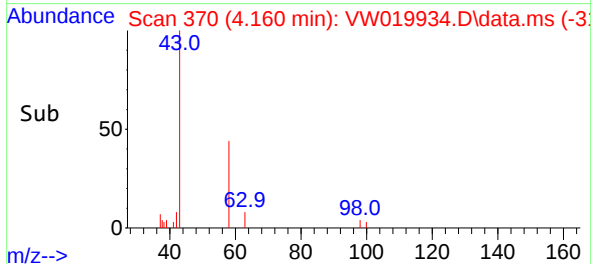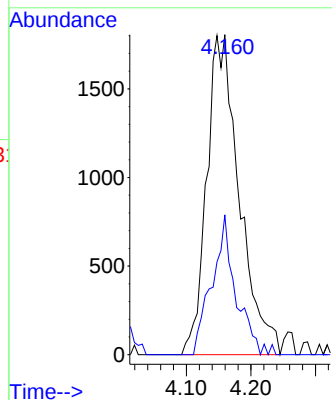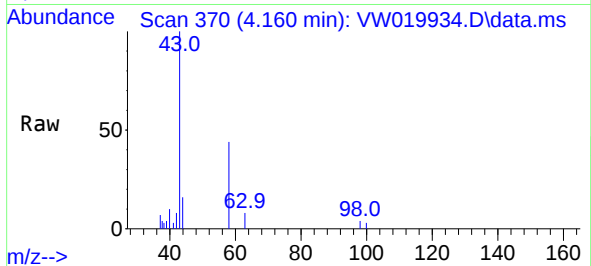

#16
Methylene chloride
Concen: 1.657 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.000 min
Lab File: VW019934.D
Acq: 30 Aug 2021 13:09

Tgt Ion: 84 Resp: 12347
Ion Ratio Lower Upper
84 100
86 60.7 45.3 84.1
49 118.5 86.6 160.8

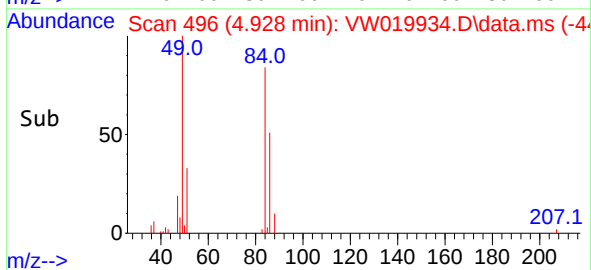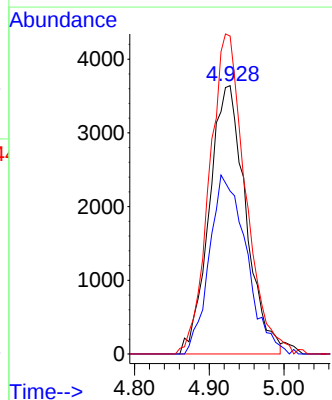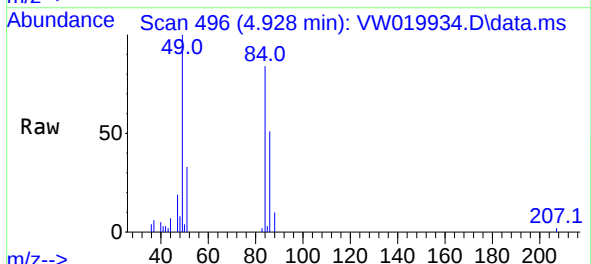

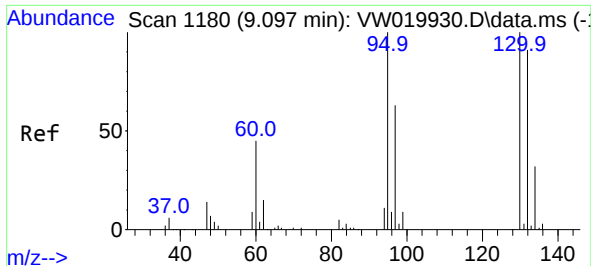

#34
Trichloroethene
Concen: 0.553 ug/L
RT: 9.092 min Scan# 1179
Delta R.T. -0.006 min
Lab File: VW019934.D
Acq: 30 Aug 2021 13:09





Tgt Ion: 95 Resp: 3559

Ion	Ratio	Lower	Upper
95	100		
97	71.1	47.3	87.8
132	102.5	71.0	131.8
130	82.8	65.1	120.9

Instrument :
MSVOA_W
ClientSampled :
GB6A3

Manual Integrations
APPROVED




MMDadoda
9/1/2021 6:40:10 PM

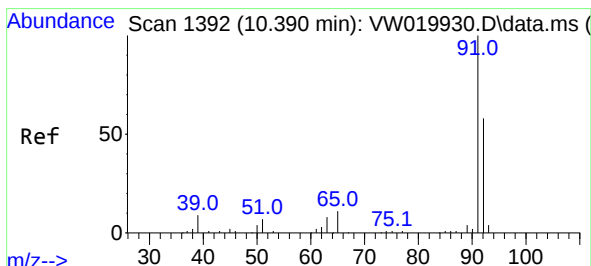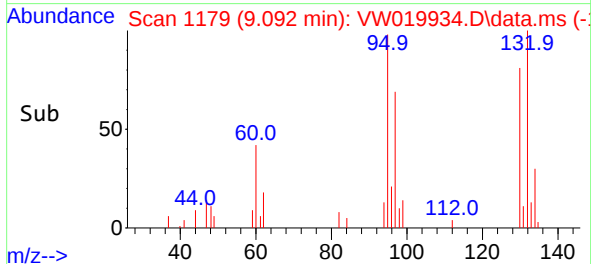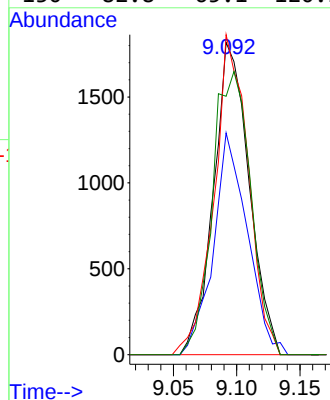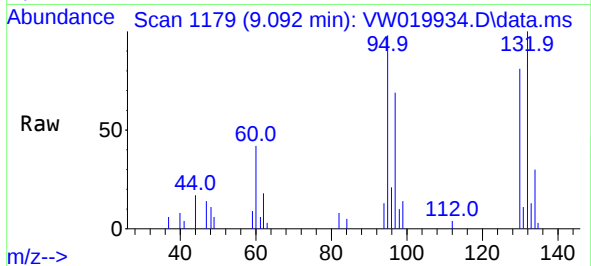


#42
Toluene
Concen: 0.365 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.000 min
Lab File: VW019934.D
Acq: 30 Aug 2021 13:09


Tgt Ion: 91 Resp: 9568

Ion	Ratio	Lower	Upper
91	100		
92	63.5	39.5	73.3

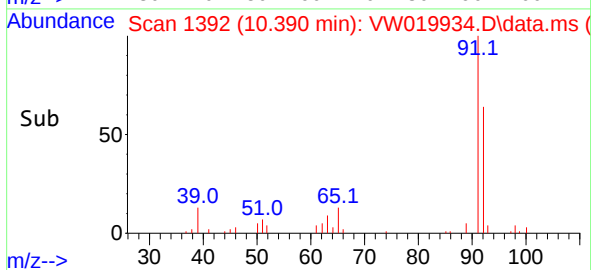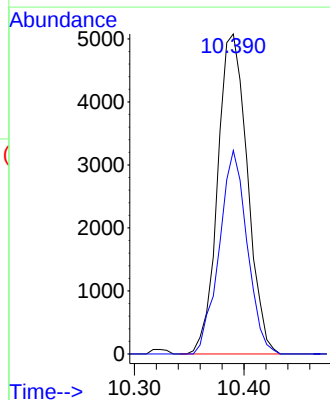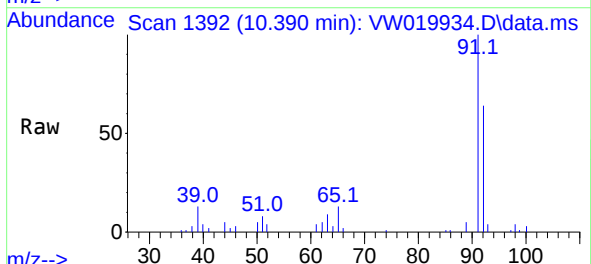


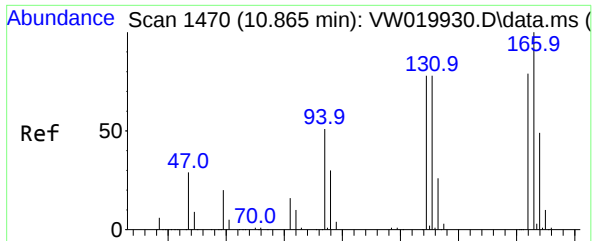


#46
Tetrachloroethene
Concen: 41.276 ug/L
RT: 10.866 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VW019934.D
Acq: 30 Aug 2021 13:09

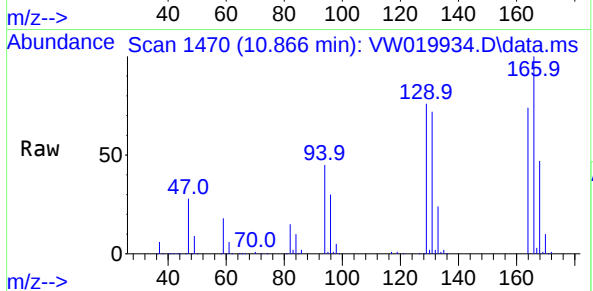

Tgt Ion:164 Resp: 201108

Ion	Ratio	Lower	Upper
164	100		
129	102.4	66.7	123.9
131	97.7	61.1	113.5
166	135.1	87.0	161.6

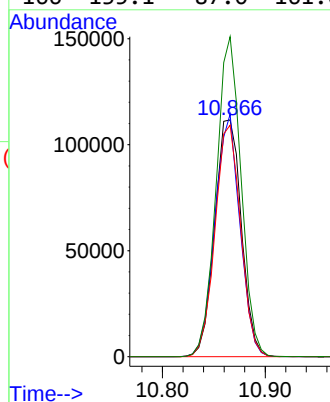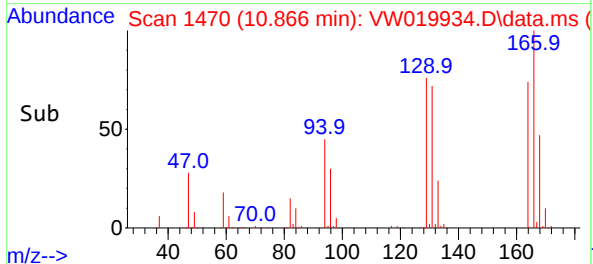

Instrument :
MSVOA_W
ClientSampleId :
GB6A3

Manual Integrations
APPROVED

MMDadoda
9/1/2021 6:40:10 PM