




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083023\
 Data File : VW026963.D
 Acq On : 30 Aug 2023 14:14
 Operator : SY/MD
 Sample : 04235-01
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYD8

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:30:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 31 01:29:13 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 09/01/2023

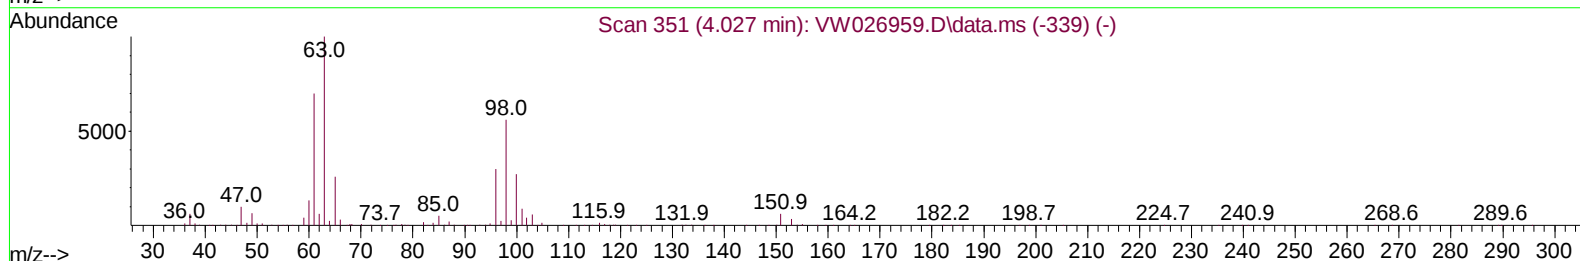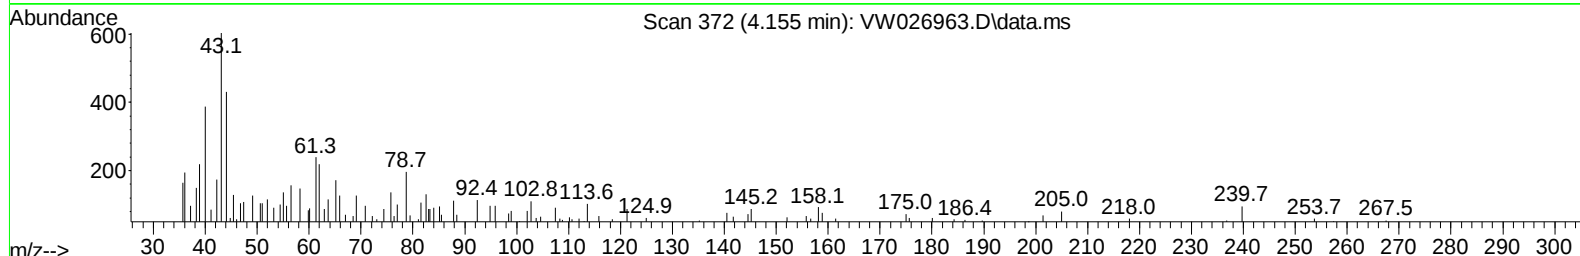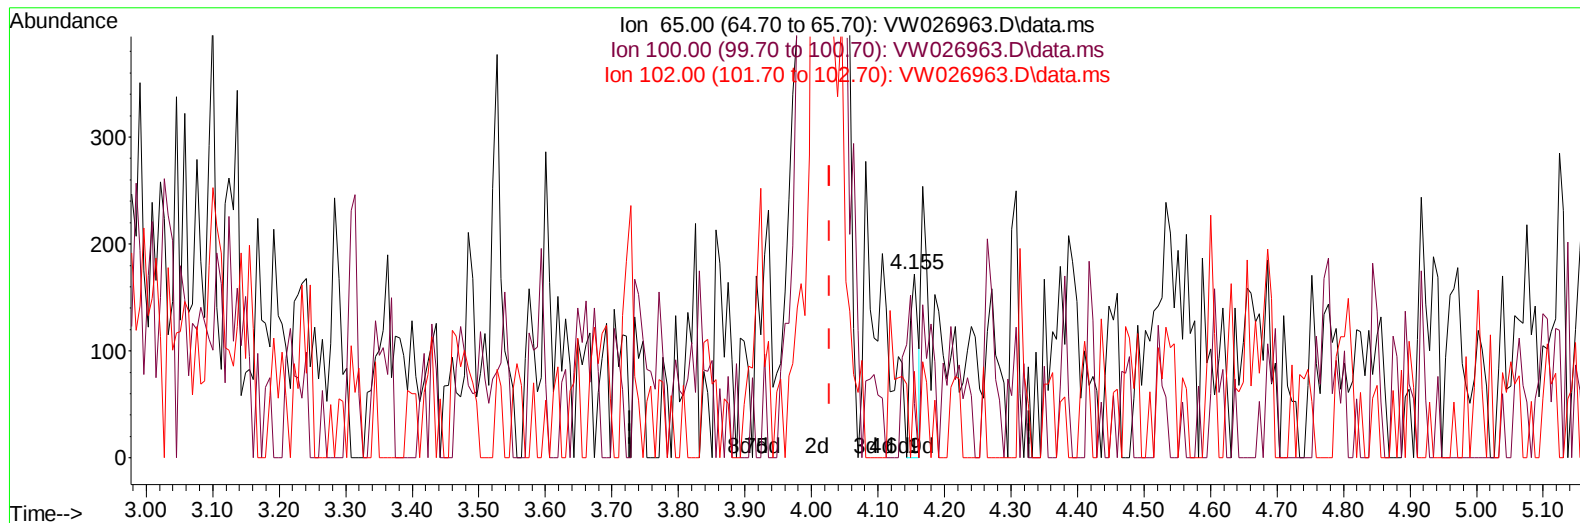

TIC: VW026963.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.155min (+ 0.128) 0.26 ug/L

response 147

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	124.90	100.00
102.00	16.90	20.41
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083023\
 Data File : VW026963.D
 Acq On : 30 Aug 2023 14:14
 Operator : SY/MD
 Sample : 04235-01
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYD8

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:30:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 31 01:29:13 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 09/01/2023

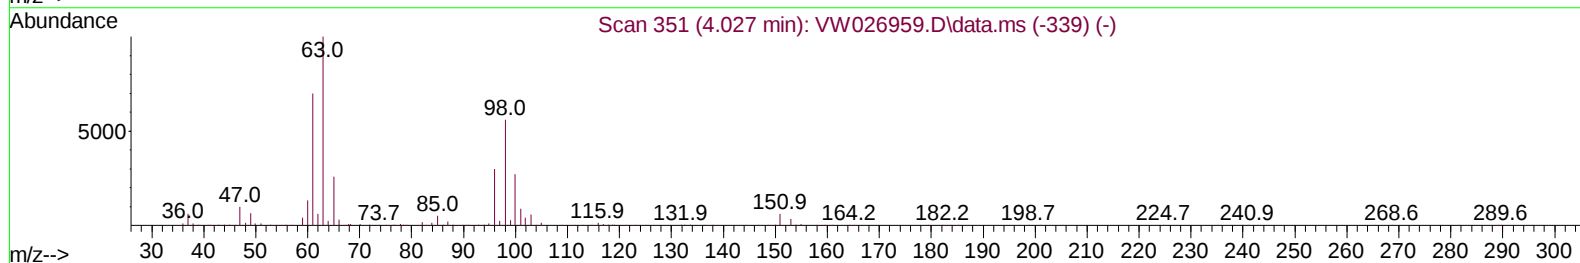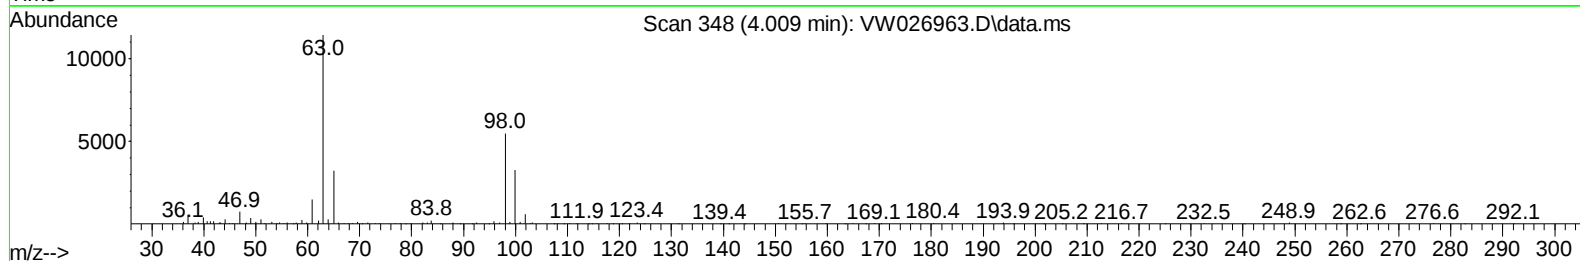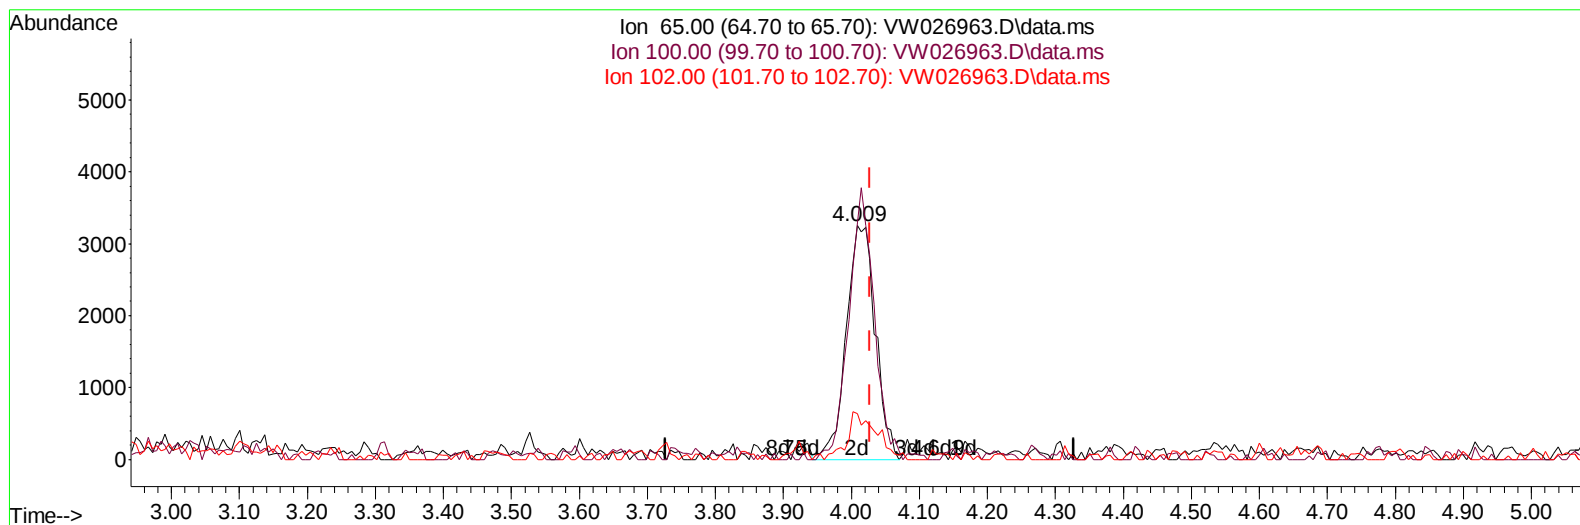

TIC: VW026963.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.009min (-0.018) 17.29 ug/L m

response 9648

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	124.90	1.52#
102.00	16.90	0.31#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083023\
 Data File : VW026963.D
 Acq On : 30 Aug 2023 14:14
 Operator : SY/MD
 Sample : 04235-01
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYD8

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:30:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 31 01:29:13 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 09/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	69022	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	55122	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	14567	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	15977	14.081	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.320%	
7) Chloroethane-d5	2.887	69	15702	18.610	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.440%	
11) 1,1-Dichloroethene-d2	4.009	65	9648m	17.289	ug/L	-0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	69.160%	
21) 2-Butanone-d5	7.087	46	15554	47.694	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.380%	
24) Chloroform-d	7.654	84	56803	24.520	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.080%	
26) 1,2-Dichloroethane-d4	8.307	65	36357	28.439	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	113.760%	
32) Benzene-d6	8.276	84	86985	22.897	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	9.276	67	32216	27.224	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	108.880%	
41) Toluene-d8	10.325	98	61826	18.959	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.840%	
43) trans-1,3-Dichloroprop...	10.581	79	9512	19.469	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.880%	
47) 2-Hexanone-d5	10.928	63	6195	49.822	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	99.640%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	27974	29.934	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	119.720%	
66) 1,2-Dichlorobenzene-d4	13.855	152	14395	27.609	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	110.440%	
Target Compounds						
					Qvalue	
13) Acetone	4.125	43	2211	6.819	ug/L	79
16) Methylene chloride	4.911	84	5195	3.891	ug/L	90
34) Trichloroethene	9.087	95	1468m	1.436	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083023\
Data File : VW026963.D
Acq On : 30 Aug 2023 14:14
Operator : SY/MD
Sample : 04235-01
Misc : 6.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYD8

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:30:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 31 01:29:13 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 09/01/2023

